


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
Data File : BN014684.D
Acq On : 20 May 2021 17:22
Operator : CG/JU
Sample : M2465-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARK2

Manual Integrations
APPROVED

mohammad
5/21/2021 3:22:23 PM

Quant Time: May 20 17:57:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 20 16:48:16 2021
Response via : Initial Calibration

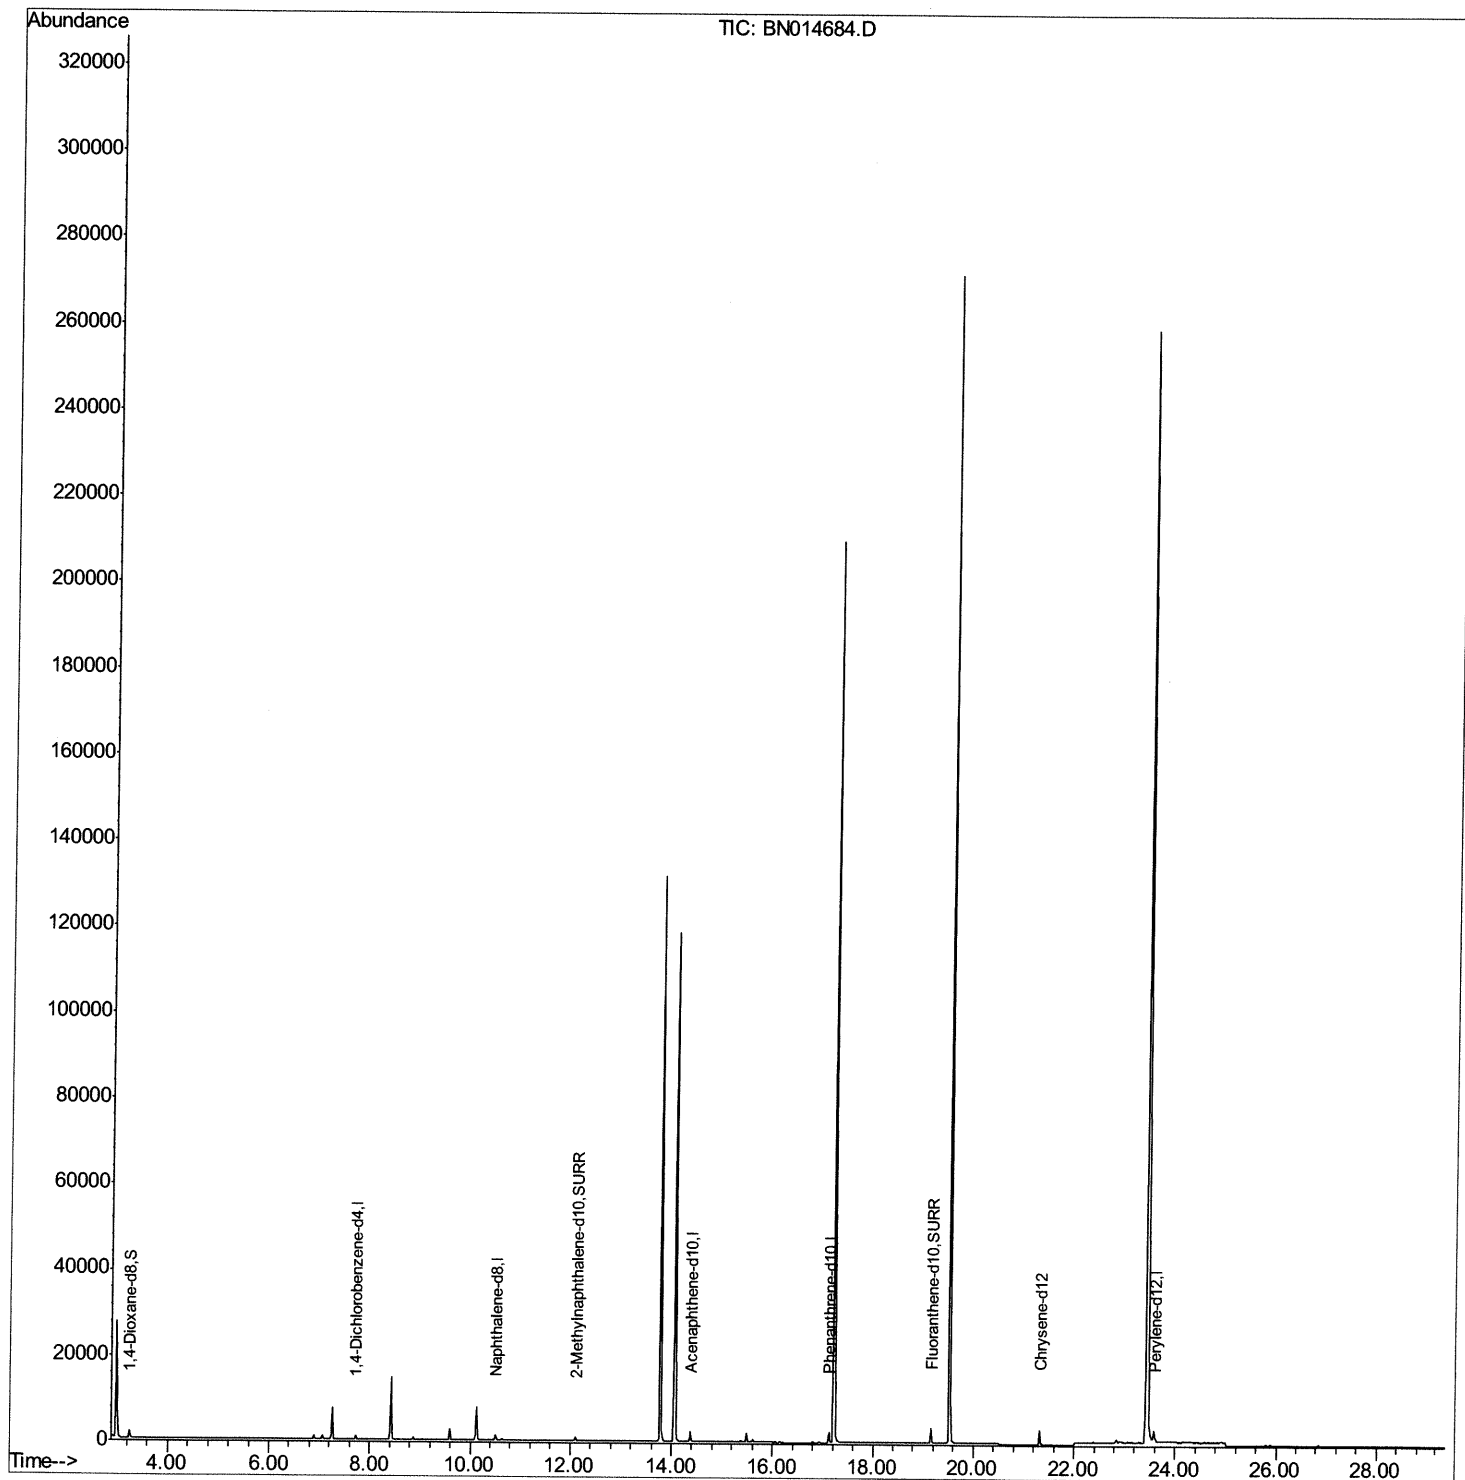

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
Data File : BN014684.D
Acq On : 20 May 2021 17:22
Operator : CG/JU
Sample : M2465-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YARK2

Manual Integrations
APPROVED

mohammad
5/21/2021 3:22:23 PM

Quant Time: May 20 17:56:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 20 16:48:16 2021
Response via : Initial Calibration

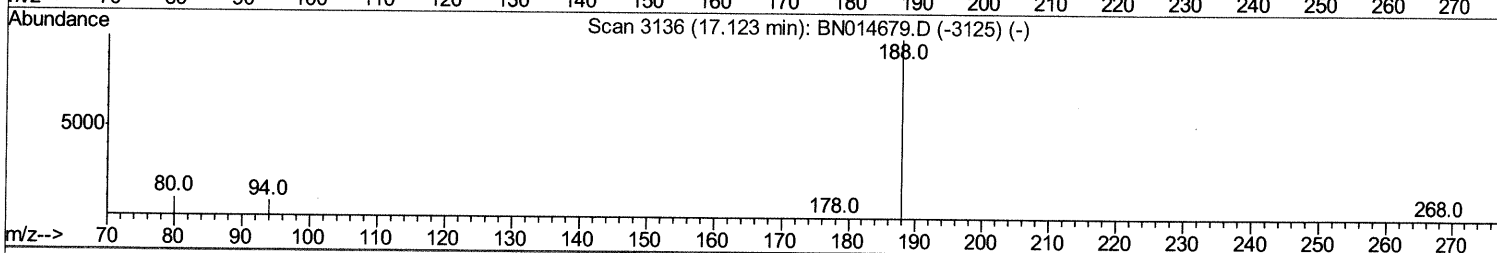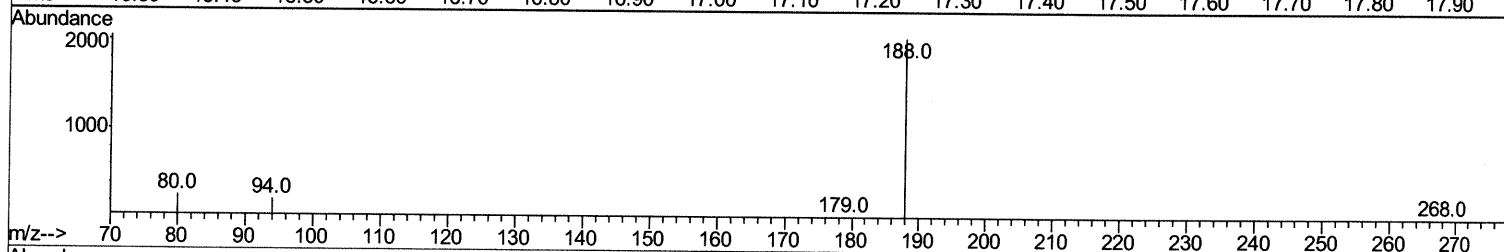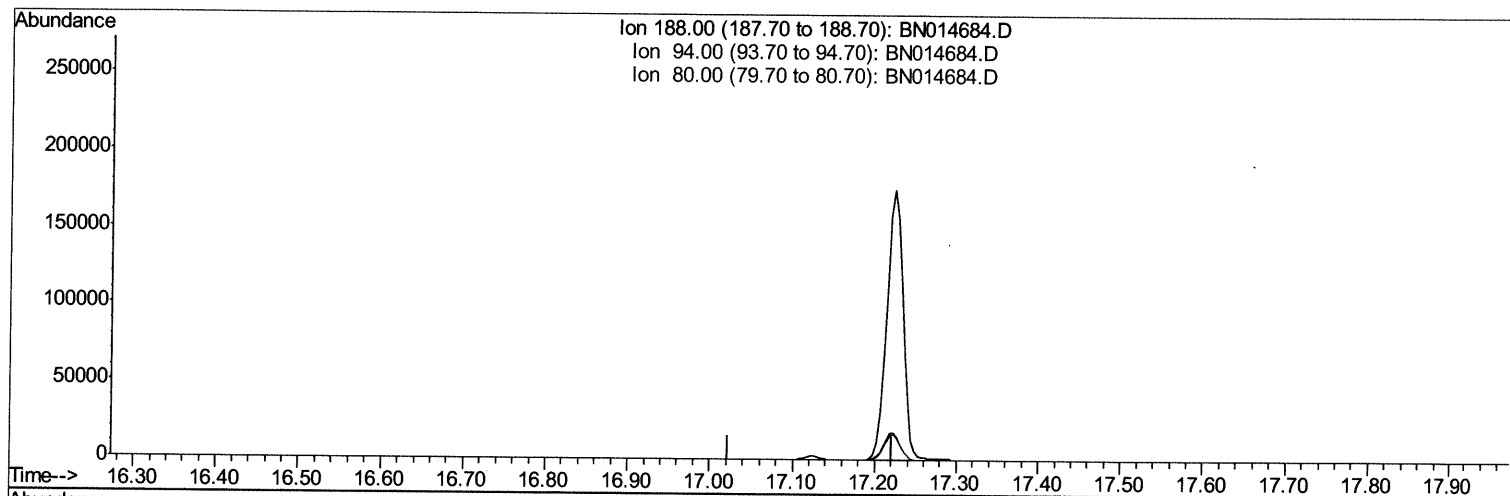

TIC: BN014684.D

(13) Phenanthrene-d10 (I)

17.123min (-17.123) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
 Data File : BN014684.D
 Acq On : 20 May 2021 17:22
 Operator : CG/JU
 Sample : M2465-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARK2

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:22:23 PM

Quant Time: May 20 17:56:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 20 16:48:16 2021
 Response via : Initial Calibration

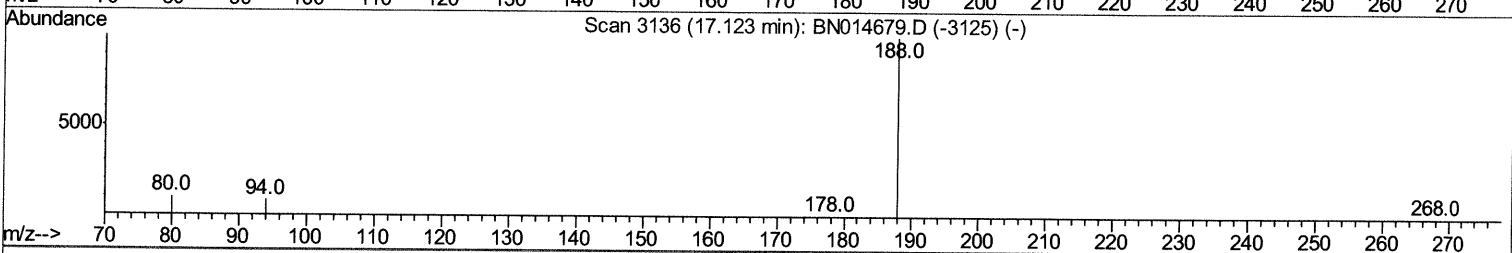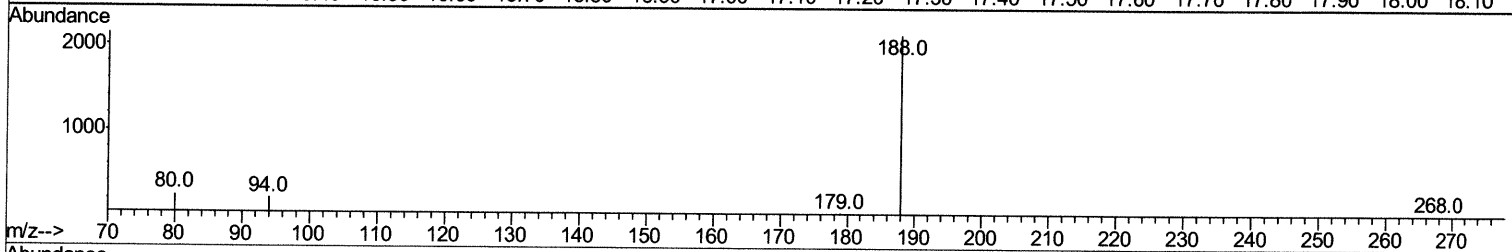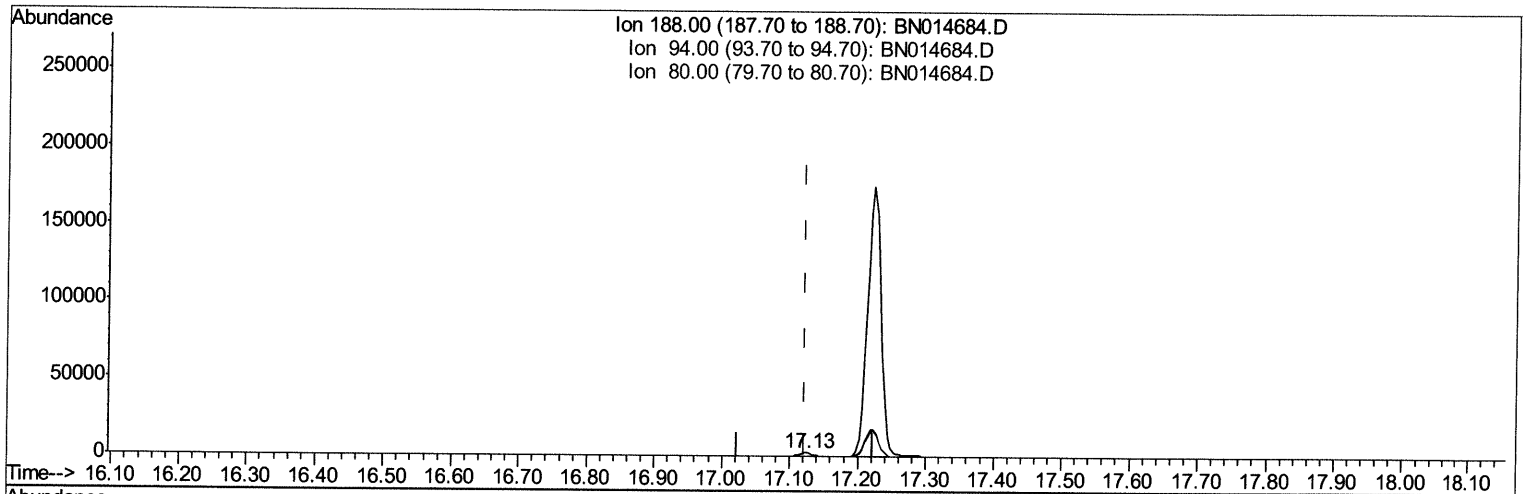

TIC: BN014684.D

(13) Phenanthrene-d10 (I)

17.126min (+0.003) 0.40ng/ul m 05/25/21 JU

response 3011

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	10.07
80.00	12.50	11.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN052021\
 Data File : BN014684.D
 Acq On : 20 May 2021 17:22
 Operator : CG/JU
 Sample : M2465-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YARK2

Manual Integrations
 APPROVED

mohammad
 5/21/2021 3:22:23 PM

Quant Time: May 20 17:57:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 20 16:48:16 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	476	0.40	ng/ul	0.00
4) Naphthalene-d8	10.51	136	1619	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.37	164	1257	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.13	188	3011m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.32	240	3309	0.40	ng/ul	0.00
23) Perylene-d12	23.58	264	3422	0.40	ng/ul	0.00

05/25/21ju

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	1363	2.79	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.11	152	990	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.16	212	3843	0.46	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed