

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019875.D
 Acq On : 20 May 2022 18:52
 Operator : CG/JU
 Sample : PB144915BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK915

Quant Time: May 21 01:53:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3786	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	12860	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	8132	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	17474	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	15188	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	13476	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	24062	5.370	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	6634	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	15747	0.328	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.609	202	2052	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	4065	0.070	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019875.D
Acq On : 20 May 2022 18:52
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK915

Quant Time: May 21 01:53:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration




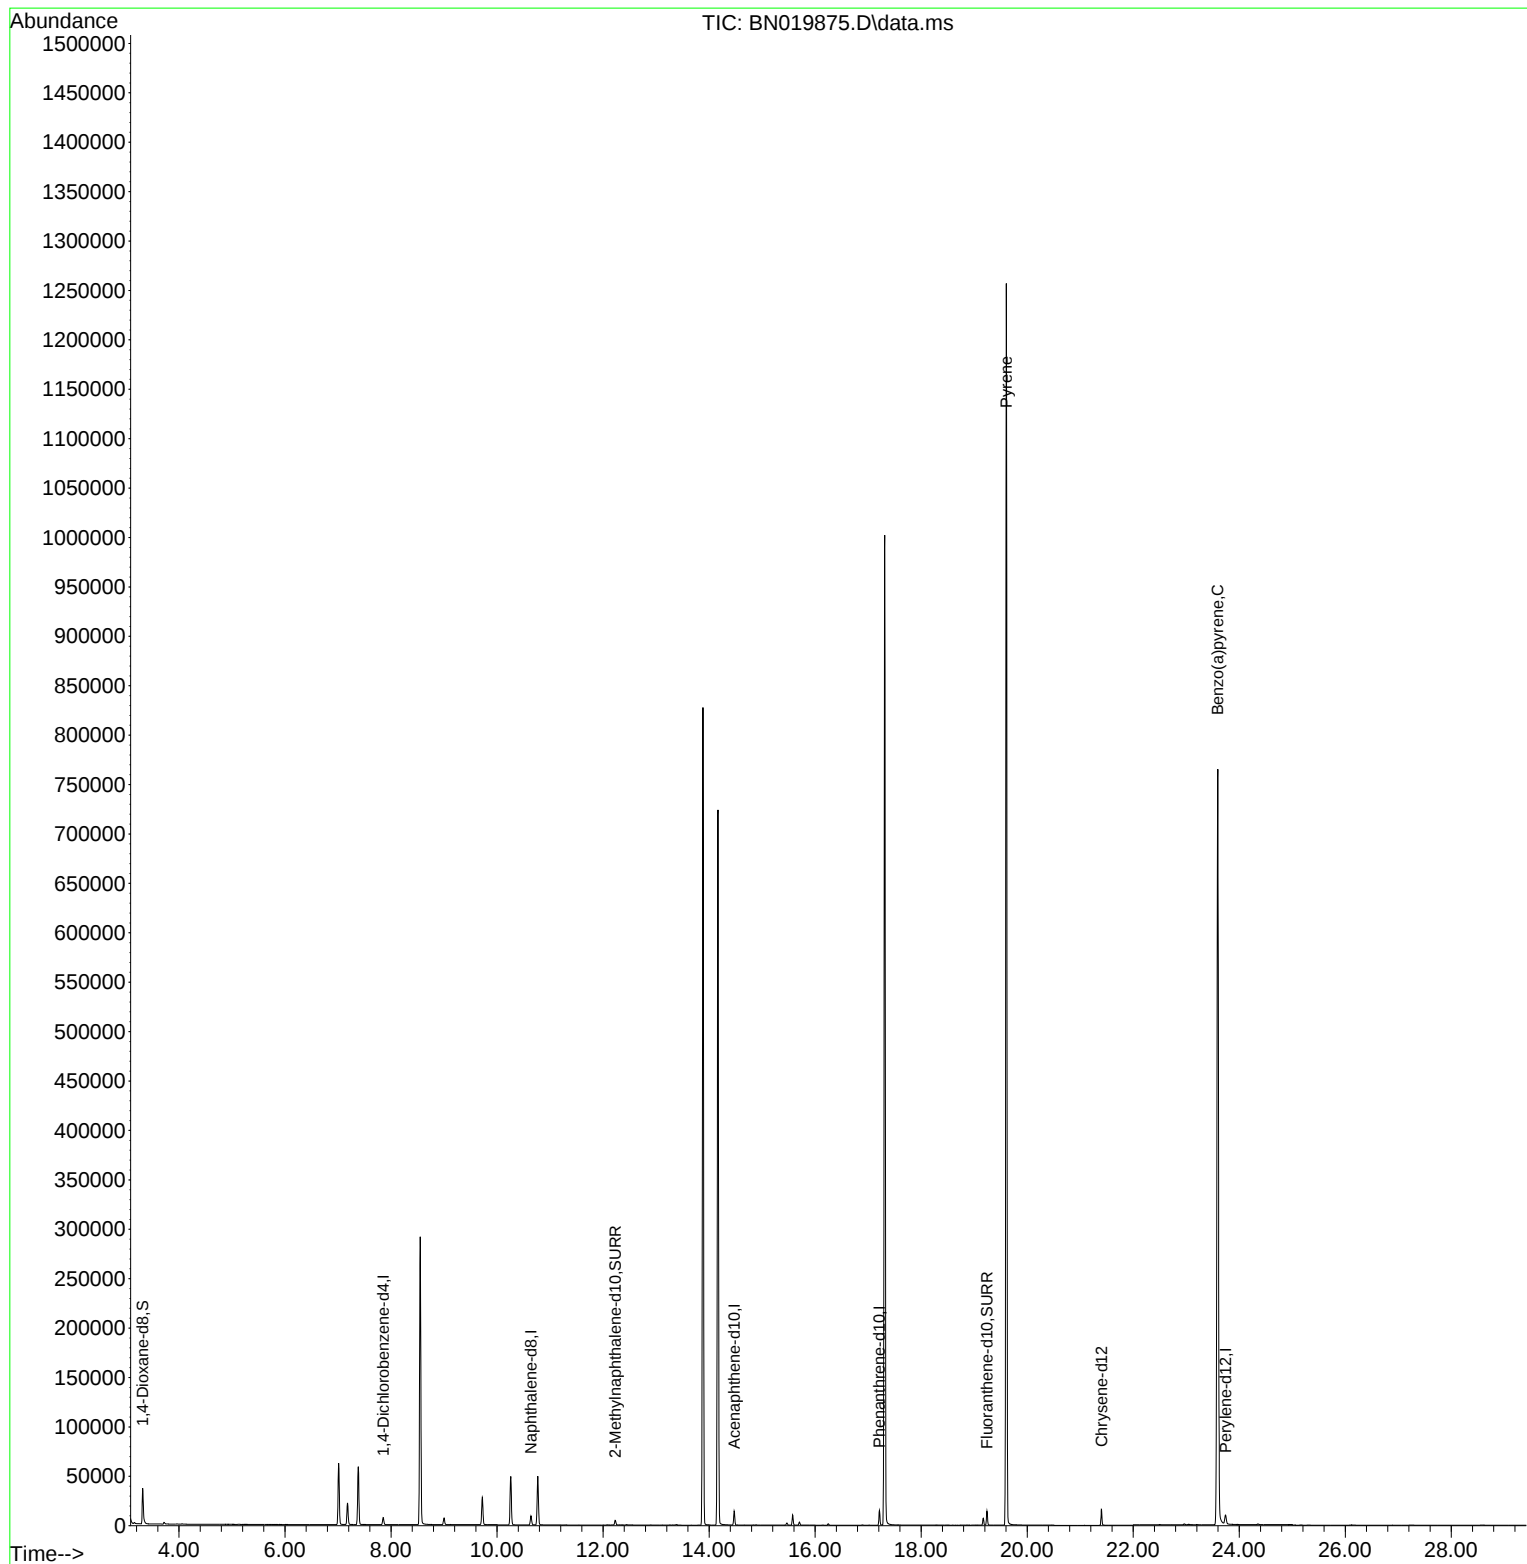


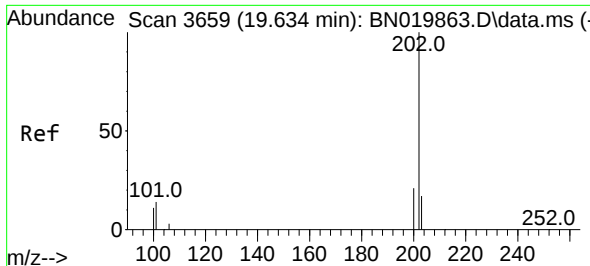

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.609 min Scan# 30
Delta R.T. -0.025 min
Lab File: BN019875.D
Acq: 20 May 2022 18:52

Instrument :
BNA_N
ClientSampleId :
SBLK915

Tgt Ion:202 Resp: 2052
Ion Ratio Lower Upper
202 100
101 162.9 11.4 17.0#
100 1162.8 9.0 13.4#

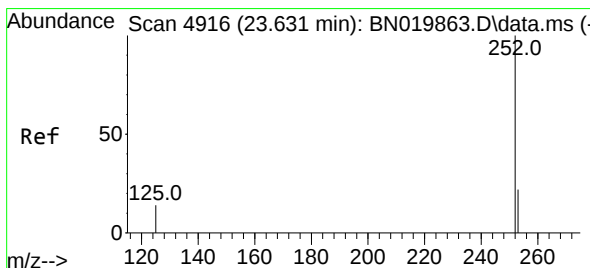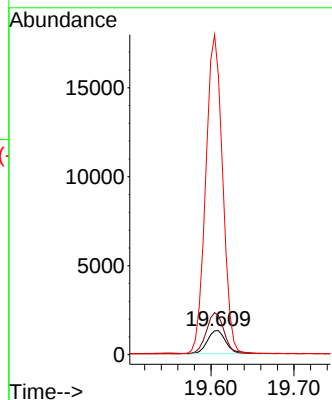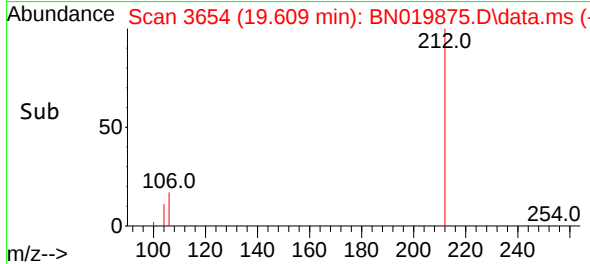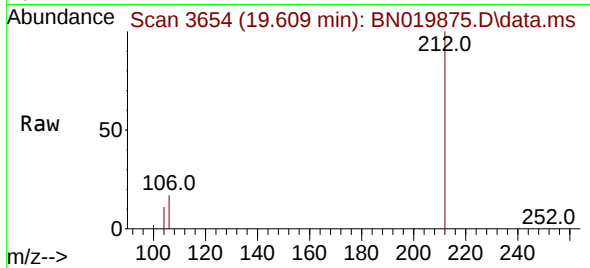

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.592 min Scan# 4903
Delta R.T. -0.047 min
Lab File: BN019875.D
Acq: 20 May 2022 18:52

Tgt Ion:252 Resp: 4065
Ion Ratio Lower Upper
252 100
253 38.4 23.4 35.0#
125 32.7 28.3 42.5

