
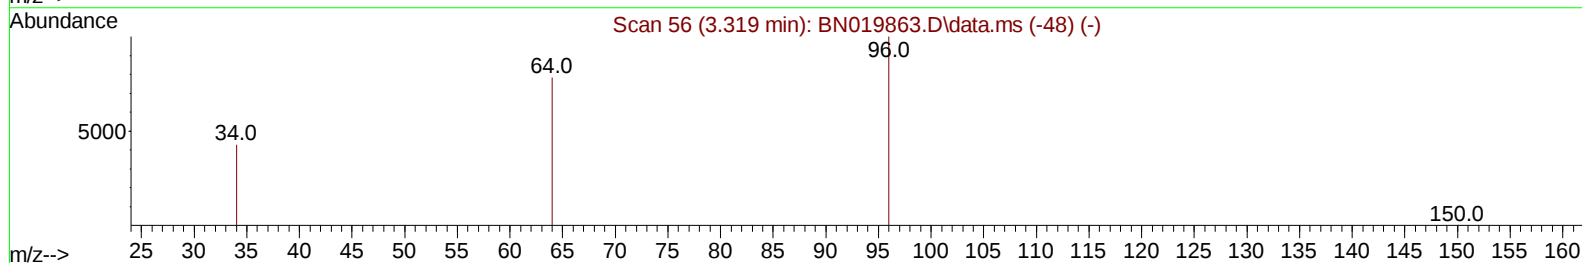
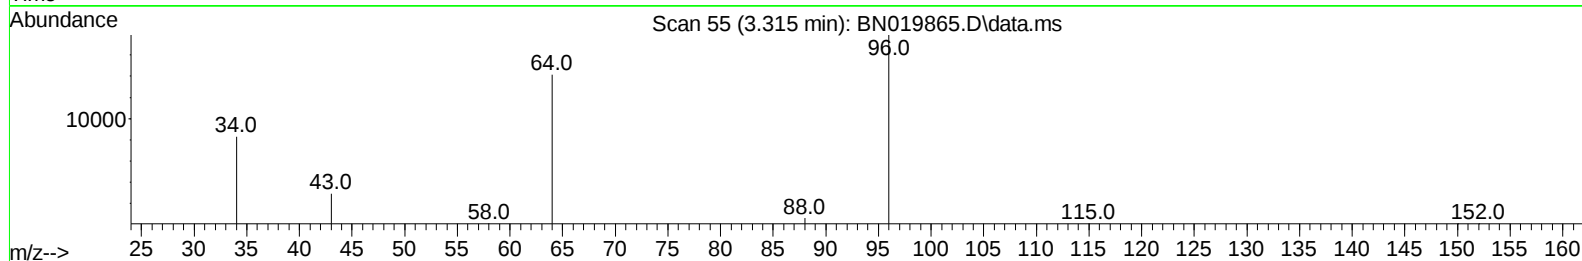


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019865.D
Acq On : 20 May 2022 12:09
Operator : CG/JU
Sample : PB144952BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 21 01:53:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

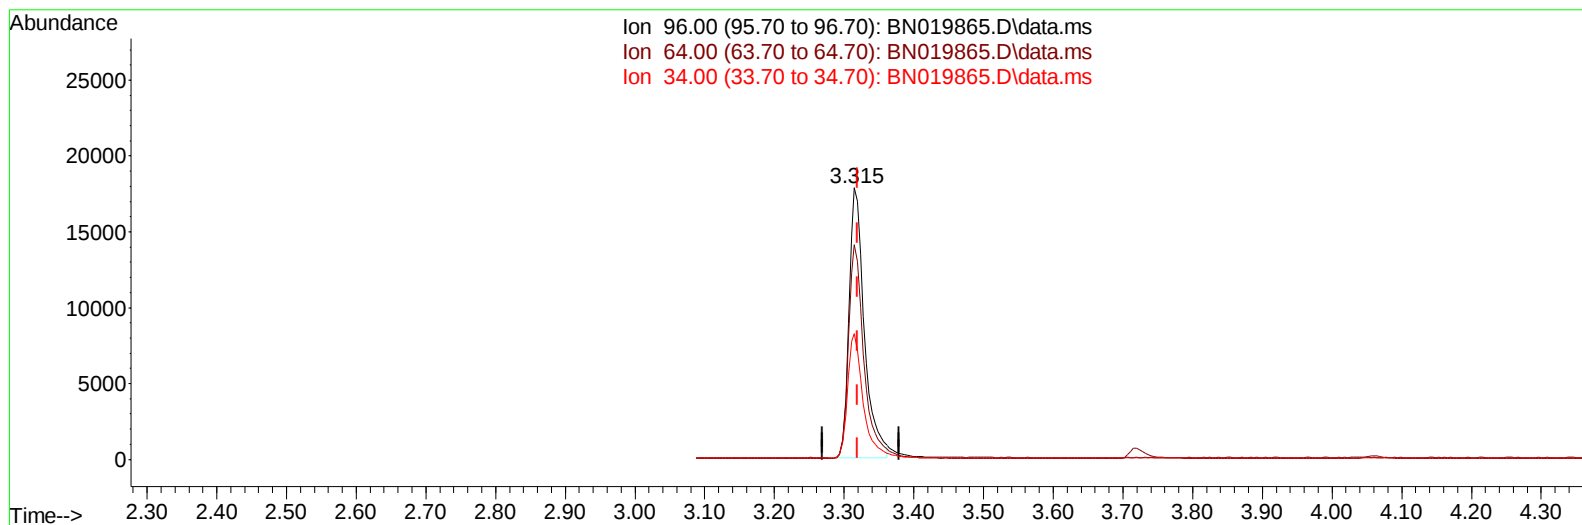

TIC: BN019865.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 6.62 ng/u1

response 26969

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.20#
34.00	22.70	46.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019865.D
Acq On : 20 May 2022 12:09
Operator : CG/JU
Sample : PB144952BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 21 01:53:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

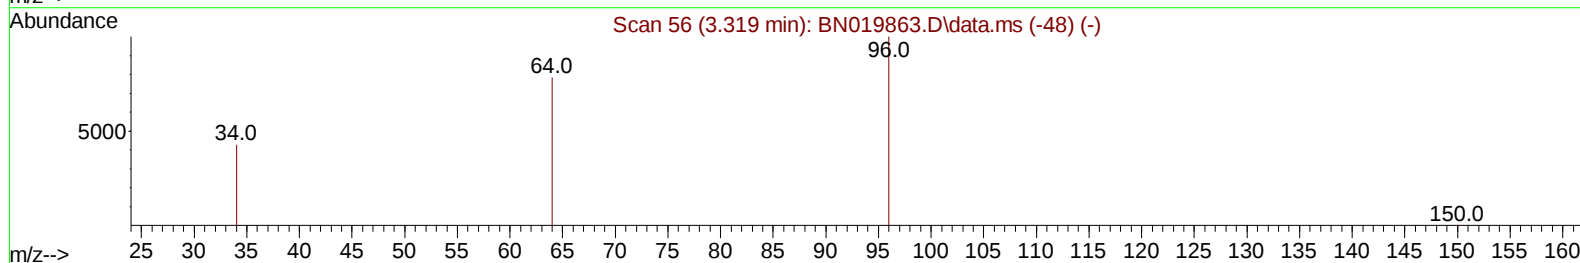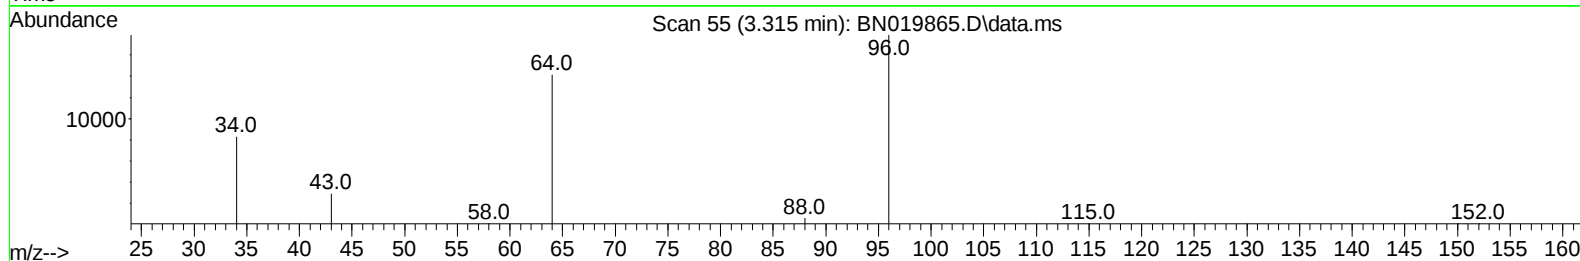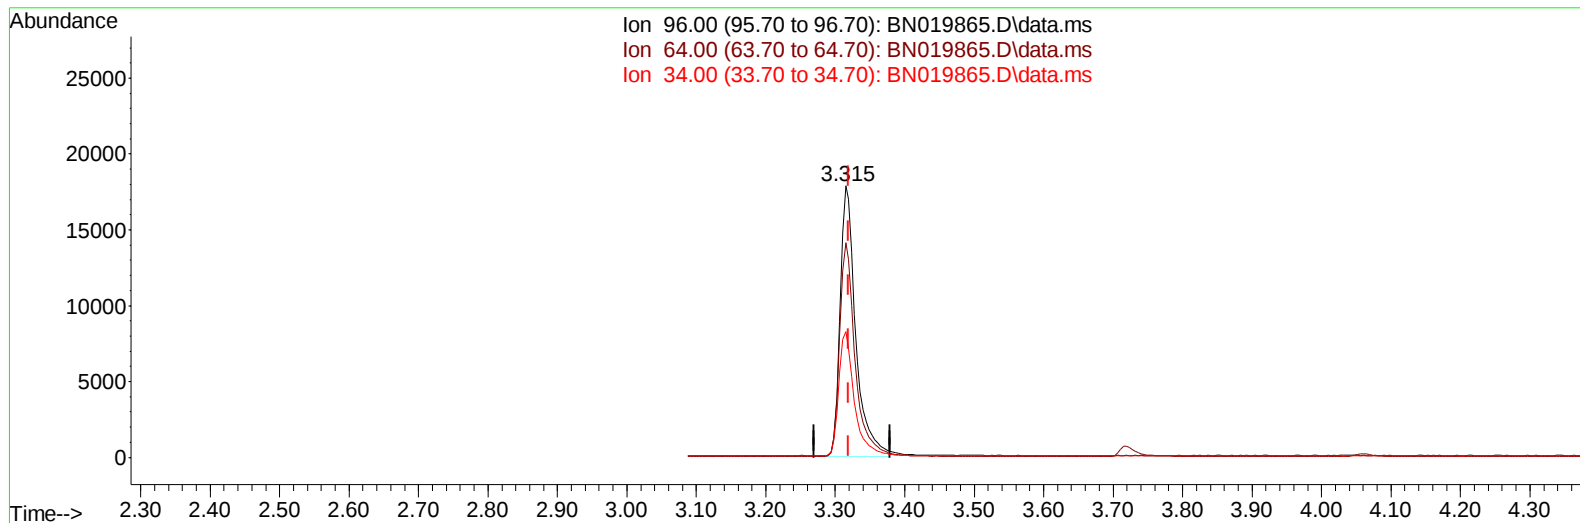

TIC: BN019865.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.315min (-0.004) 6.78 ng/ul m

response 27623

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.20#
34.00	22.70	46.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019865.D
 Acq On : 20 May 2022 12:09
 Operator : CG/JU
 Sample : PB144952BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 21 01:53:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3441	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	11640	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	7310	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	15704	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	14037	0.400	ng/ul	0.00
23) Perylene-d12	23.734	264	12816	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	27623m	6.783	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	7219	0.410	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	17283	0.389	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019865.D
Acq On : 20 May 2022 12:09
Operator : CG/JU
Sample : PB144952BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 21 01:53:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

