
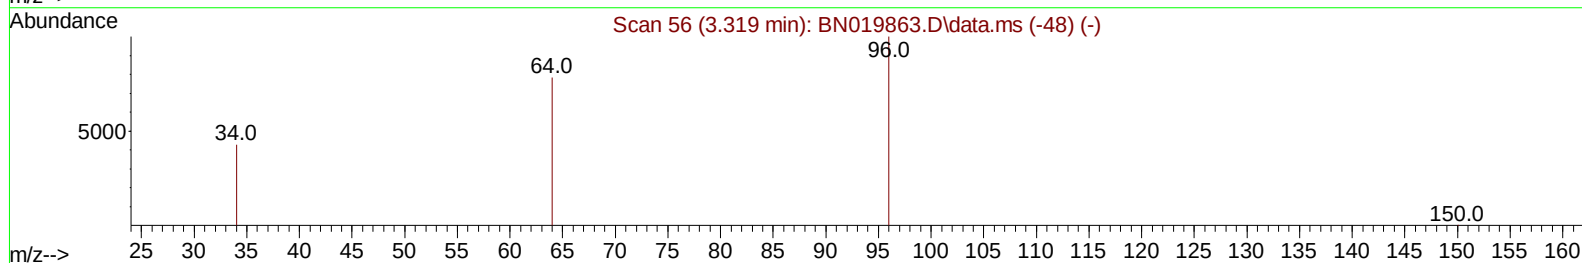
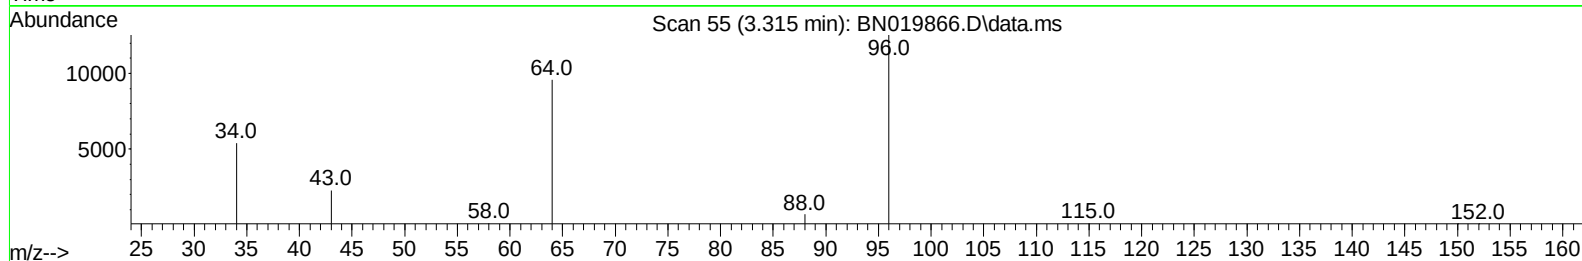


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019866.D
Acq On : 20 May 2022 12:52
Operator : CG/JU
Sample : N2918-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 21 01:53:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

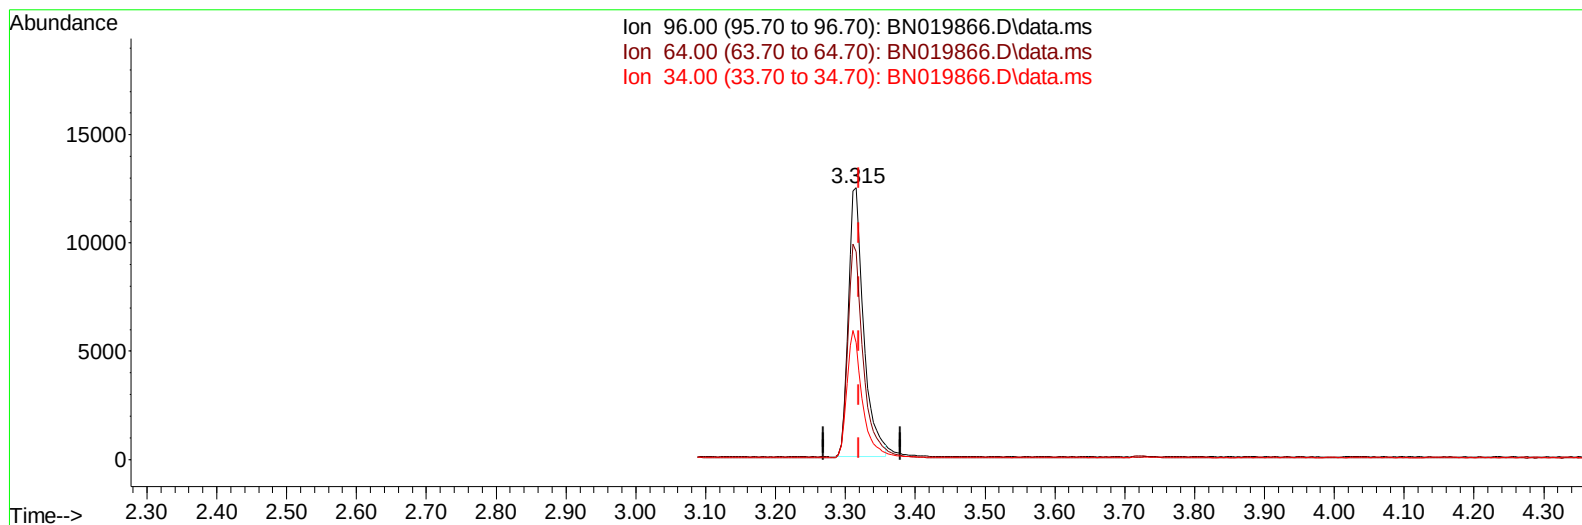

TIC: BN019866.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 4.03 ng/u1

response 18894

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.43#
34.00	22.70	43.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019866.D
Acq On : 20 May 2022 12:52
Operator : CG/JU
Sample : N2918-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 21 01:53:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

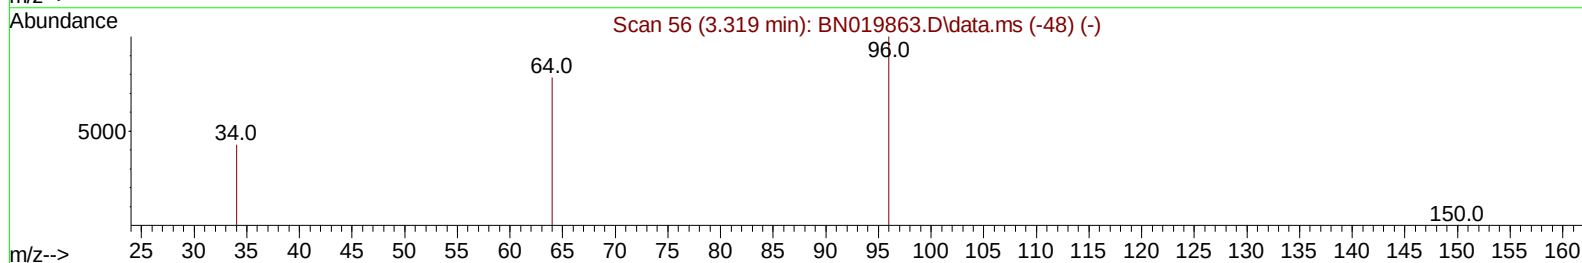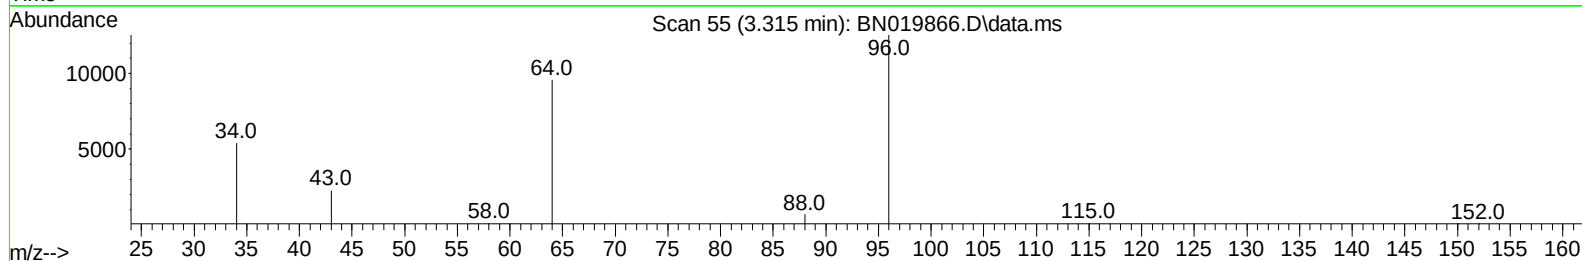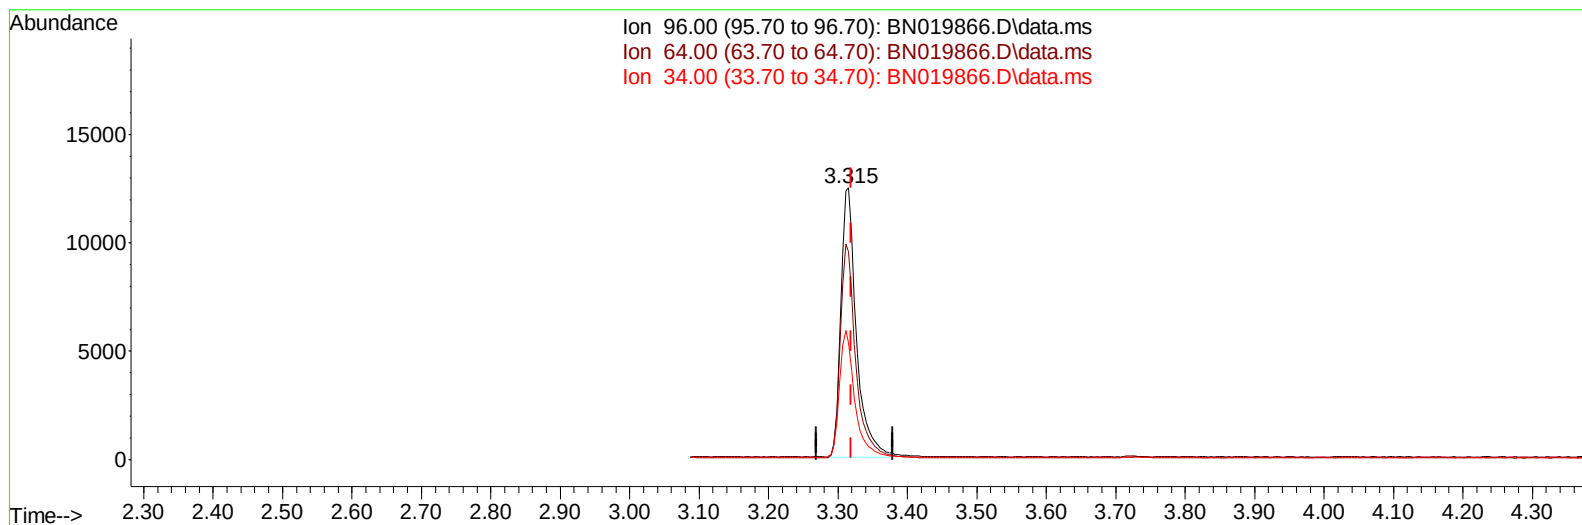

TIC: BN019866.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.315min (-0.004) 4.10 ng/ul m

response 19243

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.43#
34.00	22.70	43.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019866.D
 Acq On : 20 May 2022 12:52
 Operator : CG/JU
 Sample : N2918-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 21 01:53:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.847	152	3964	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	13395	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.470	164	8658	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	18460	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	16229	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	13674	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	19243m	4.102	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	6888	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	19223	0.374	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.689	128	1936309	44.648	ng/ul	98
7) 2-Methylnaphthalene	12.300	142	153985	5.829	ng/ul#	100
8) 1-Methylnaphthalene	12.515	142	108333	4.428	ng/ul#	100
10) Acenaphthylene	14.192	152	10971	0.256	ng/ul	98
11) Acenaphthene	14.534	153	140158	4.073	ng/ul	99
12) Fluorene	15.520	166	33259	0.881	ng/ul	99
14) Pentachlorophenol	16.867	266	4072	1.025	ng/ul	91
15) Phenanthrene	17.255	178	22752	0.335	ng/ul	100
16) Anthracene	17.344	178	3422	0.062	ng/ul	94
19) Fluoranthene	19.272	202	4041	0.054	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019866.D
Acq On : 20 May 2022 12:52
Operator : CG/JU
Sample : N2918-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 21 01:53:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

