
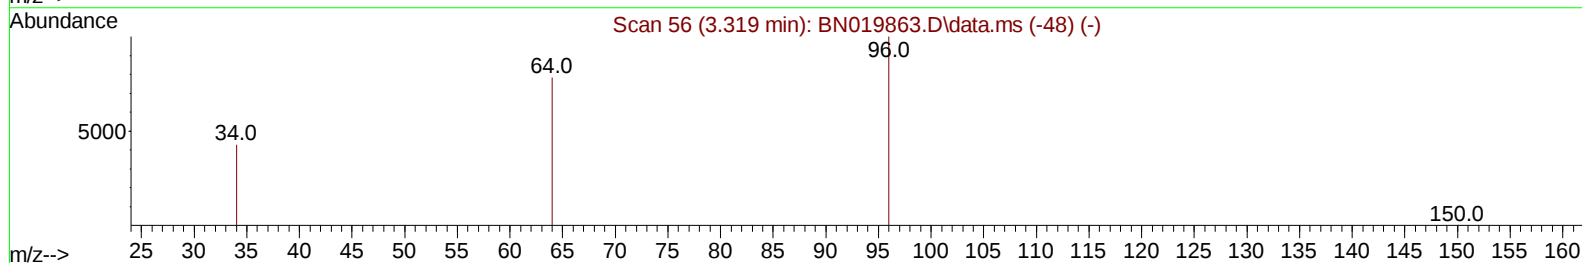
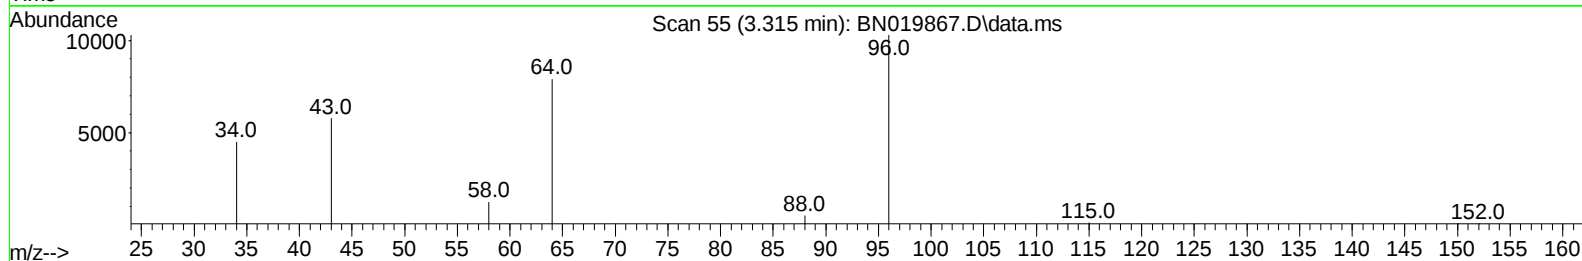


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019867.D
Acq On : 20 May 2022 13:28
Operator : CG/JU
Sample : N2918-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 23 06:00:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

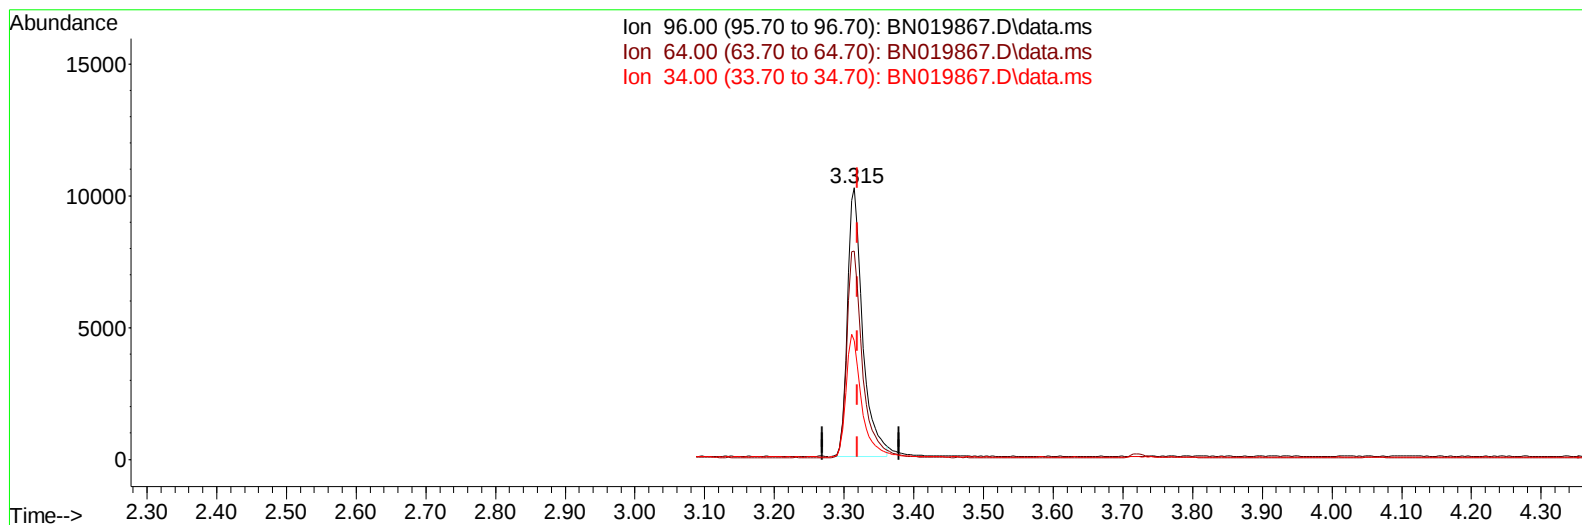

TIC: BN019867.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 3.81 ng/u1

response 15258

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.86#
34.00	22.70	43.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019867.D
 Acq On : 20 May 2022 13:28
 Operator : CG/JU
 Sample : N2918-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 21 01:53:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

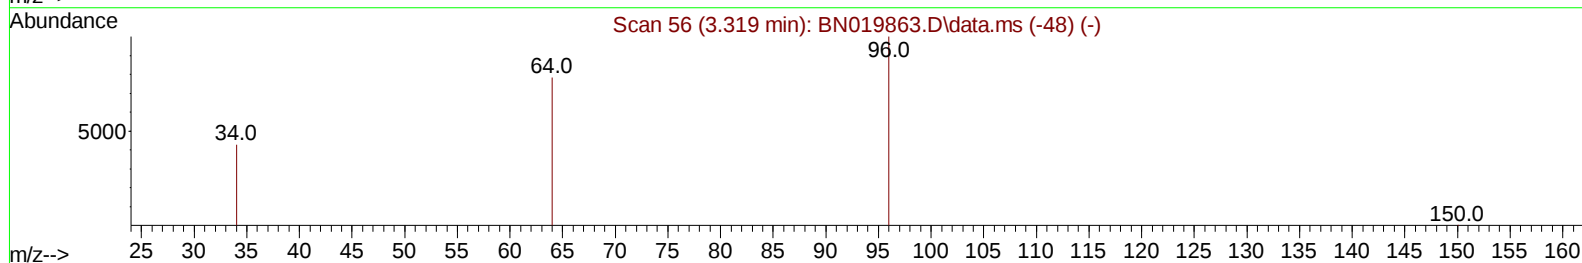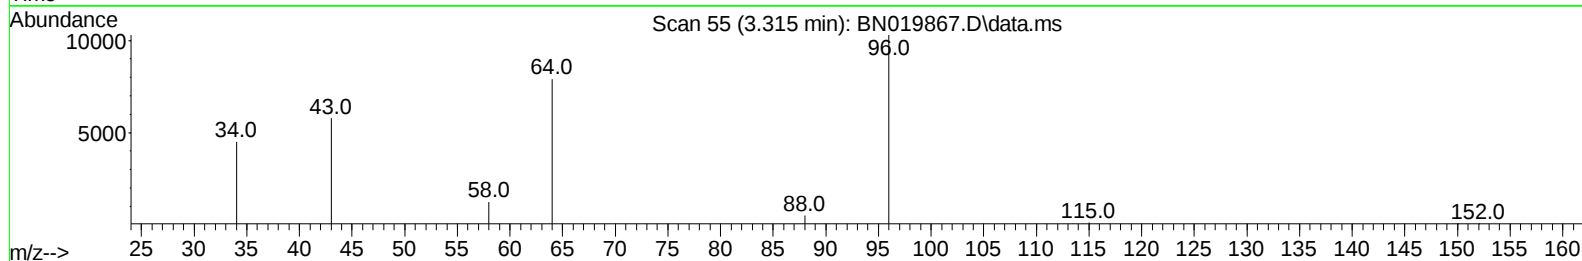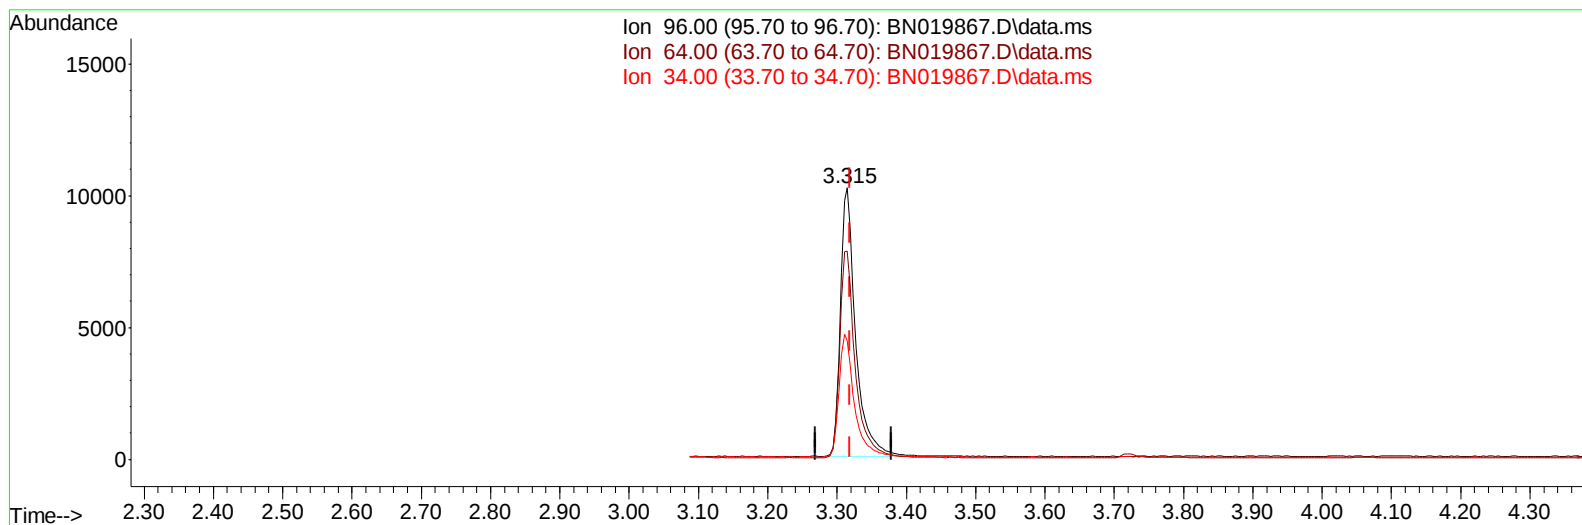

TIC: BN019867.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 3.88 ng/ul m

response 15517

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.86#
34.00	22.70	43.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019867.D
Acq On : 20 May 2022 13:28
Operator : CG/JU
Sample : N2918-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 23 06:00:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

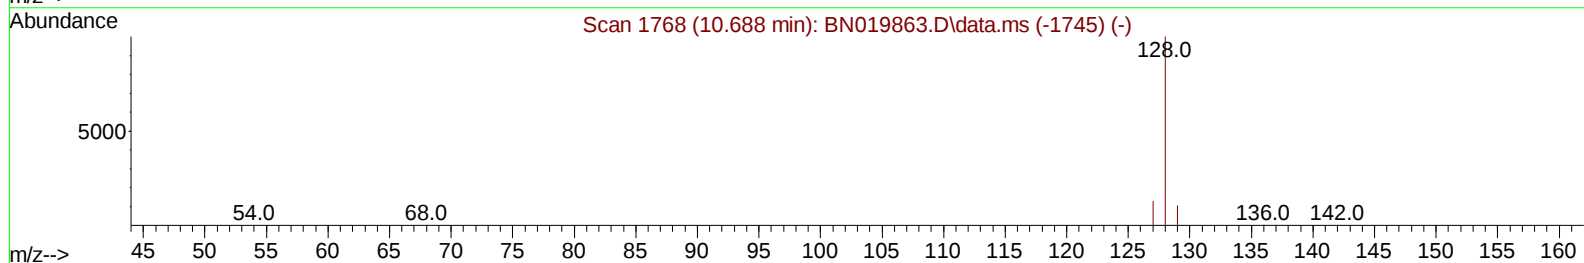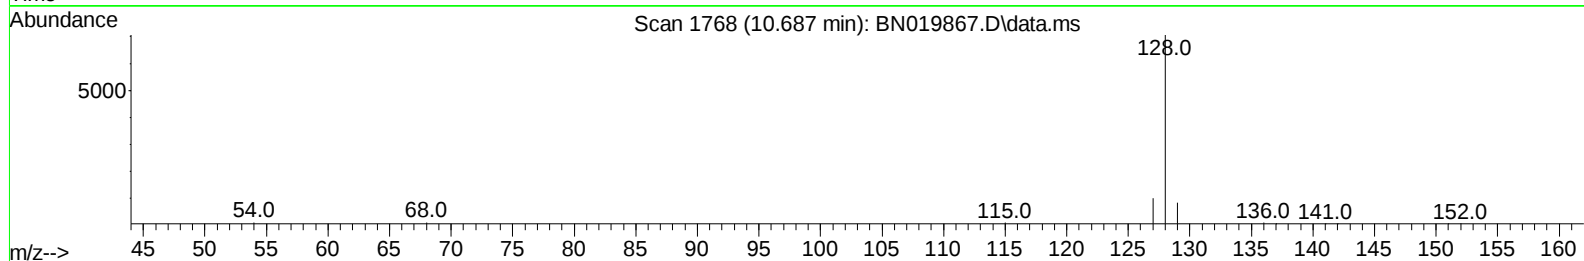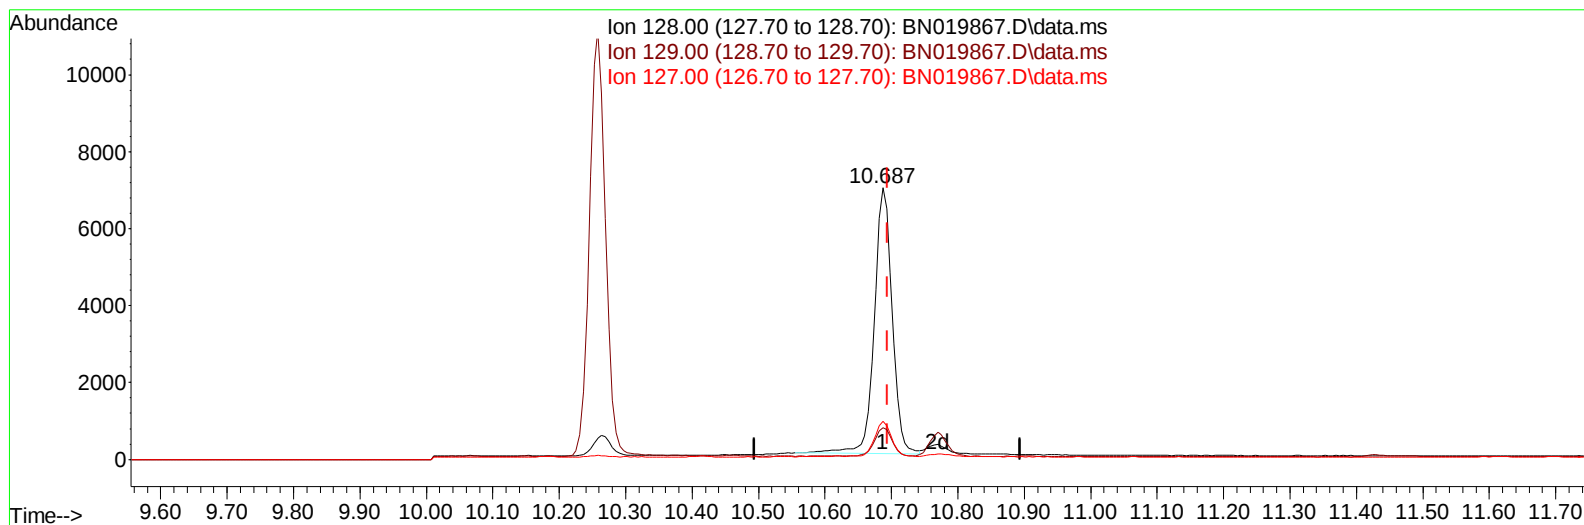




TIC: BN019867.D\data.ms

(5) Naphthalene**10.687min (-0.007) 0.35 ng/ul****response 12936**

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	11.90	11.80
127.00	13.70	14.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019867.D
Acq On : 20 May 2022 13:28
Operator : CG/JU
Sample : N2918-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 21 01:53:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

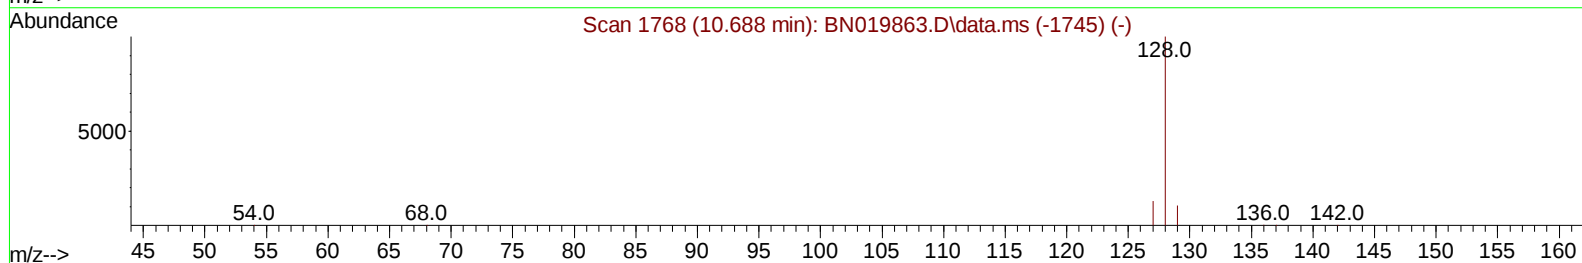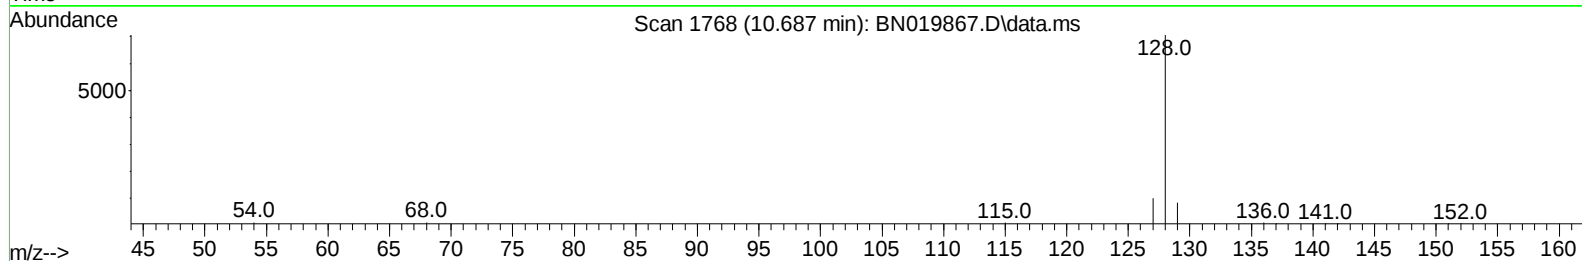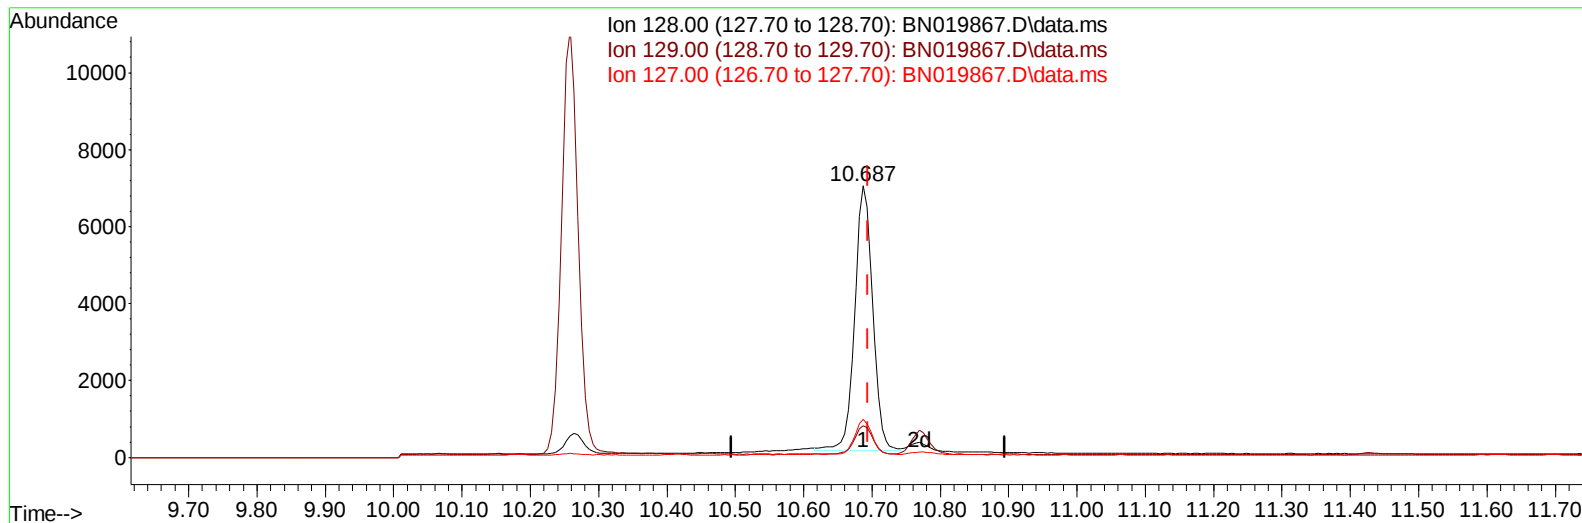

TIC: BN019867.D\data.ms

(5) Naphthalene**10.687min (-0.007) 0.34 ng/ul m****response 12636**

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	11.90	11.80
127.00	13.70	14.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019867.D
 Acq On : 20 May 2022 13:28
 Operator : CG/JU
 Sample : N2918-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 21 01:53:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3381	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	11333	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	7287	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	16092	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	14862	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	13153	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	15517m	3.878	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	5463	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	17136	0.364	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.687	128	12636m	0.344	ng/ul	
7) 2-Methylnaphthalene	12.299	142	1138	0.051	ng/ul#	100
8) 1-Methylnaphthalene	12.519	142	1078	0.052	ng/ul#	100
11) Acenaphthene	14.537	153	1496	0.052	ng/ul	97
12) Fluorene	15.518	166	1245	0.039	ng/ul#	95
15) Phenanthrene	17.254	178	2081	0.035	ng/ul#	89
16) Anthracene	17.346	178	1516	0.031	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019867.D
Acq On : 20 May 2022 13:28
Operator : CG/JU
Sample : N2918-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 21 01:53:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

