
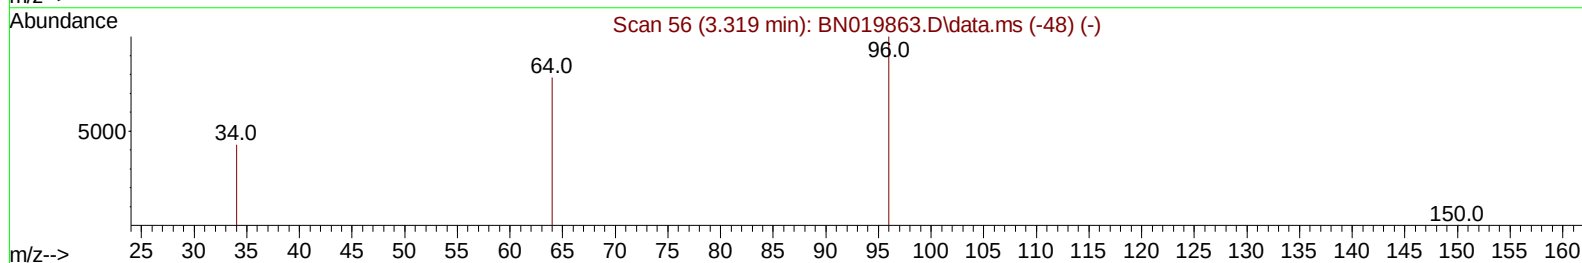
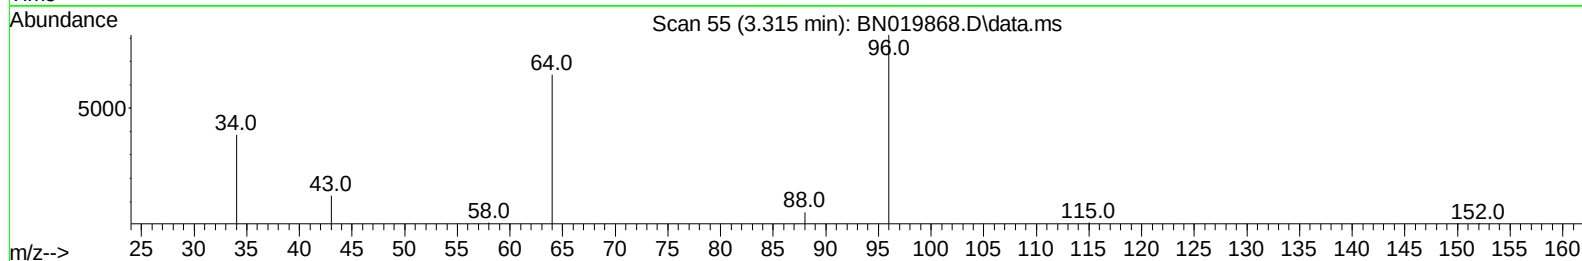


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019868.D
Acq On : 20 May 2022 14:40
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

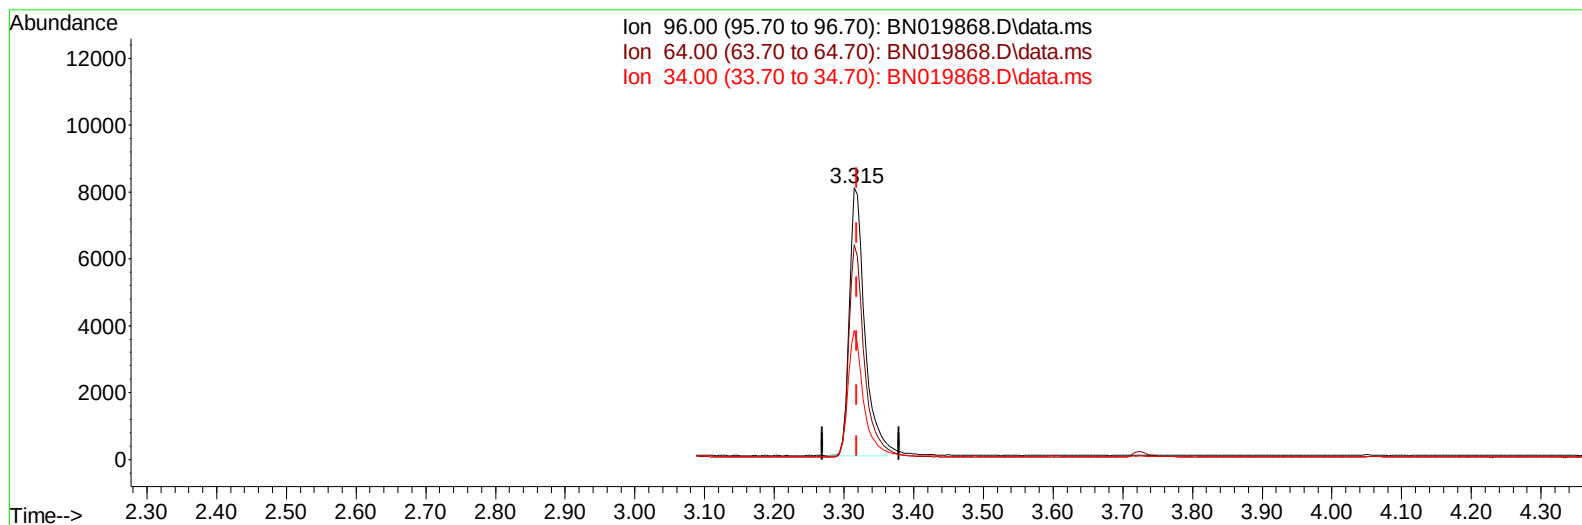

TIC: BN019868.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 2.96 ng/uI

response 12217

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.06#
34.00	22.70	47.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019868.D
 Acq On : 20 May 2022 14:40
 Operator : CG/JU
 Sample : N2918-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

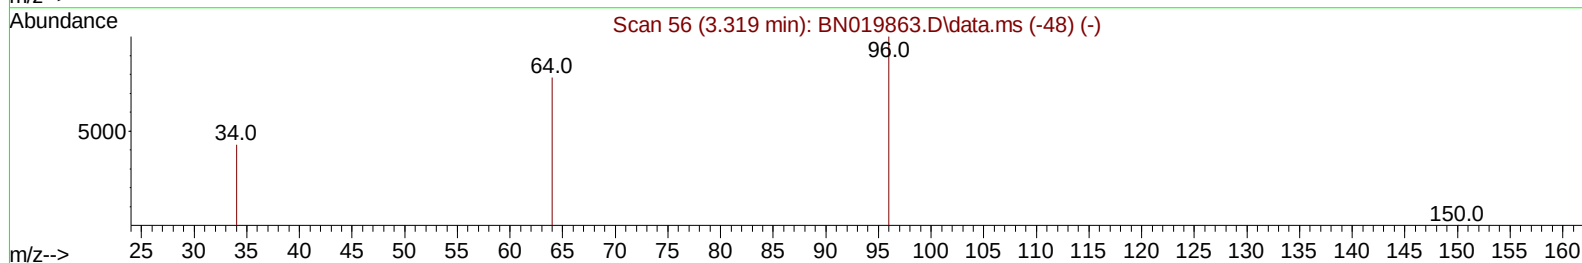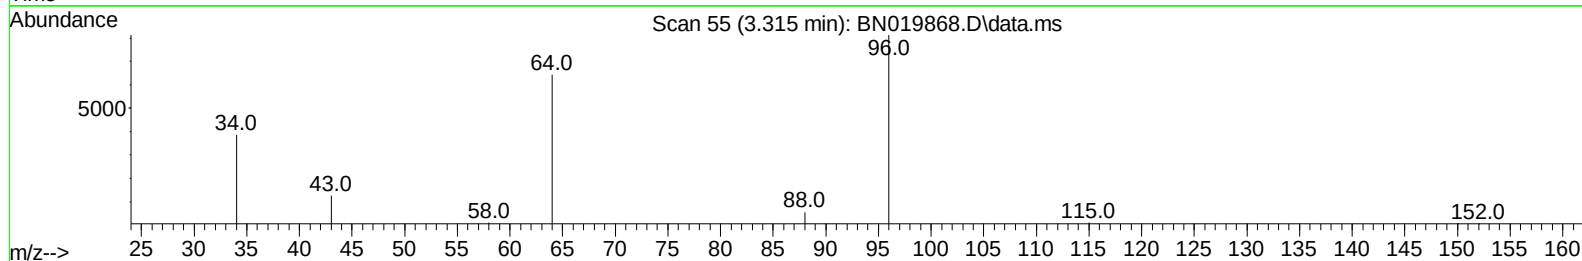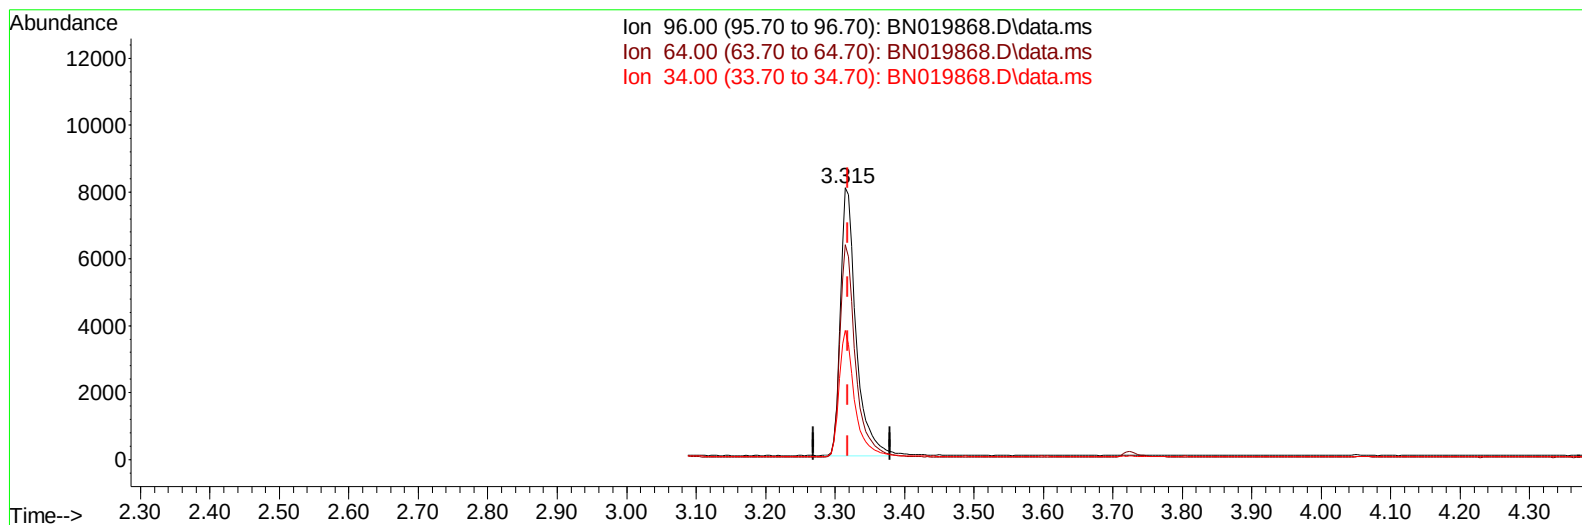

TIC: BN019868.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 3.02 ng/ul m

response 12460

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.06#
34.00	22.70	47.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019868.D
Acq On : 20 May 2022 14:40
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

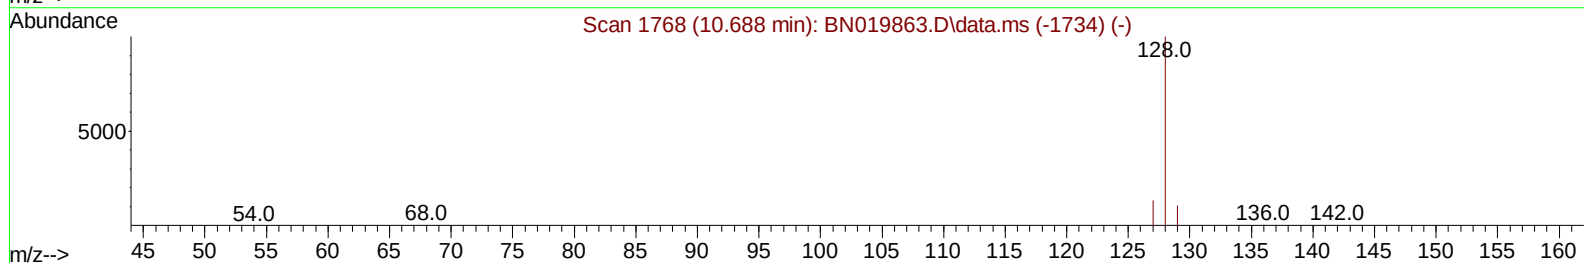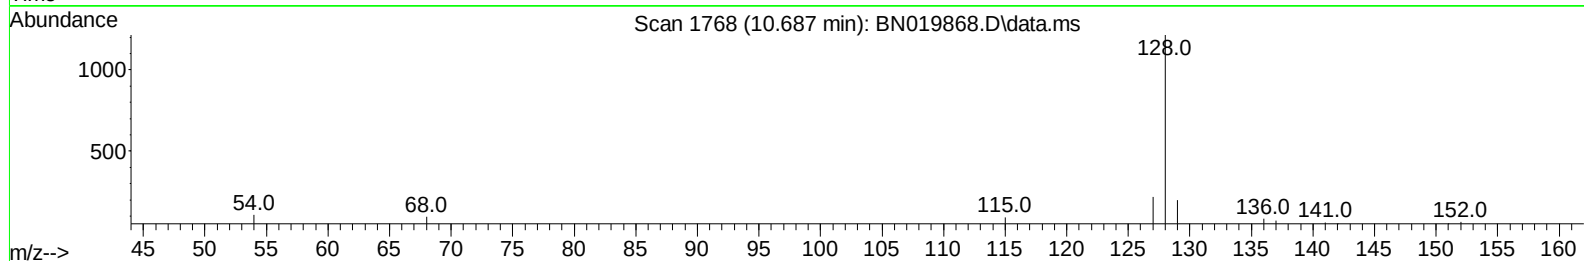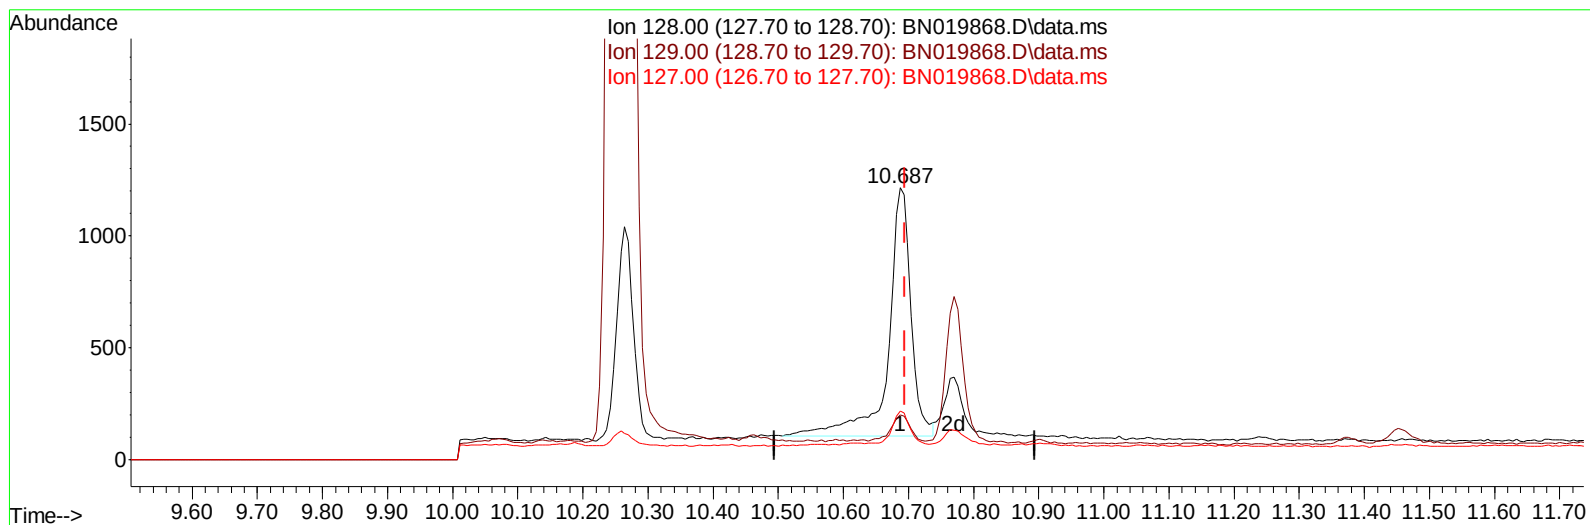




TIC: BN019868.D\data.ms

(5) Naphthalene**10.687min (-0.007) 0.07 ng/u1****response 2686**

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	11.90	16.47#
127.00	13.70	17.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019868.D
Acq On : 20 May 2022 14:40
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

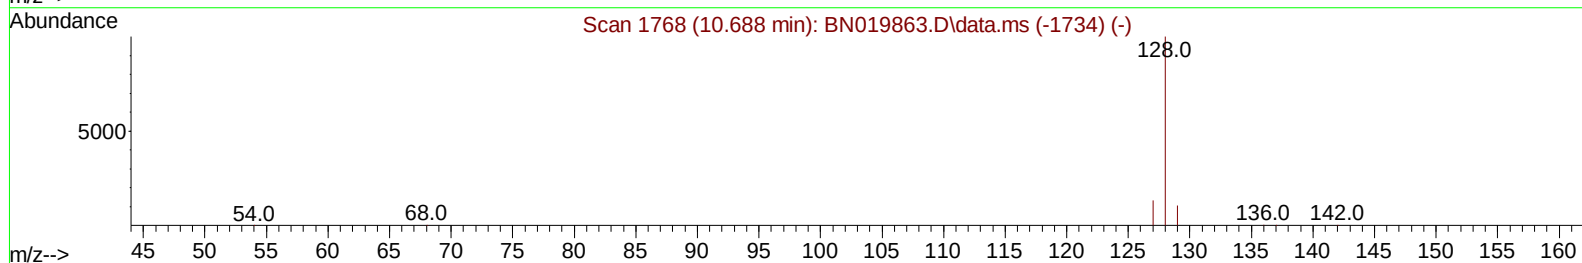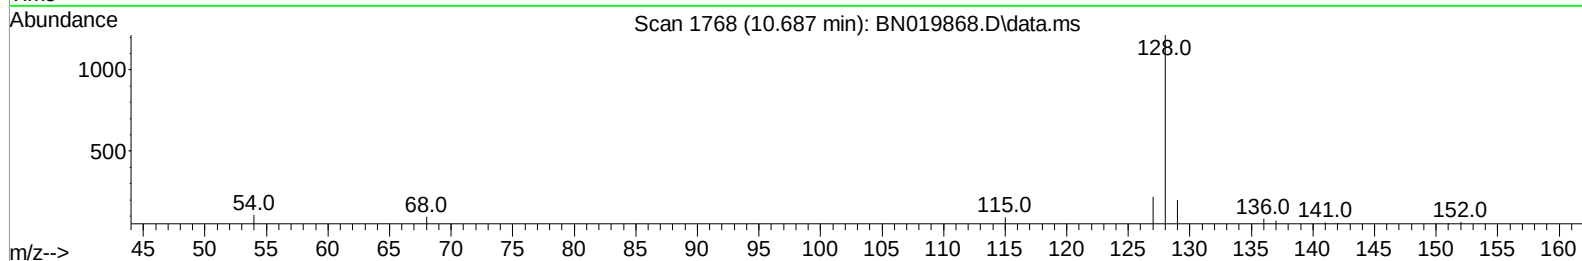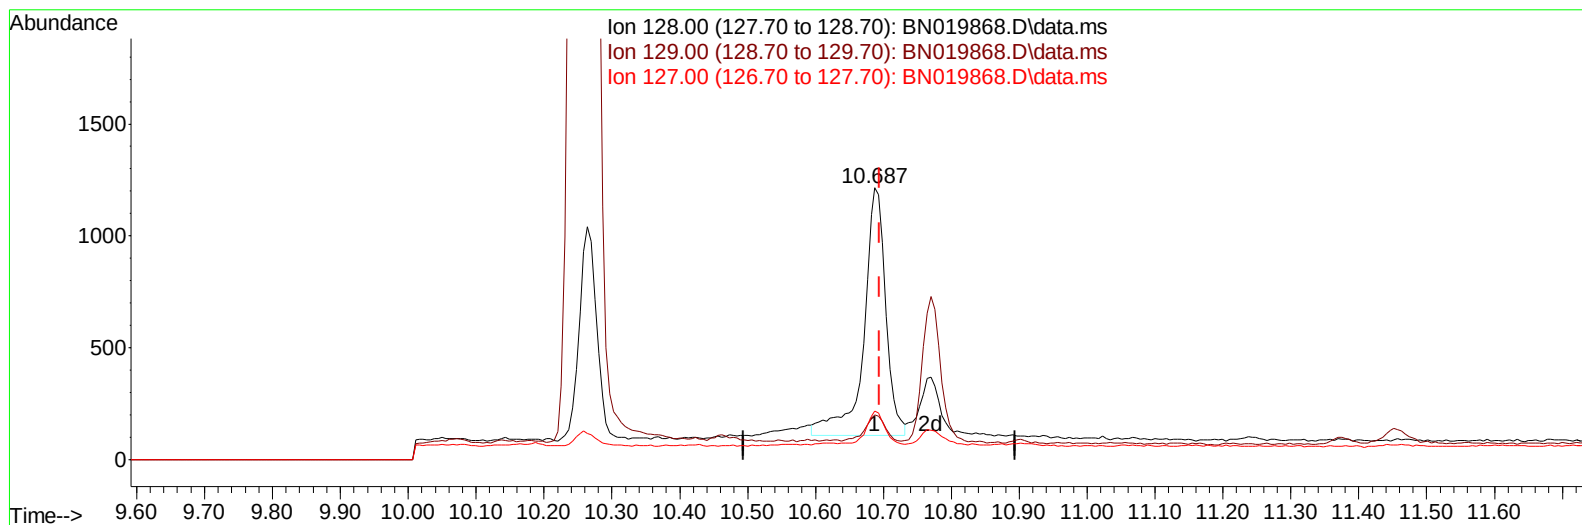

TIC: BN019868.D\data.ms

(5) Naphthalene**10.687min (-0.007) 0.07 ng/ul m****response 2502**

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	11.90	16.47#
127.00	13.70	17.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019868.D
 Acq On : 20 May 2022 14:40
 Operator : CG/JU
 Sample : N2918-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3484	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	11794	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	7530	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	16100	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	14187	0.400	ng/ul	0.00
23) Perylene-d12	23.738	264	12253	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	12460m	3.022	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	6742	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	18524	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.687	128	2502m	0.066	ng/ul	
7) 2-Methylnaphthalene	12.299	142	486	0.021	ng/ul#	100
11) Acenaphthene	14.538	153	1995	0.067	ng/ul	98
12) Fluorene	15.518	166	1737	0.053	ng/ul#	93
14) Pentachlorophenol	16.870	266	73	0.021	ng/ul#	84
15) Phenanthrene	17.254	178	1647	0.028	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019868.D
Acq On : 20 May 2022 14:40
Operator : CG/JU
Sample : N2918-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 21 01:53:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

