
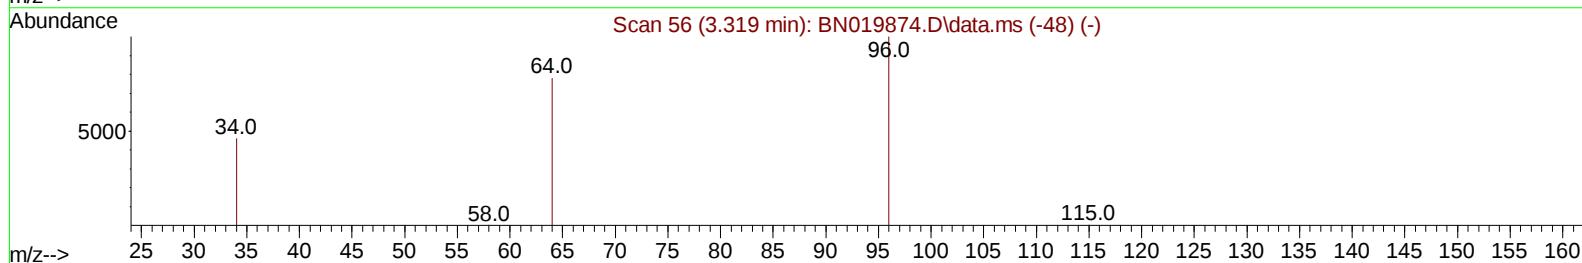
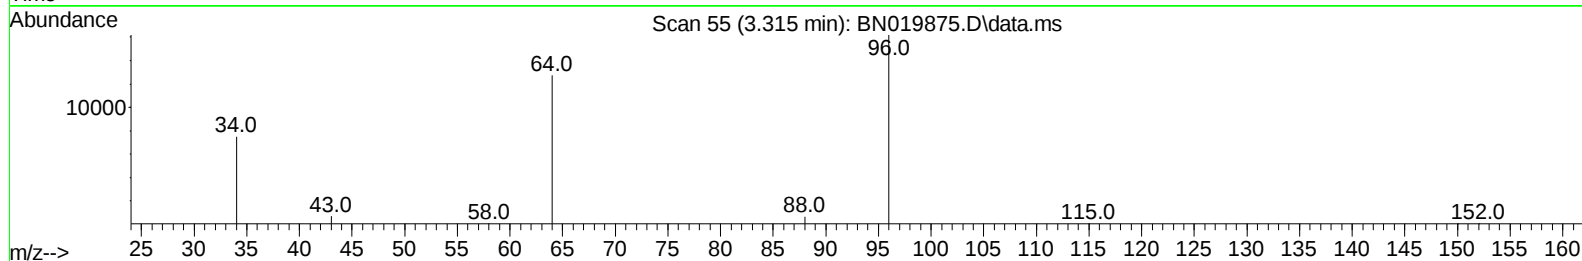


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019875.D
Acq On : 20 May 2022 18:52
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 21 01:53:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

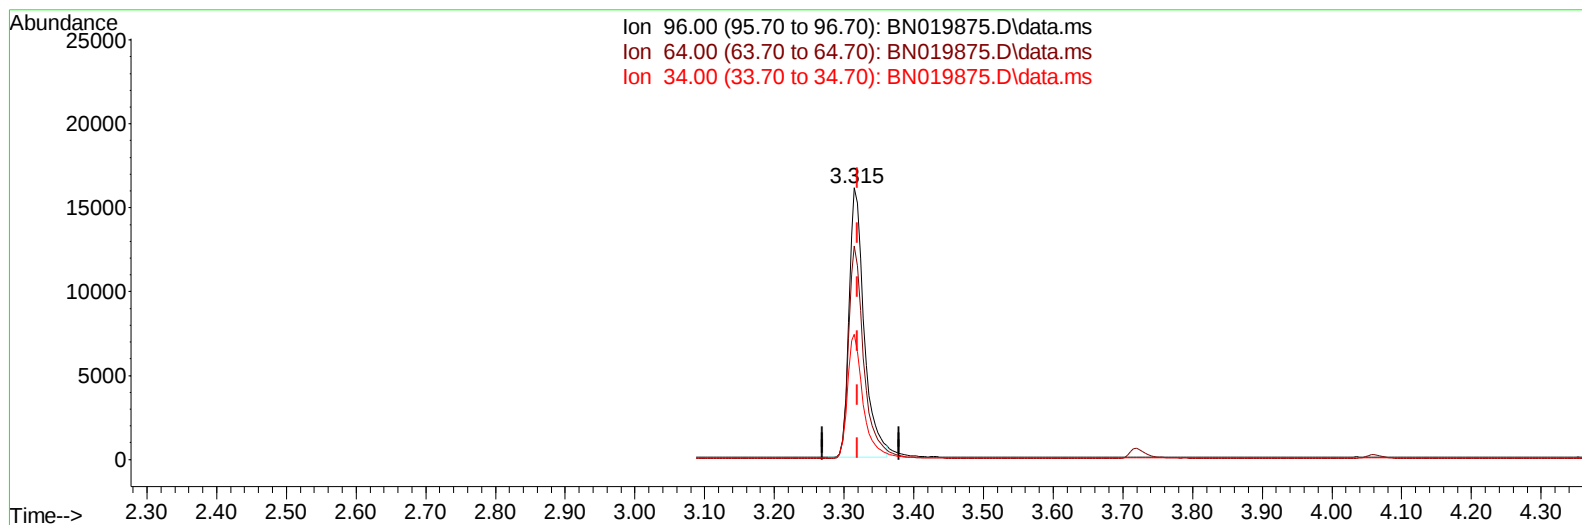

TIC: BN019875.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 5.37 ng/u1

response 24062

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	78.60#
34.00	22.70	46.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019875.D
Acq On : 20 May 2022 18:52
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 21 01:53:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

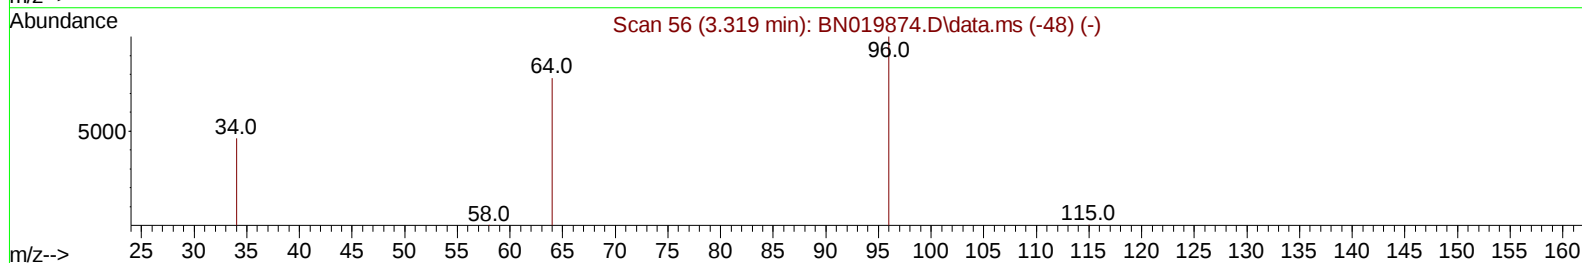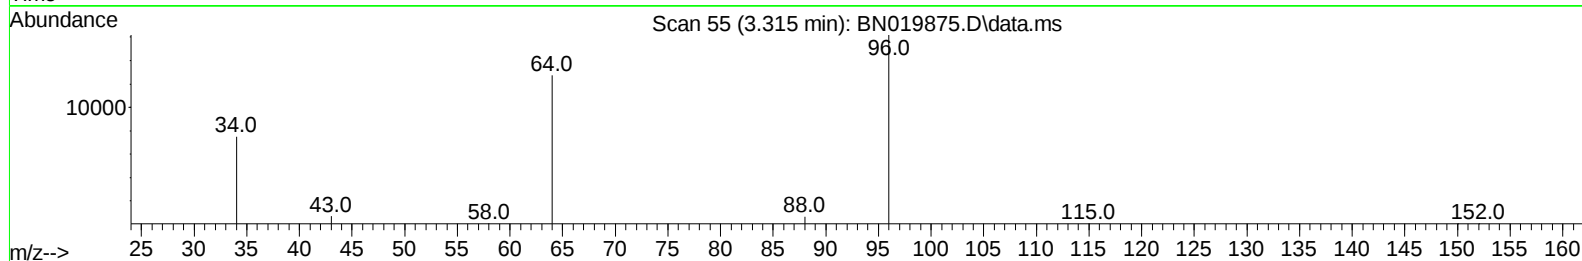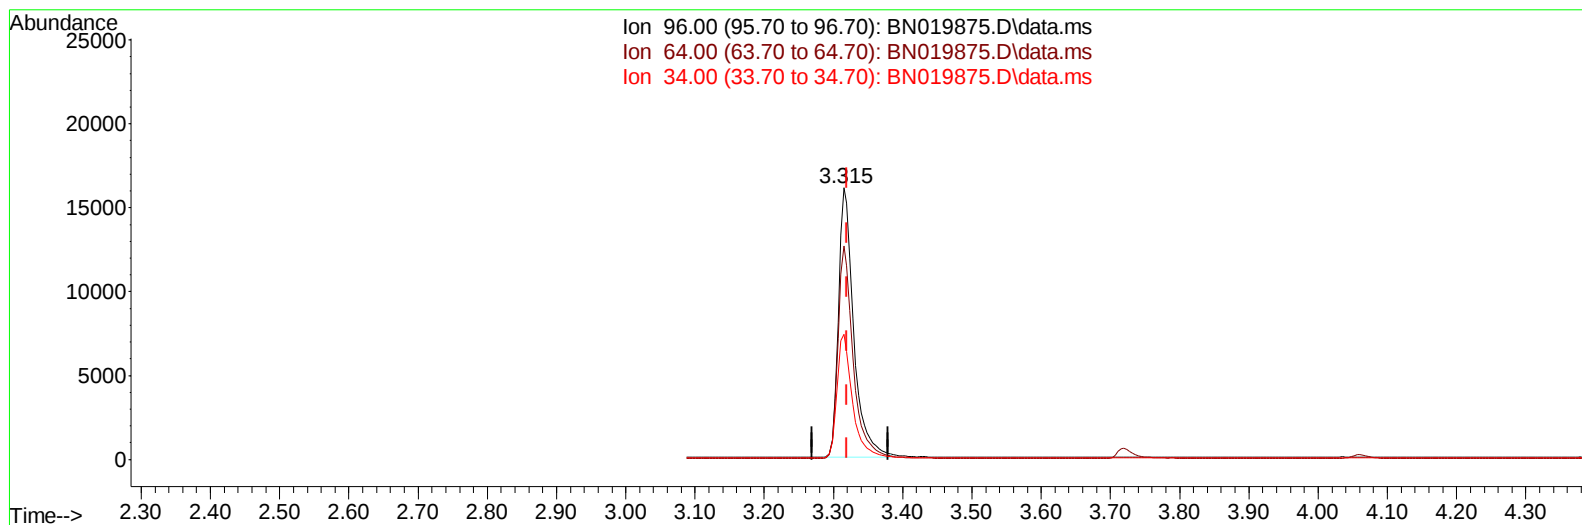

TIC: BN019875.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.315min (-0.004) 5.47 ng/ul m

response 24502

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	78.60#
34.00	22.70	46.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019875.D
 Acq On : 20 May 2022 18:52
 Operator : CG/JU
 Sample : PB144915BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 21 01:53:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	3786	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	12860	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	8132	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	17474	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	15188	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	13476	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	24502m	5.468	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	6634	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	15747	0.328	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019875.D
Acq On : 20 May 2022 18:52
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: May 21 01:53:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

