
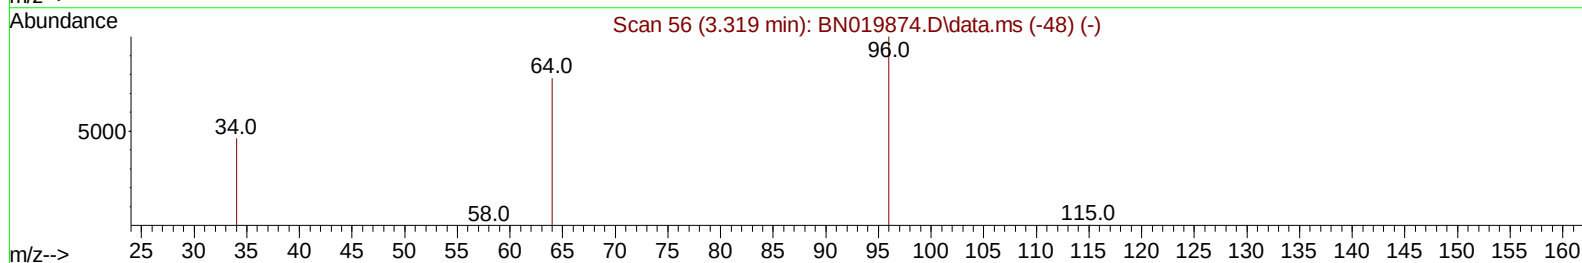
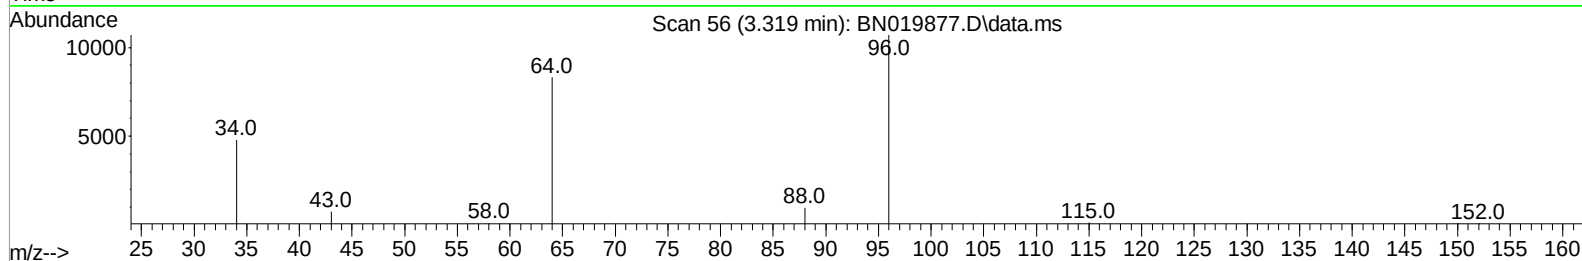


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019877.D
Acq On : 20 May 2022 20:04
Operator : CG/JU
Sample : N2843-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 21 01:54:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

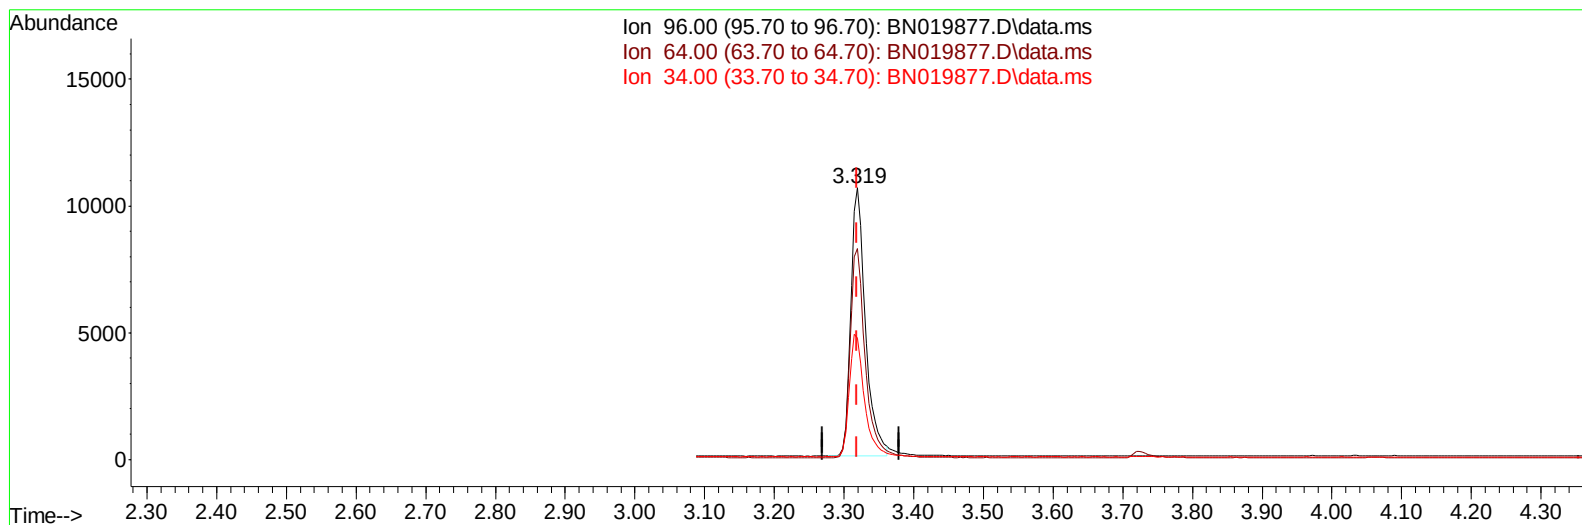

TIC: BN019877.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.319min (+ 0.000) 2.74 ng/ul

response 15385

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.69#
34.00	22.70	44.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019877.D
Acq On : 20 May 2022 20:04
Operator : CG/JU
Sample : N2843-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 21 01:54:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

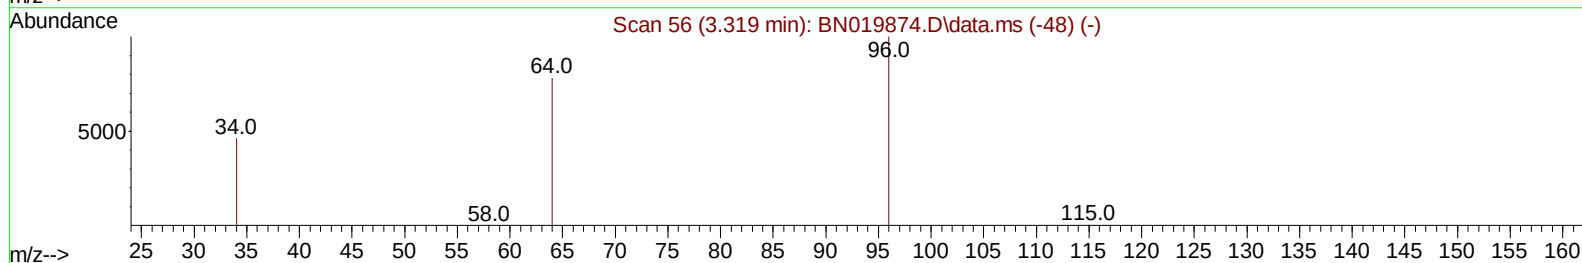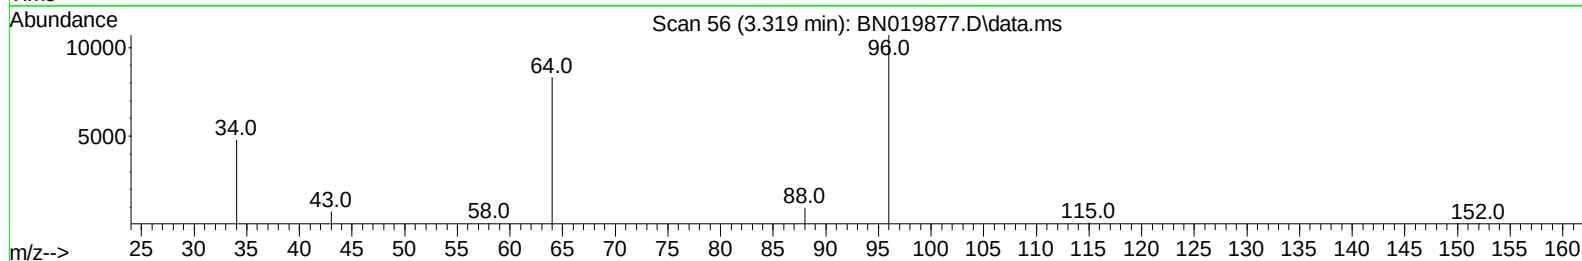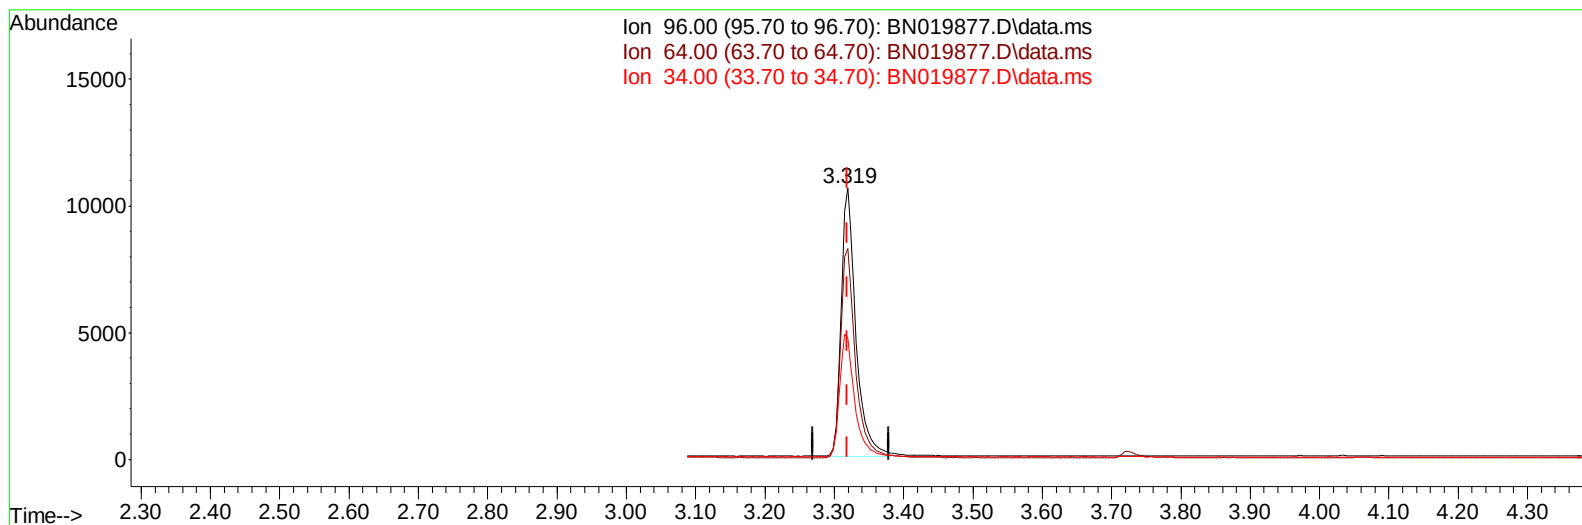

TIC: BN019877.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.319min (+ 0.000) 2.79 ng/ul m****response 15655**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	77.69#
34.00	22.70	44.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019877.D
 Acq On : 20 May 2022 20:04
 Operator : CG/JU
 Sample : N2843-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 21 01:54:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4743	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	15938	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.473	164	10553	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.212	188	19427	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.403	240	16241	0.400	ng/ul	# 0.00
23) Perylene-d12	23.744	264	13946	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	15655m	2.789	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	4990	0.207	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	11172	0.217	ng/ul	0.00
Target Compounds				Qvalue		
5) Naphthalene	10.687	128	1463	0.028	ng/ul#	78
7) 2-Methylnaphthalene	12.299	142	4922	0.157	ng/ul#	100
8) 1-Methylnaphthalene	12.519	142	4344	0.149	ng/ul#	100
12) Fluorene	15.518	166	6600	0.143	ng/ul#	58
15) Phenanthrene	17.254	178	41441	0.580	ng/ul#	83
19) Fluoranthene	19.275	202	8119	0.109	ng/ul#	66
20) Pyrene	19.637	202	13800	0.186	ng/ul#	67
22) Chrysene	21.418	228	11775	0.165	ng/ul#	14

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019877.D
Acq On : 20 May 2022 20:04
Operator : CG/JU
Sample : N2843-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 21 01:54:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

