
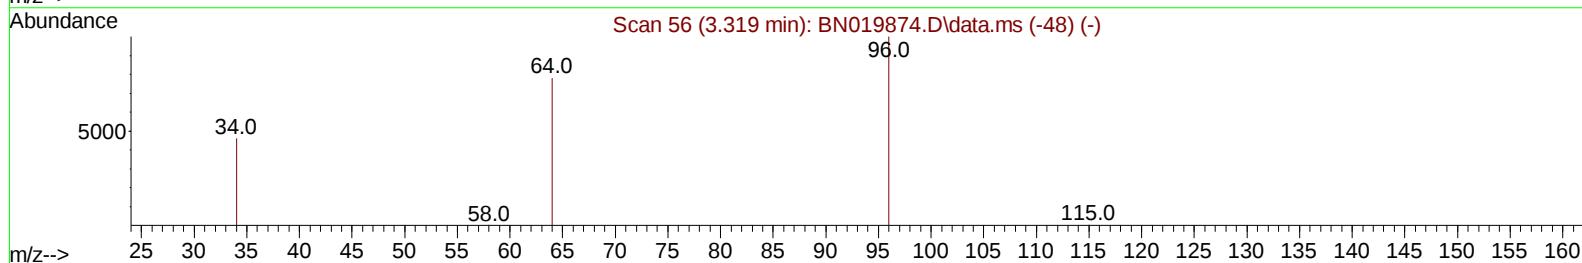
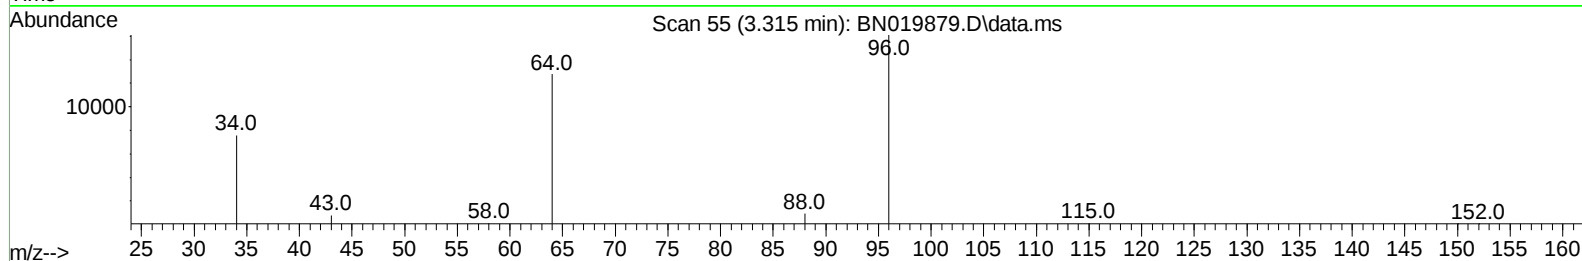


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019879.D
Acq On : 20 May 2022 21:16
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

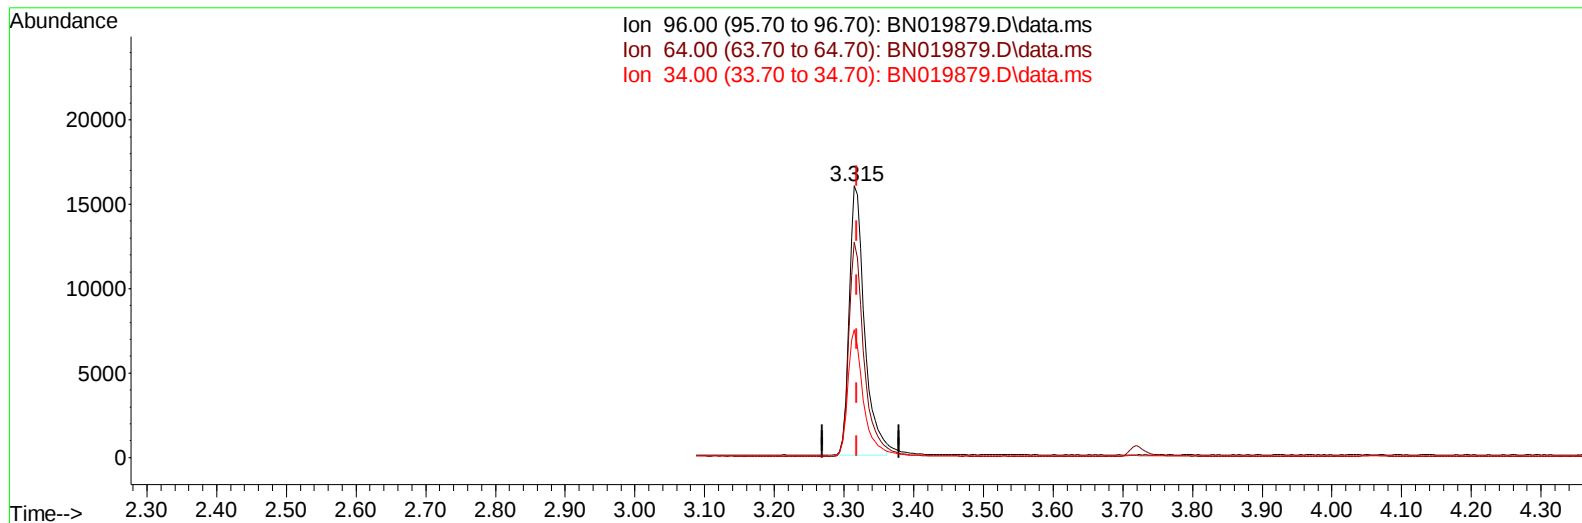

TIC: BN019879.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 5.89 ng/u1

response 24190

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.35#
34.00	22.70	47.07#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019879.D
Acq On : 20 May 2022 21:16
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

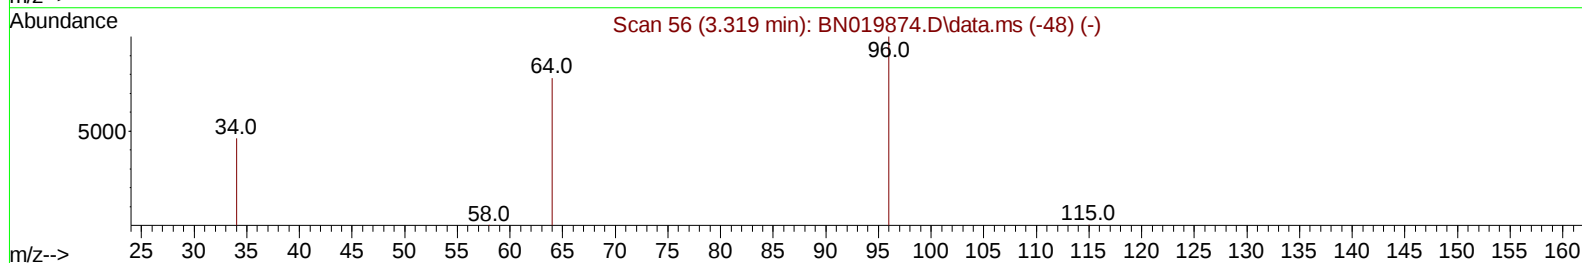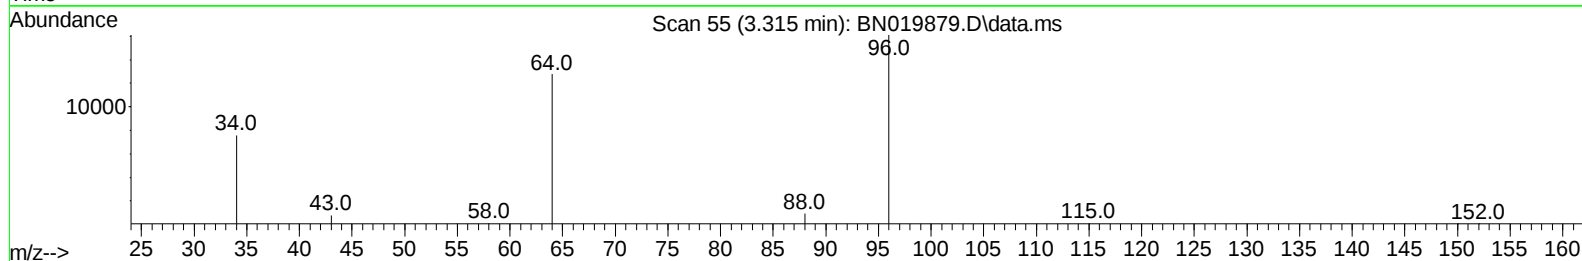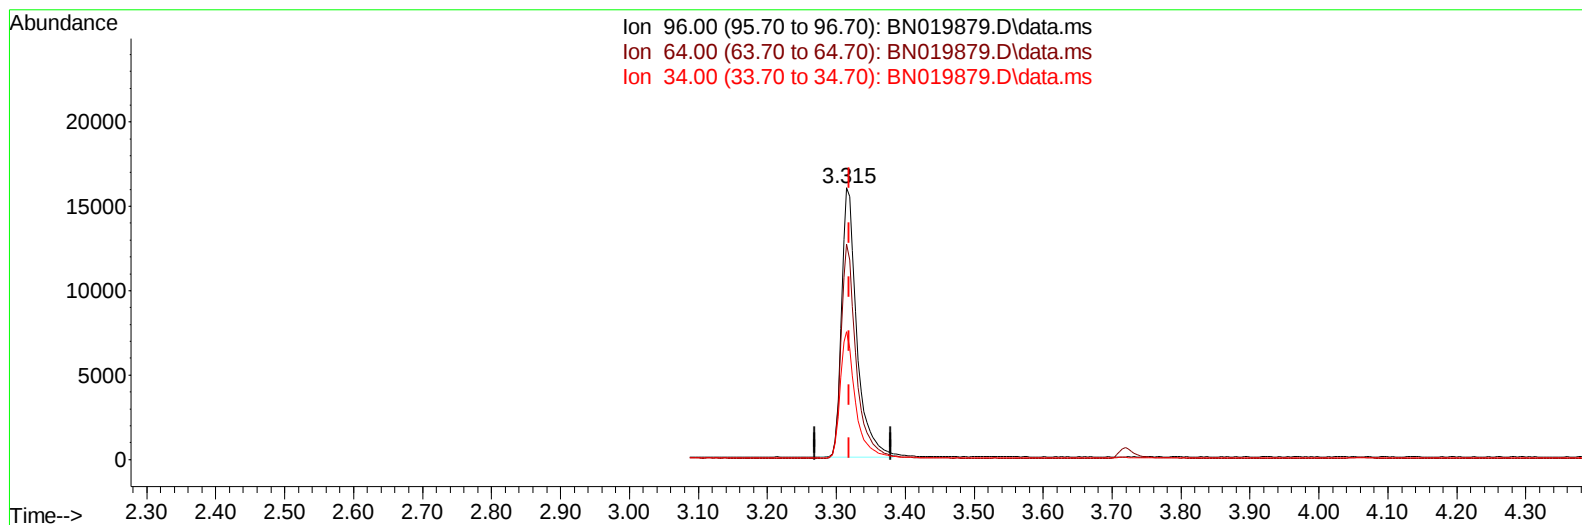

TIC: BN019879.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 6.03 ng/ul m

response 24784

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.35#
34.00	22.70	47.07#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019879.D
Acq On : 20 May 2022 21:16
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

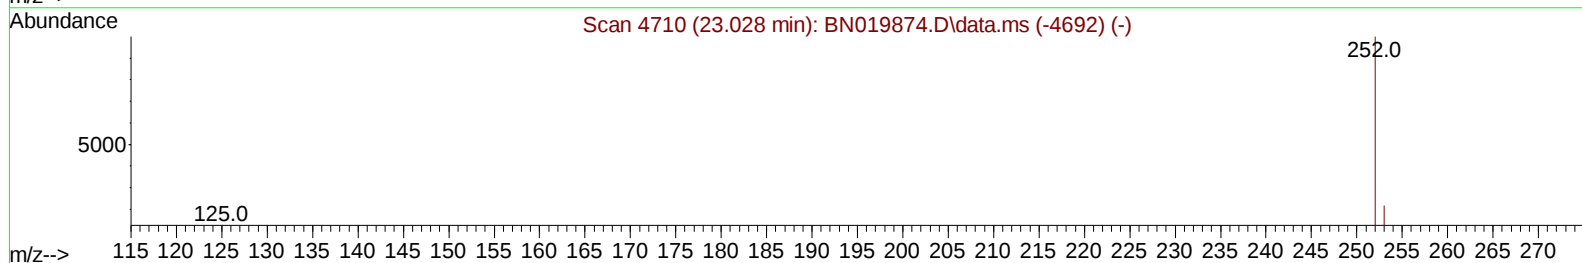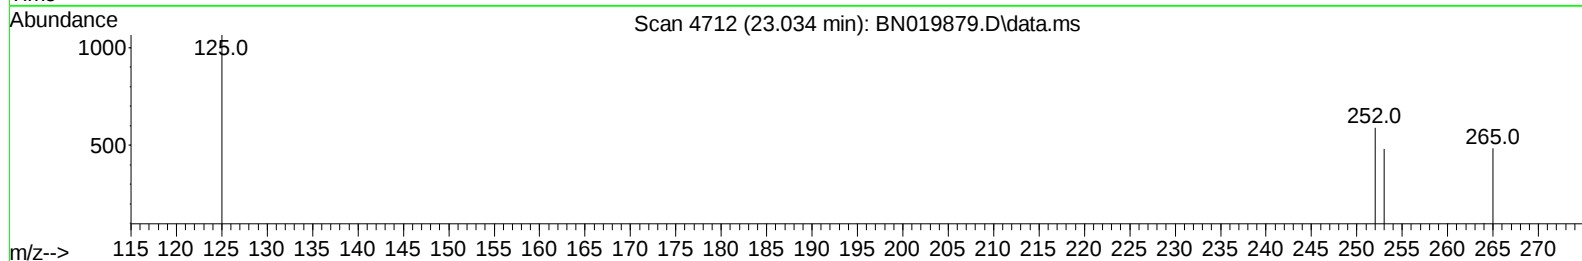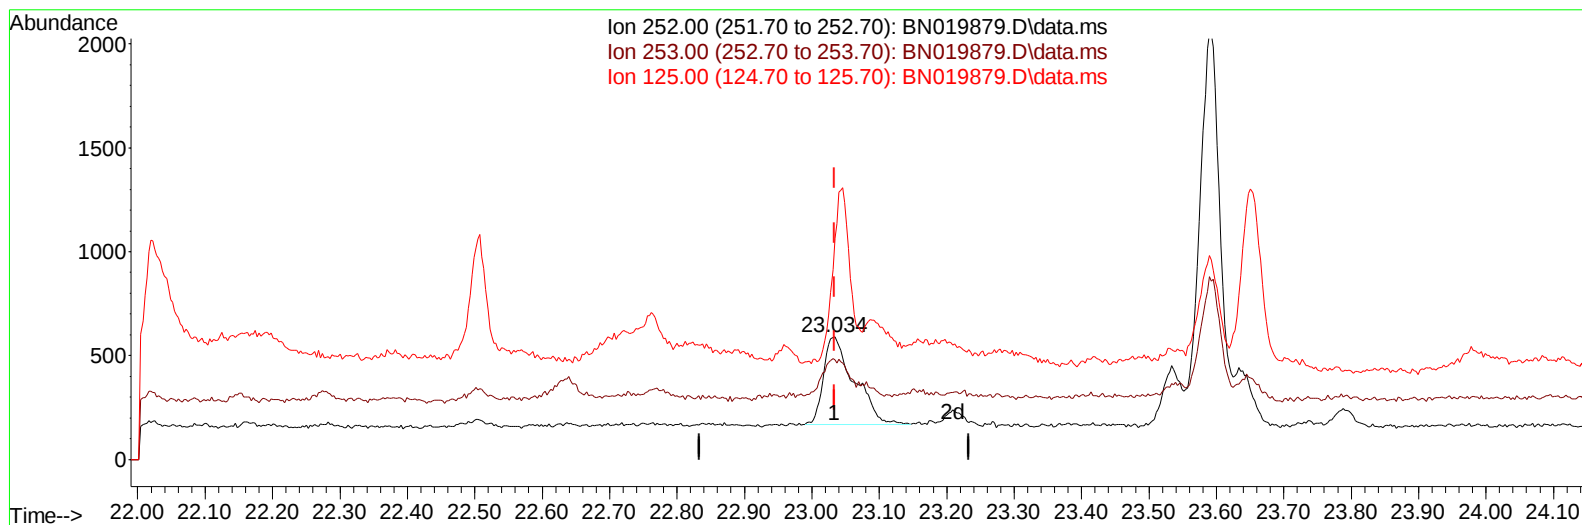

TIC: BN019879.D\data.ms

(24) Benzo(b)fluoranthene




23.034min (+ 0.000) 0.02 ng/u1

response 1343

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.00	81.36#
125.00	20.10	180.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019879.D
 Acq On : 20 May 2022 21:16
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

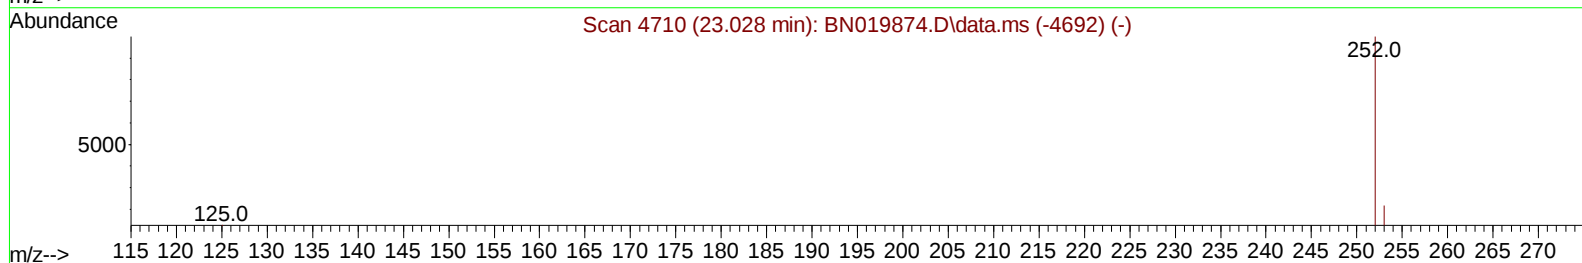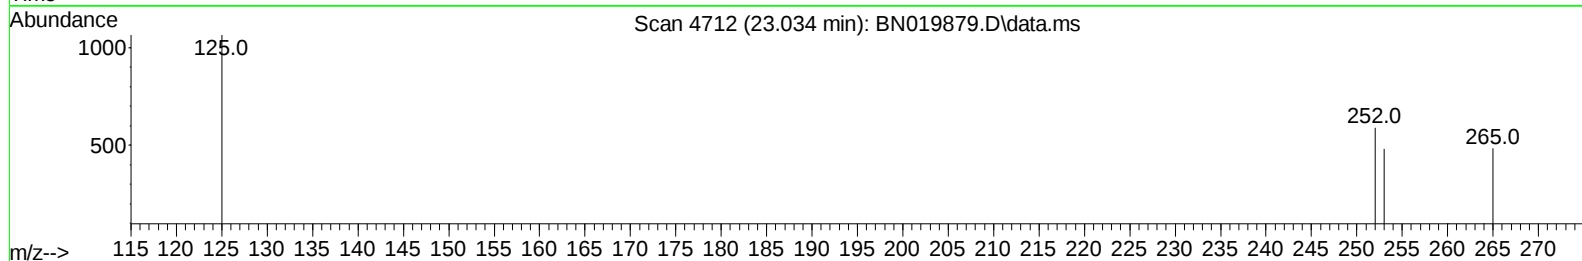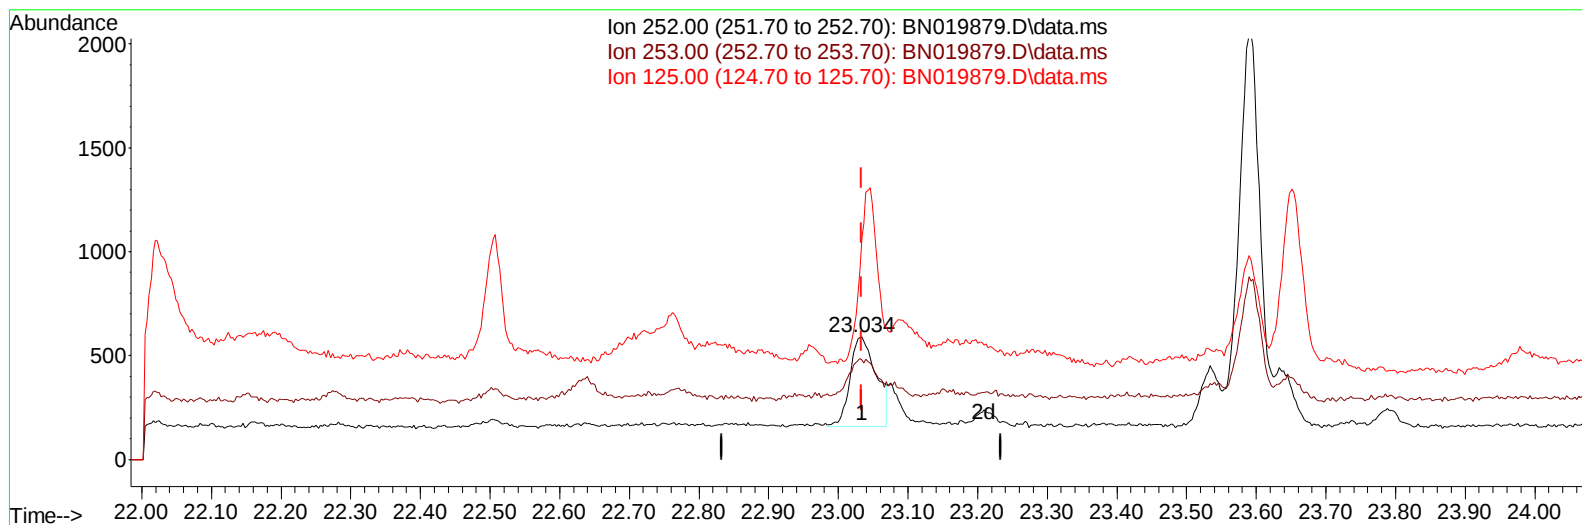

TIC: BN019879.D\data.ms

(24) Benzo(b)fluoranthene

23.034min (+ 0.000) 0.02 ng/ul m

response 1132

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.00	81.36#
125.00	20.10	180.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019879.D
 Acq On : 20 May 2022 21:16
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3471	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	12102	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	7702	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.212	188	16720	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	15161	0.400	ng/ul	0.00
23) Perylene-d12	23.736	264	12954	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	24784m	6.033	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	7161	0.391	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	16735	0.349	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.687	128	910	0.023	ng/ul#	79
7) 2-Methylnaphthalene	12.304	142	538	0.023	ng/ul#	100
8) 1-Methylnaphthalene	12.519	142	513	0.023	ng/ul#	100
15) Phenanthrene	17.254	178	1321	0.021	ng/ul#	85
19) Fluoranthene	19.270	202	1476	0.021	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019879.D
Acq On : 20 May 2022 21:16
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: May 21 01:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

