
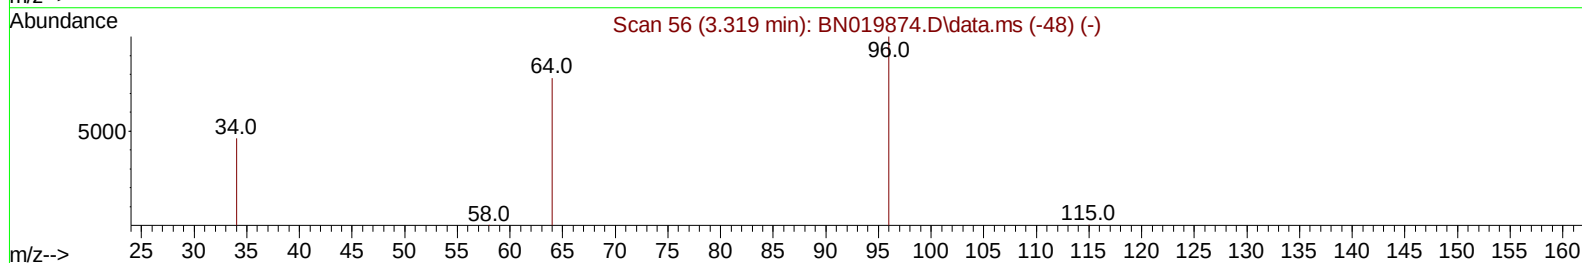
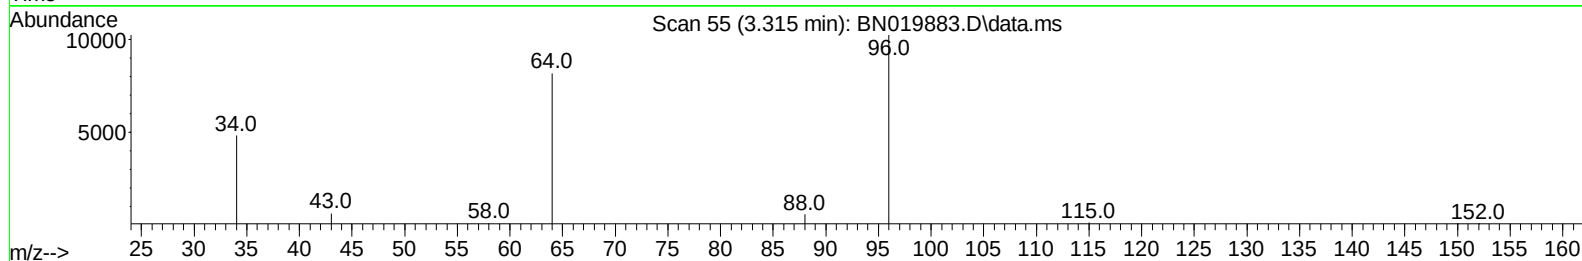


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019883.D
Acq On : 20 May 2022 23:39
Operator : CG/JU
Sample : N2843-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 21 01:54:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

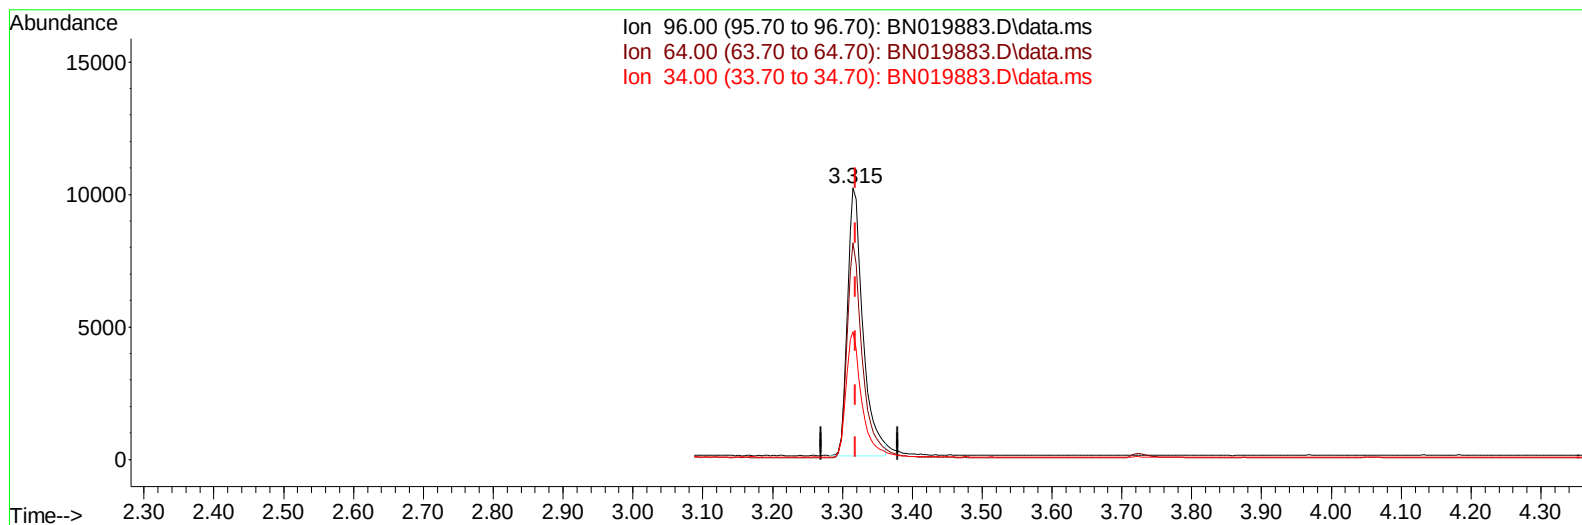

TIC: BN019883.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.315min (-0.004) 3.67 ng/u1

response 15503

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.79#
34.00	22.70	46.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019883.D
Acq On : 20 May 2022 23:39
Operator : CG/JU
Sample : N2843-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 21 01:54:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

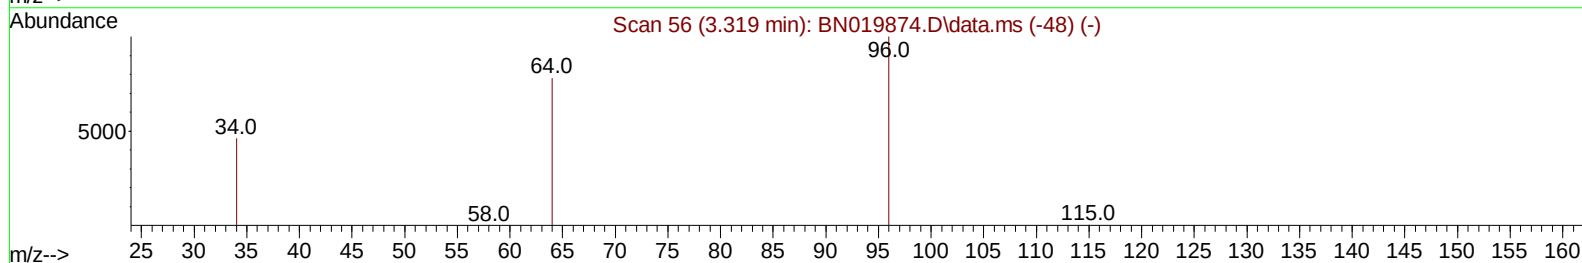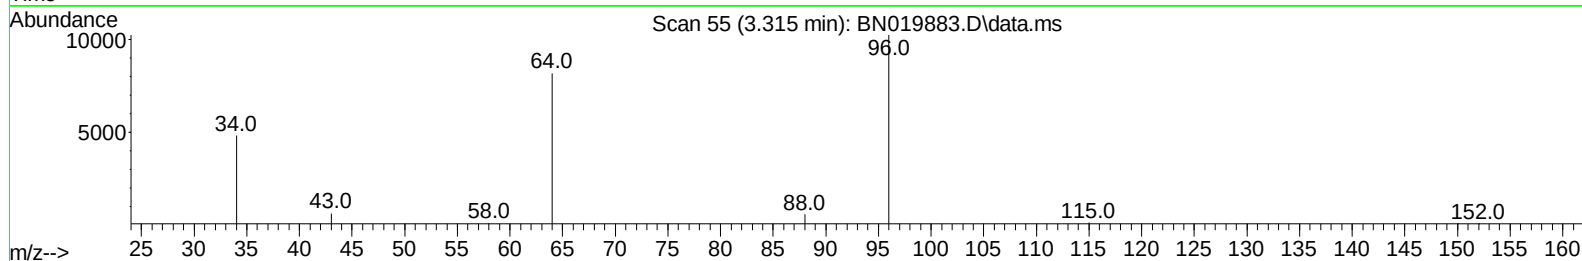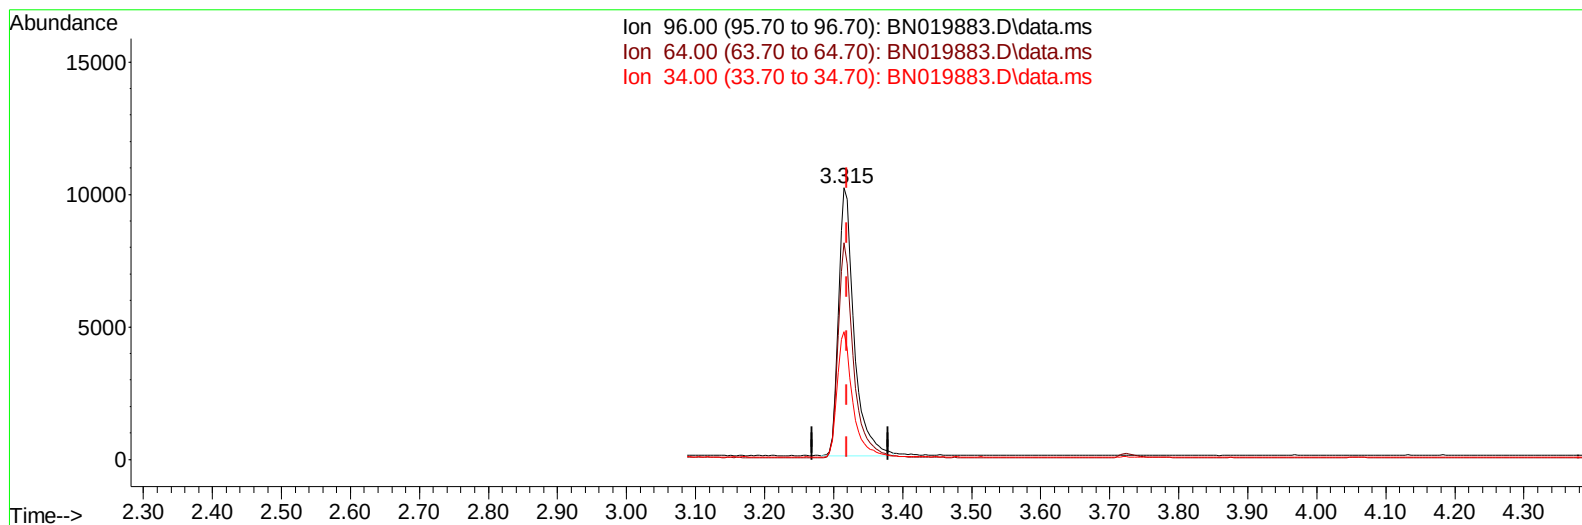

TIC: BN019883.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.315min (-0.004) 3.75 ng/ul m****response 15873**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	79.79#
34.00	22.70	46.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019883.D
 Acq On : 20 May 2022 23:39
 Operator : CG/JU
 Sample : N2843-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 21 01:54:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3574	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	12293	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	7784	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.209	188	17177	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	15476	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	13155	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	15873m	3.753	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	4835	0.260	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	12383	0.253	ng/ul	0.00
Target Compounds						Qvalue
15) Phenanthrene	17.251	178	2706	0.043	ng/ul#	86
20) Pyrene	19.634	202	3351	0.047	ng/ul#	84
22) Chrysene	21.432	228	3947	0.058	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019883.D
Acq On : 20 May 2022 23:39
Operator : CG/JU
Sample : N2843-22
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 21 01:54:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

