
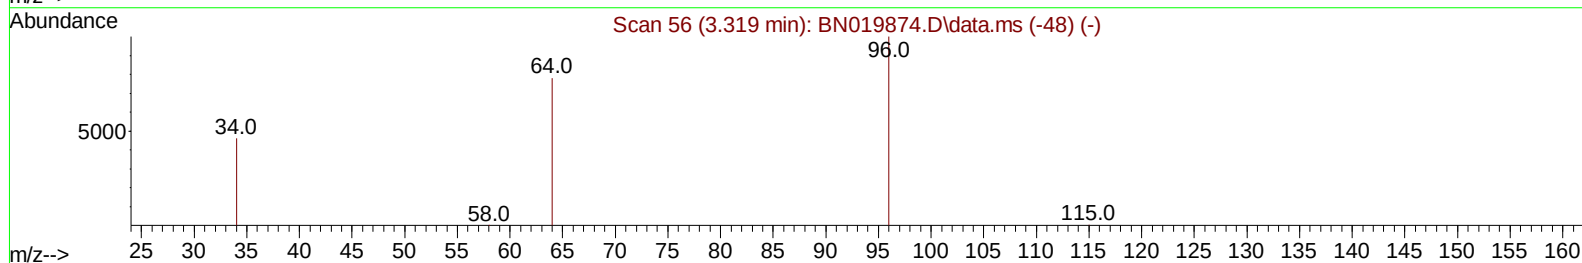
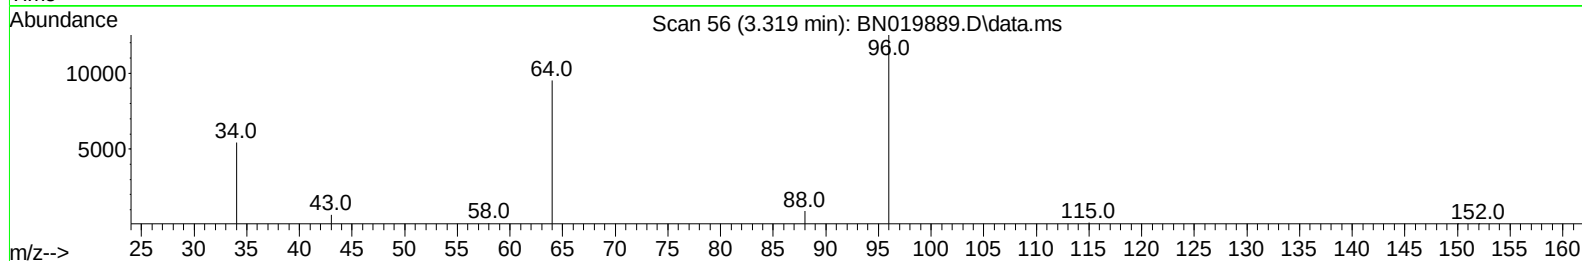


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019889.D
Acq On : 21 May 2022 03:14
Operator : CG/JU
Sample : N2843-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: May 21 04:02:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

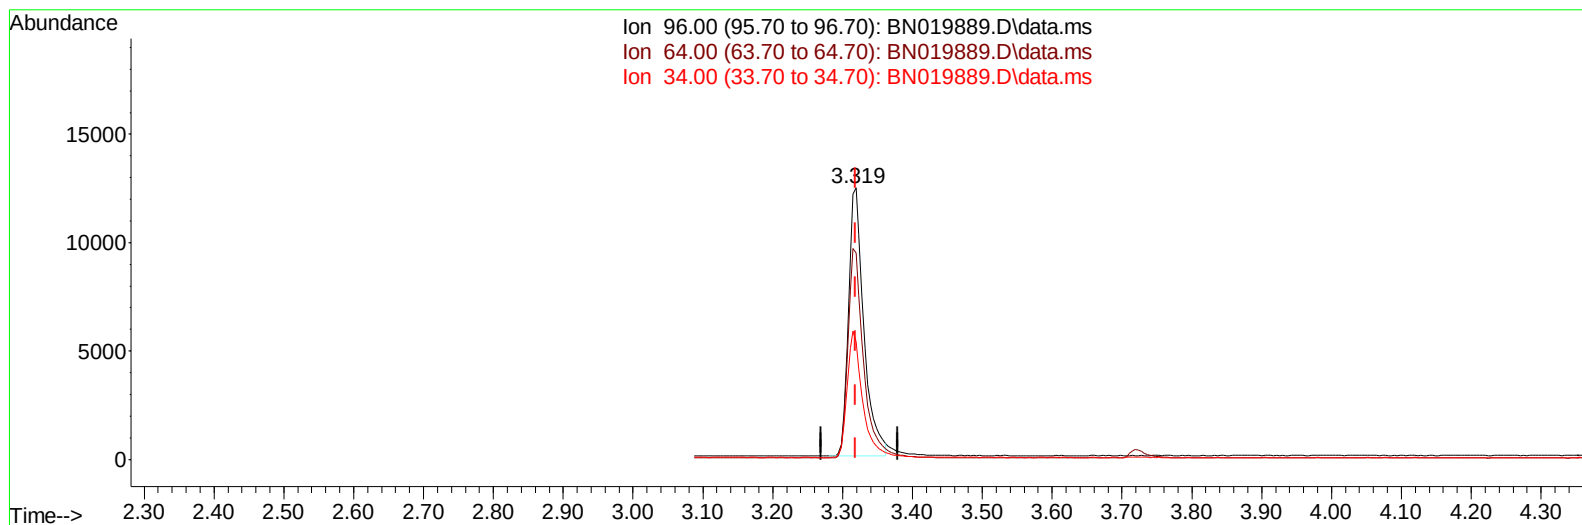




TIC: BN019889.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.319min (-0.000) 4.14 ng/uI****response 18807**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.05#
34.00	22.70	43.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019889.D
Acq On : 21 May 2022 03:14
Operator : CG/JU
Sample : N2843-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: May 21 04:02:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

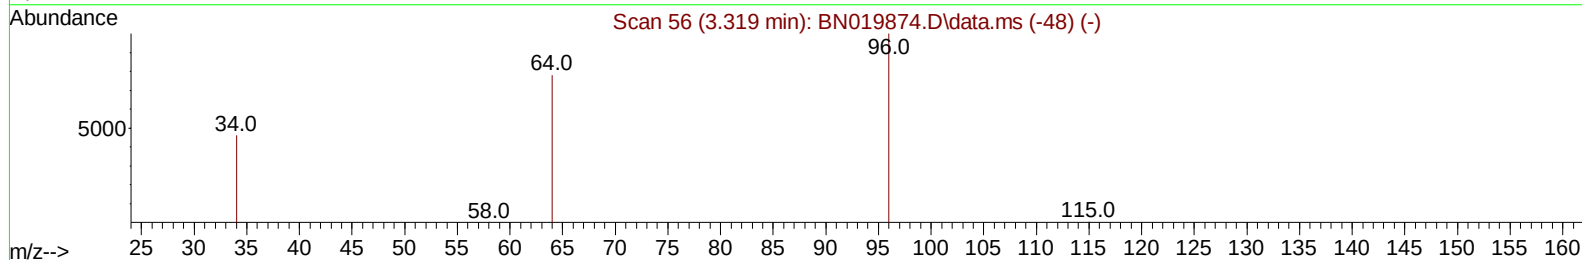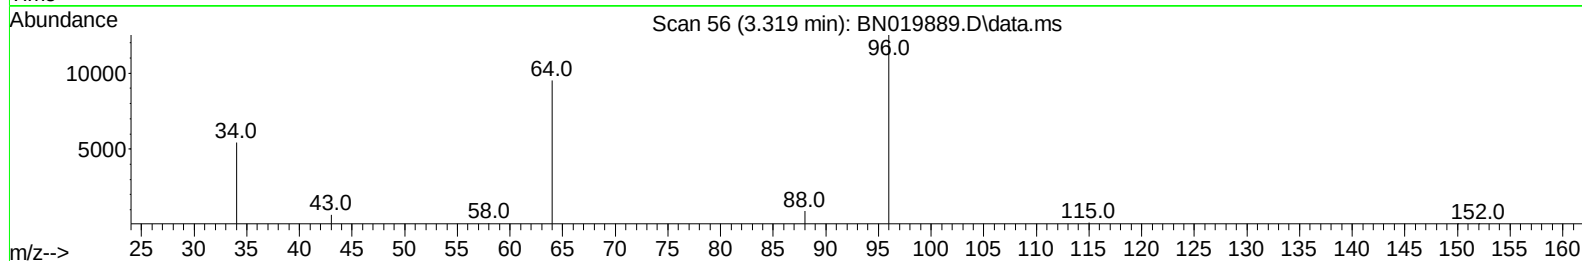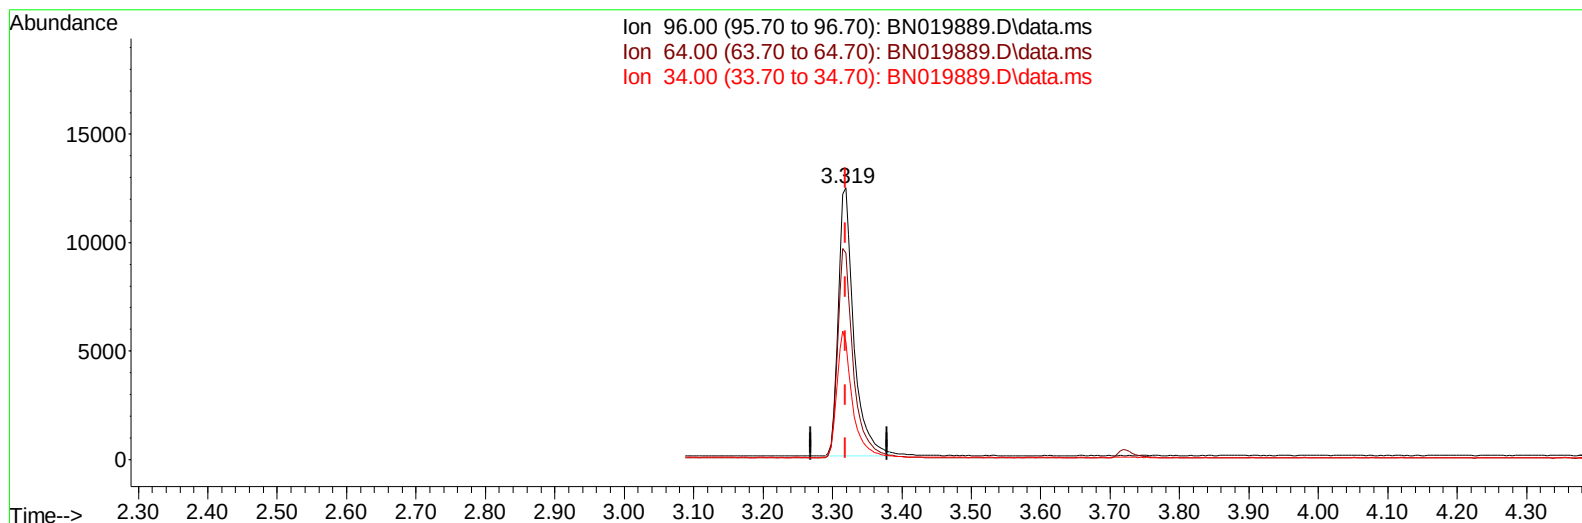

TIC: BN019889.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 4.24 ng/ul m

response 19266

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.05#
34.00	22.70	43.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019889.D
 Acq On : 21 May 2022 03:14
 Operator : CG/JU
 Sample : N2843-17
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: May 21 04:02:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	3843	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	13297	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	8334	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	18200	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	16590	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	14057	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	19266m	4.236	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	5780	0.287	ng/ul	0.00
18) Fluoranthene-d10	19.237	212	13487	0.257	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019889.D
Acq On : 21 May 2022 03:14
Operator : CG/JU
Sample : N2843-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: May 21 04:02:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

