
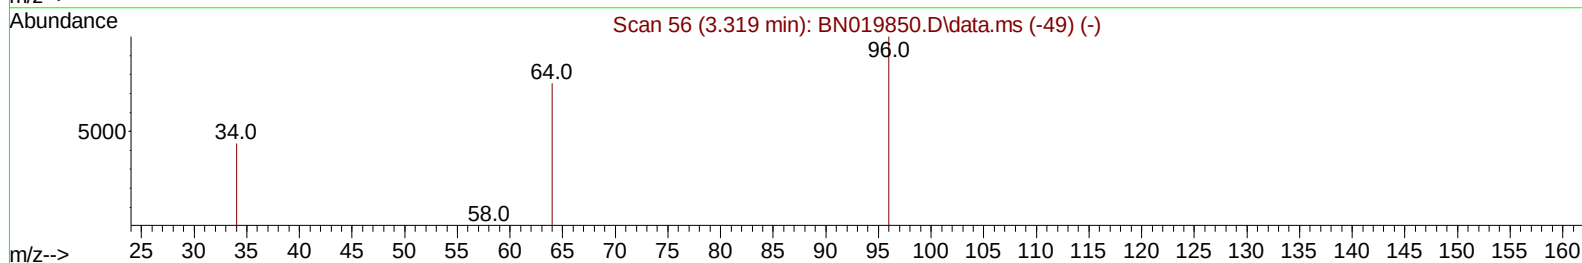
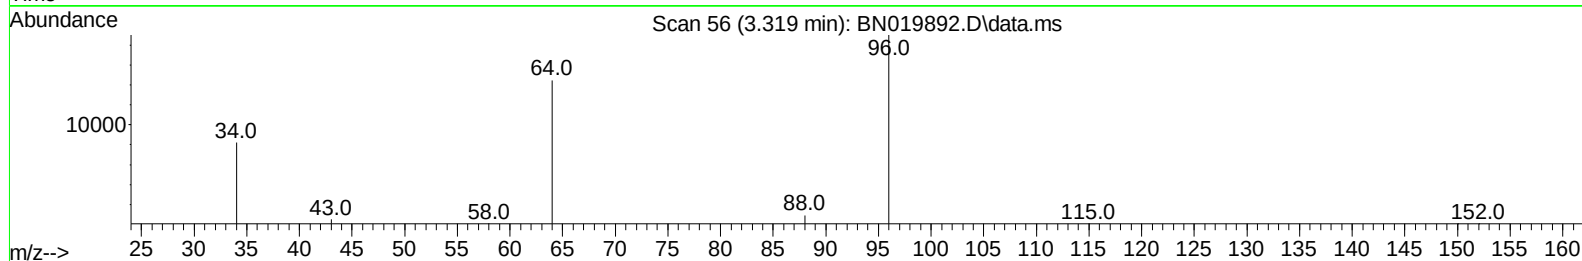


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019892.D
Acq On : 21 May 2022 05:37
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: May 21 06:34:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

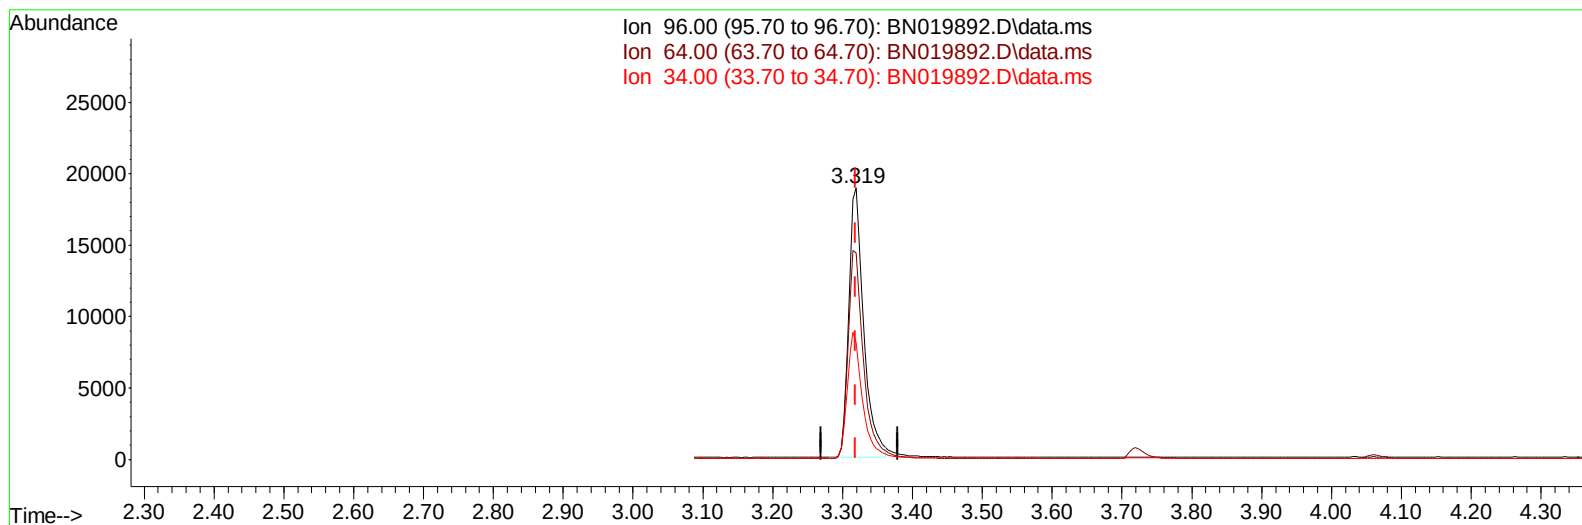

TIC: BN019892.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.319min (-0.000) 5.24 ng/u1

response 28042

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.11#
34.00	22.70	43.11#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019892.D
Acq On : 21 May 2022 05:37
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: May 21 06:34:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

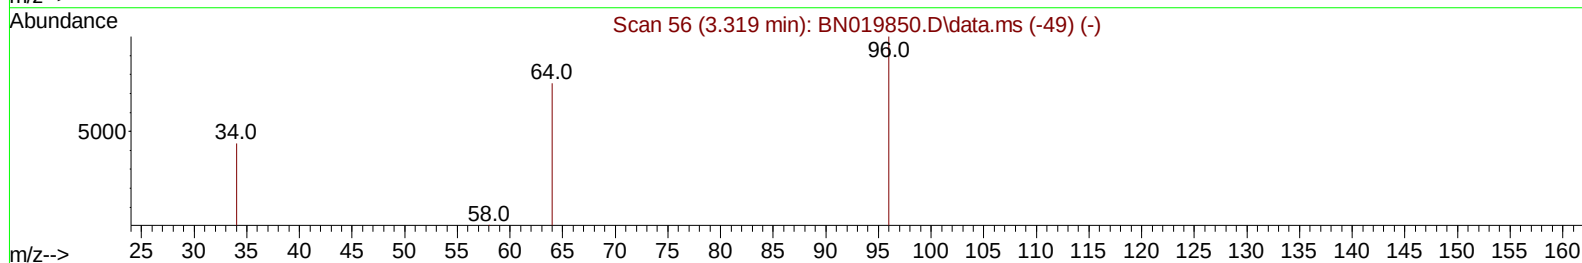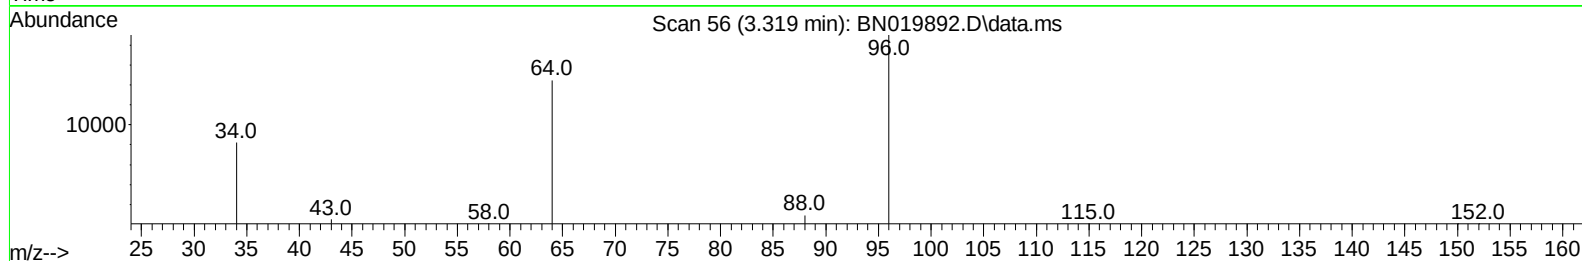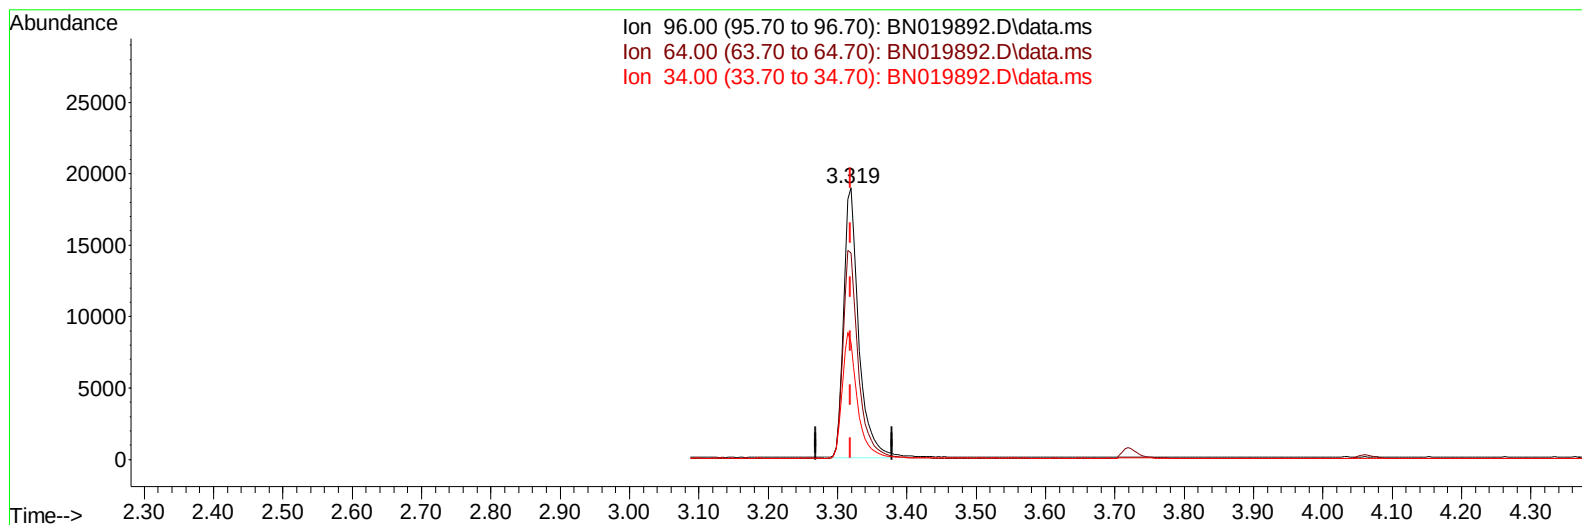

TIC: BN019892.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.319min (-0.000) 5.33 ng/ul m****response 28528**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.11#
34.00	22.70	43.11#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019892.D
 Acq On : 21 May 2022 05:37
 Operator : CG/JU
 Sample : PB144915BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Quant Time: May 21 06:34:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4522	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	15434	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	9795	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	21053	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	17588	0.400	ng/ul	0.00
23) Perylene-d12	23.737	264	15617	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	28528m	5.331	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	8009	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	18905	0.340	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019892.D
Acq On : 21 May 2022 05:37
Operator : CG/JU
Sample : PB144915BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: May 21 06:34:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

