
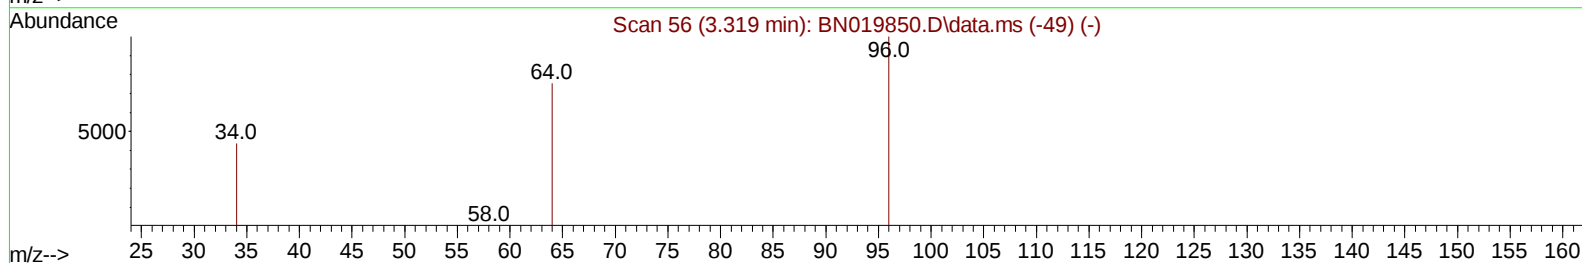
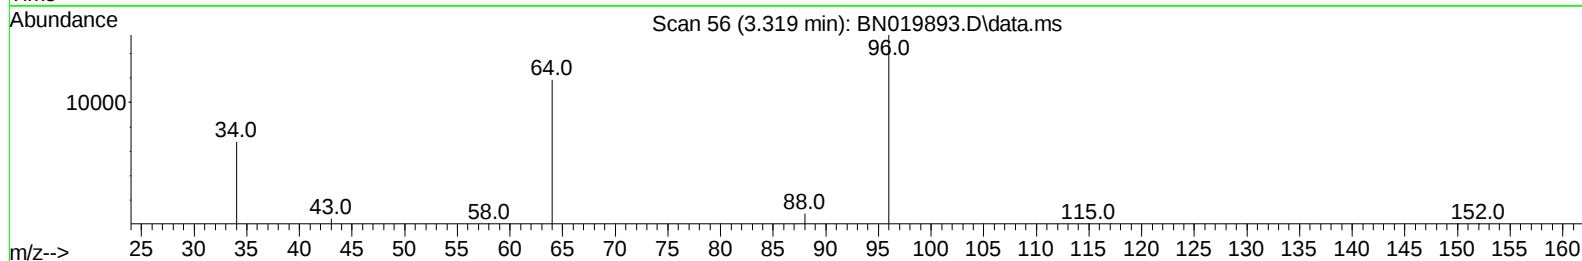


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019893.D
Acq On : 21 May 2022 06:13
Operator : CG/JU
Sample : PB144975BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 21 06:54:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

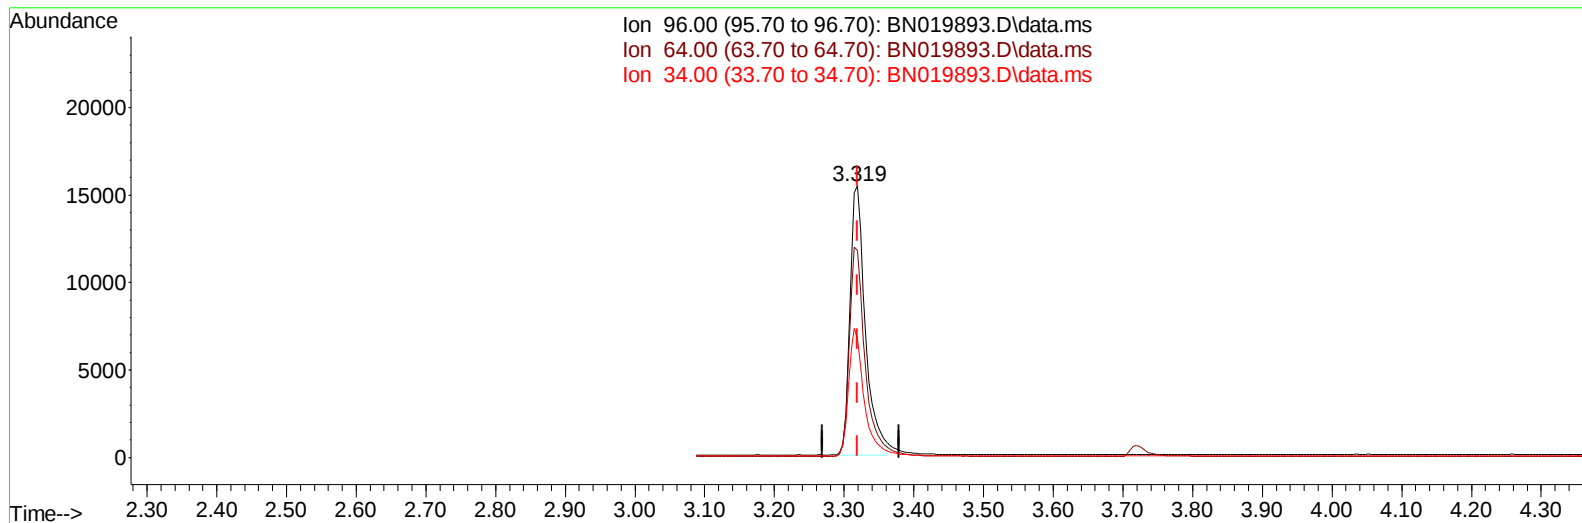

TIC: BN019893.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.319min (-0.000) 4.85 ng/u1

response 23460

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.22#
34.00	22.70	43.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019893.D
Acq On : 21 May 2022 06:13
Operator : CG/JU
Sample : PB144975BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 21 06:54:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

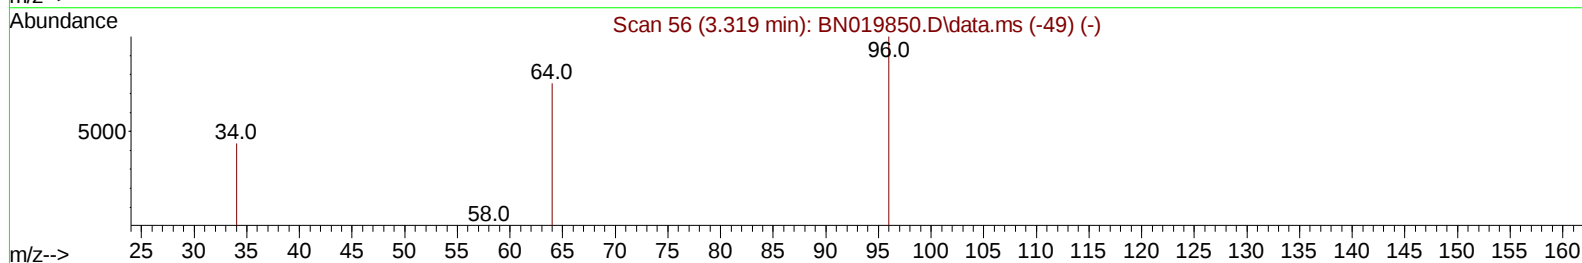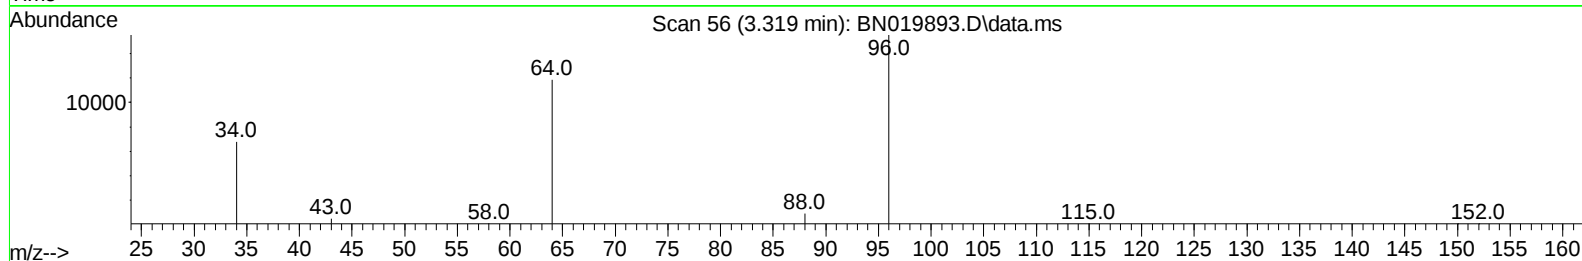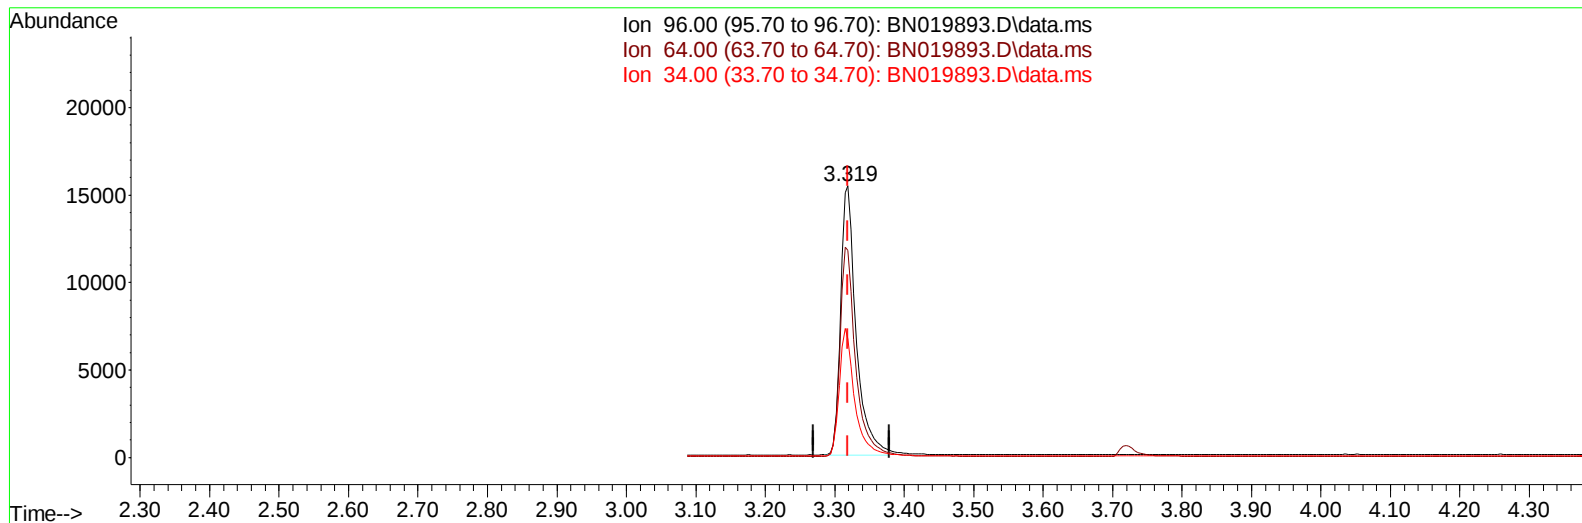

TIC: BN019893.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 4.95 ng/ul m

response 23940

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.22#
34.00	22.70	43.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019893.D
 Acq On : 21 May 2022 06:13
 Operator : CG/JU
 Sample : PB144975BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 21 06:54:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	4083	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	13846	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	8833	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.208	188	19075	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	16552	0.400	ng/ul	0.00
23) Perylene-d12	23.737	264	15099	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	23940m	4.954	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	6667	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	16634	0.318	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019893.D
Acq On : 21 May 2022 06:13
Operator : CG/JU
Sample : PB144975BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 21 06:54:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

