
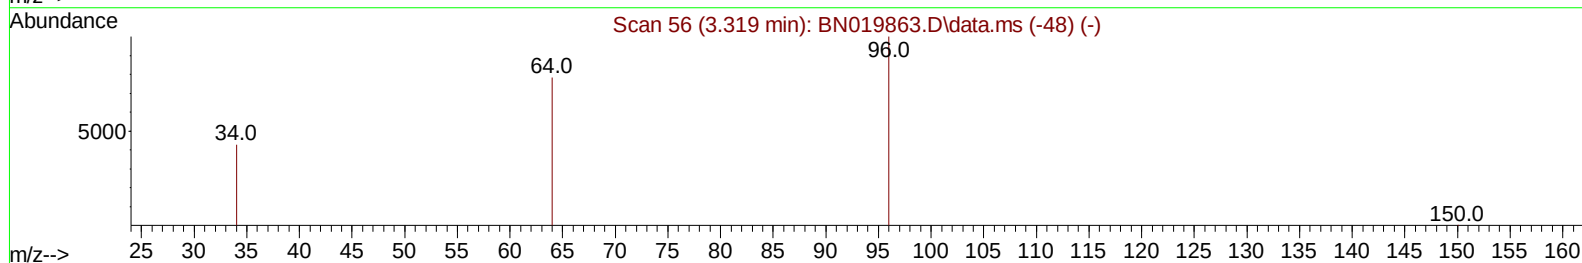
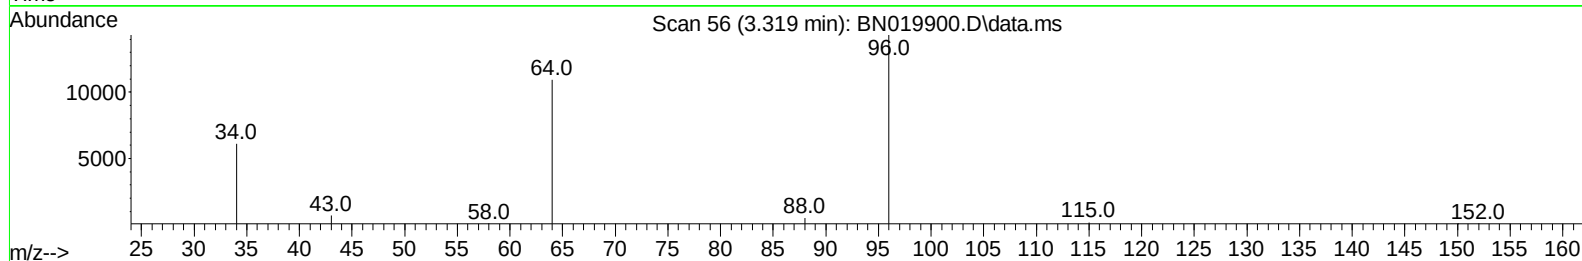


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019900.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: May 23 09:34:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

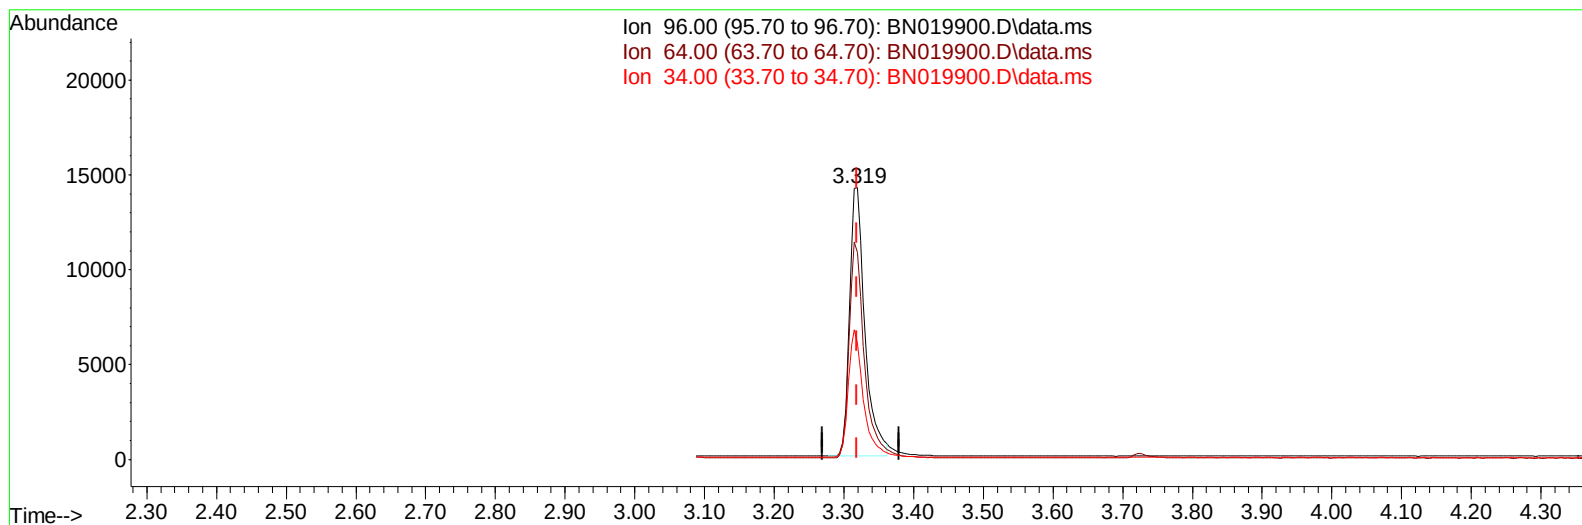




TIC: BN019900.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.319min (+ 0.000) 4.06 ng/ul****response 21574**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.30#
34.00	22.70	42.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019900.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: May 23 09:34:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

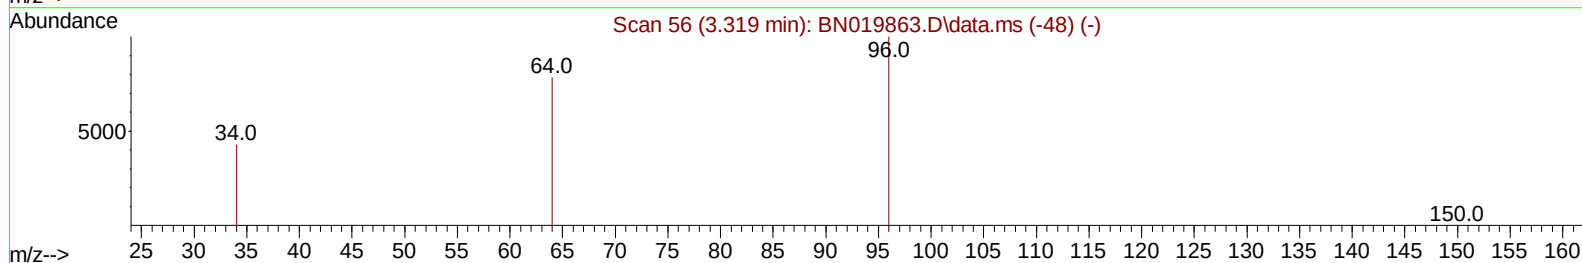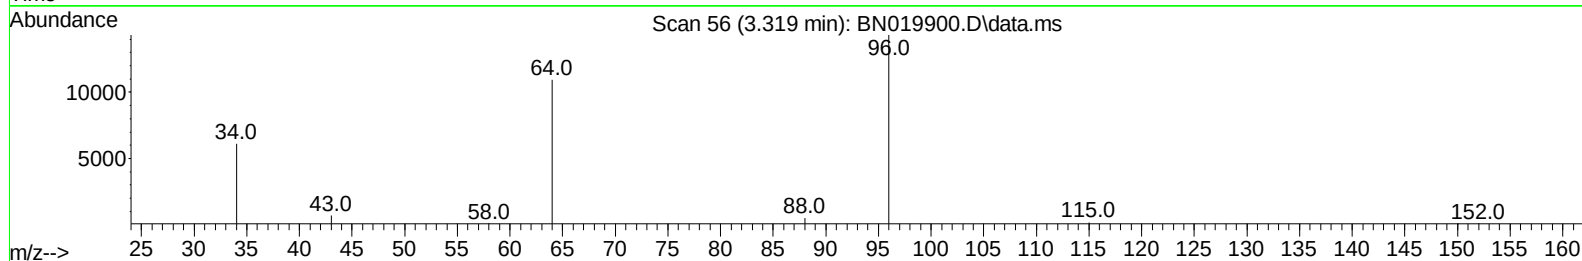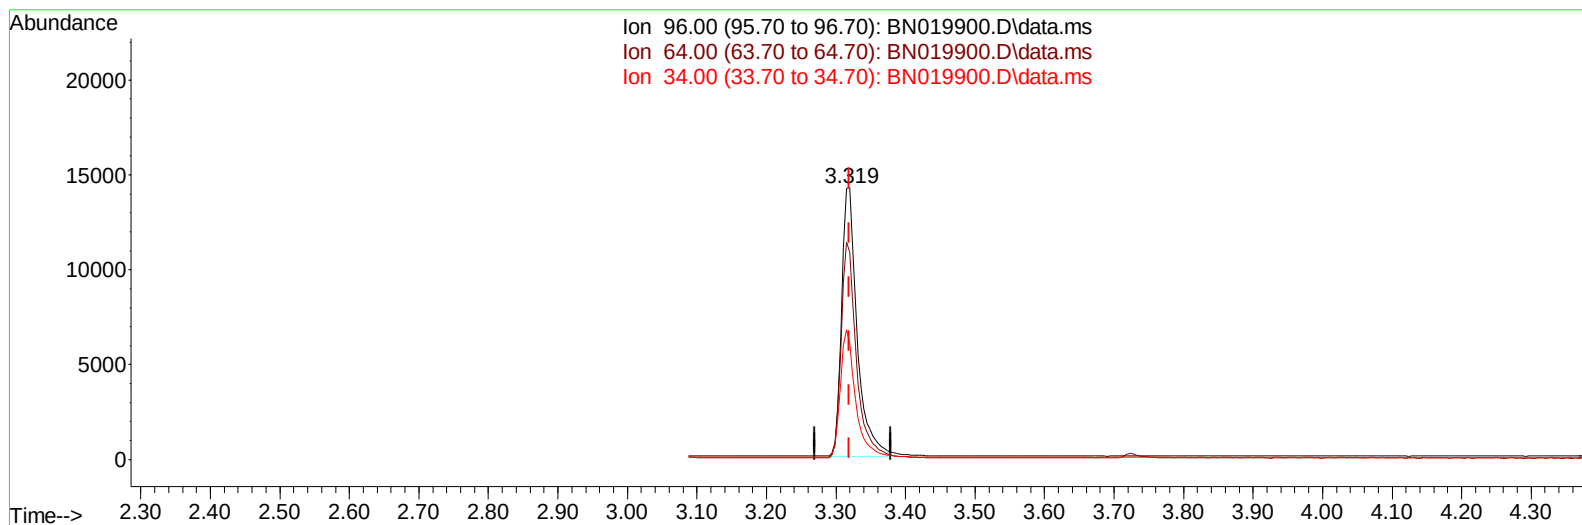

TIC: BN019900.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 4.13 ng/ul m

response 21946

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.30#
34.00	22.70	42.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019900.D
 Acq On : 21 May 2022 10:23
 Operator : CG/JU
 Sample : N2918-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Quant Time: May 23 09:34:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4488	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	14985	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	8966	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188	18917	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	15048	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264	11680	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	21946m	4.132	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	9074	0.400	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	21887	0.460	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.689	128	1105	0.023	ng/ul#	80
14) Pentachlorophenol	16.871	266	2406	0.591	ng/ul	90
16) Anthracene	17.348	178	2526	0.044	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019900.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: May 23 09:34:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

