
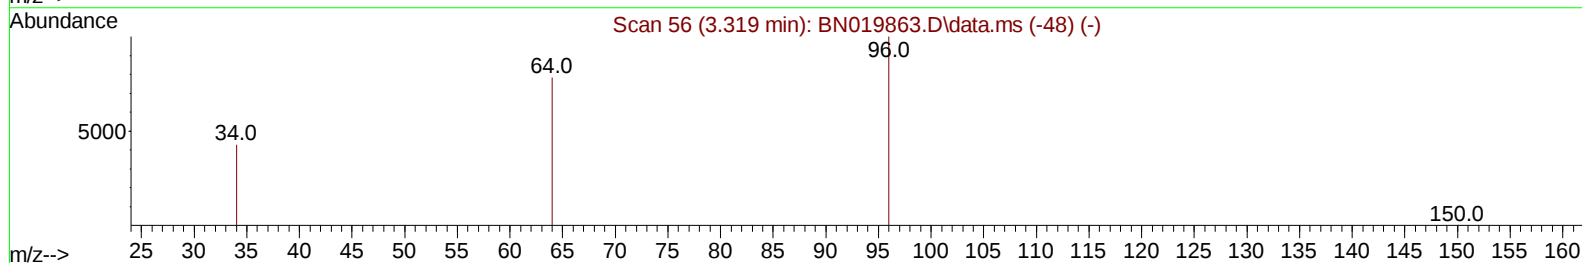
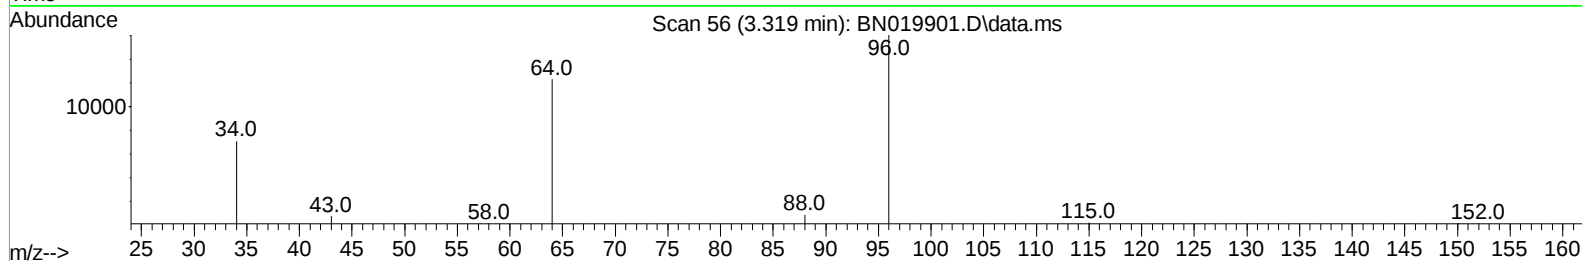


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019901.D
Acq On : 21 May 2022 10:59
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 23 09:35:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

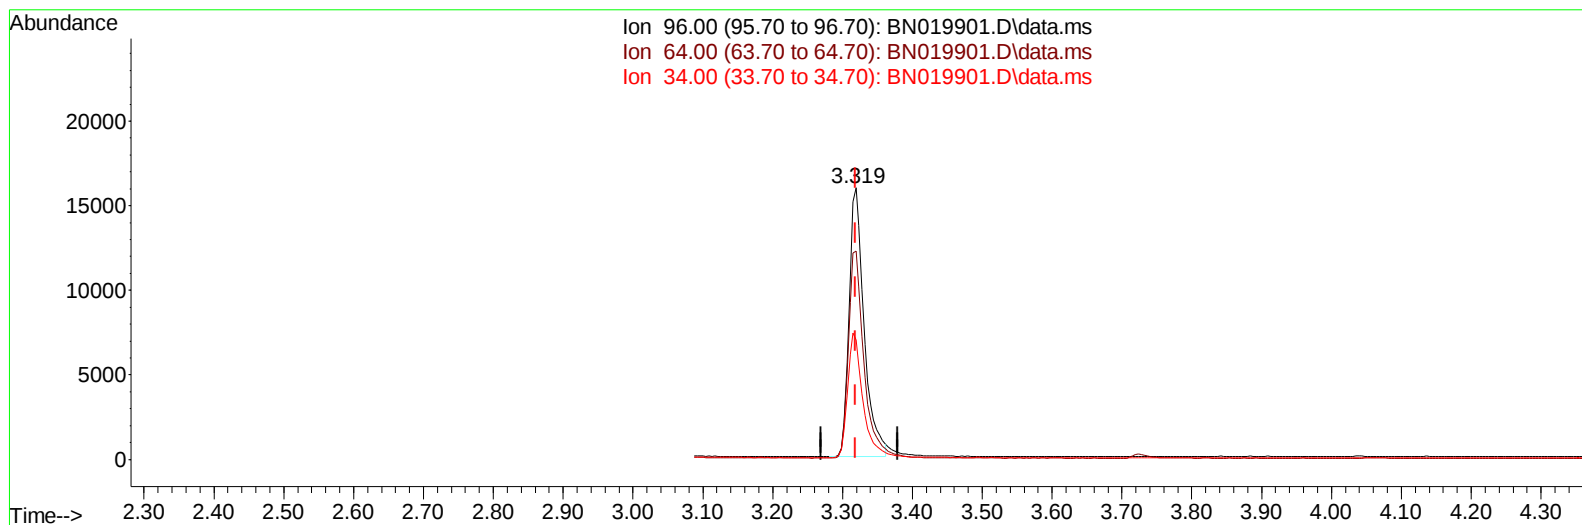

TIC: BN019901.D\data.ms

(3) 1,4-Dioxane-d8 (S)




3.319min (-0.000) 4.35 ng/u1

response 23728

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.70#
34.00	22.70	44.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019901.D
Acq On : 21 May 2022 10:59
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 23 09:35:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

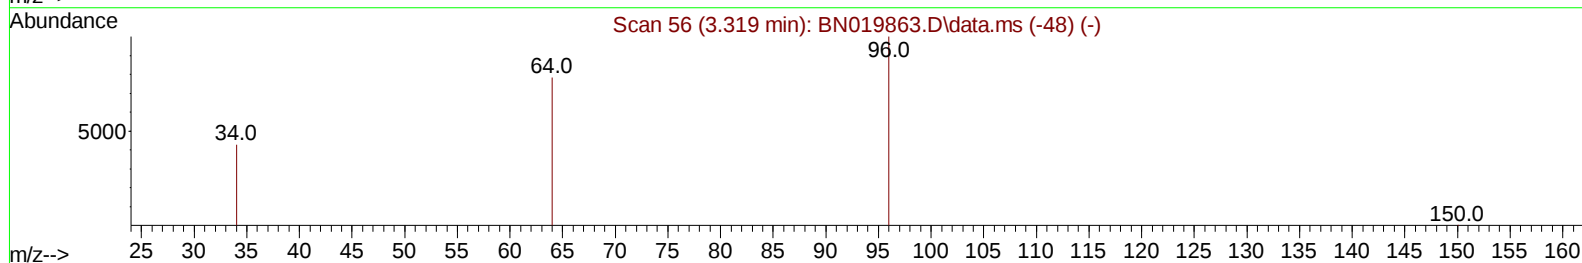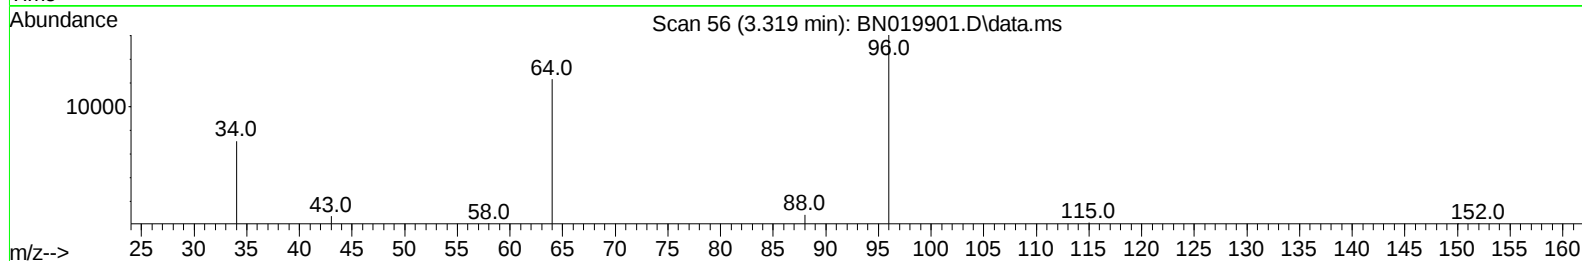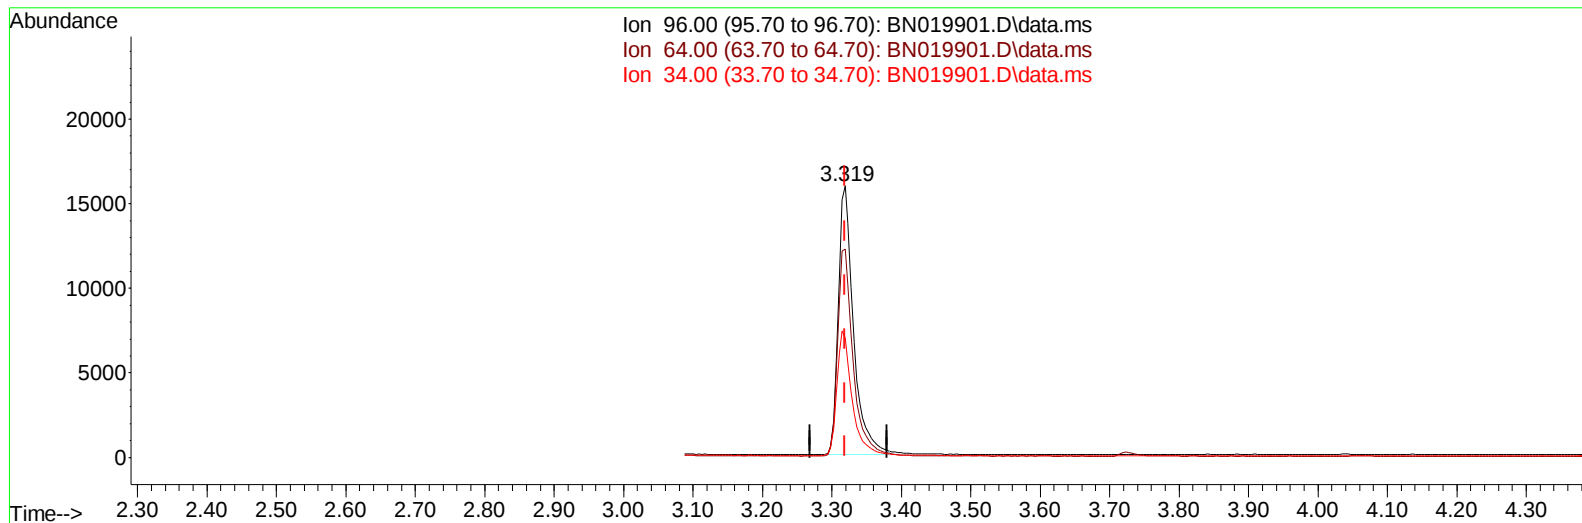

TIC: BN019901.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.000) 4.44 ng/ul m

response 24190

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.70#
34.00	22.70	44.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019901.D
 Acq On : 21 May 2022 10:59
 Operator : CG/JU
 Sample : N2918-21
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 23 09:35:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4607	0.400	ng/ul	0.00
4) Naphthalene-d8	10.643	136	15353	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.477	164	9427	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.216	188	19649	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	15514	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264	12135	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	24190m	4.437	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	10564	0.455	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	24646	0.502	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.693	128	1697	0.034	ng/ul#	78
12) Fluorene	15.523	166	31152	0.758	ng/ul	100
14) Pentachlorophenol	16.874	266	2917	0.690	ng/ul	90
16) Anthracene	17.347	178	1867	0.032	ng/ul#	84
19) Fluoranthene	19.274	202	2003	0.028	ng/ul#	84
20) Pyrene	19.637	202	3784	0.053	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019901.D
Acq On : 21 May 2022 10:59
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: May 23 09:35:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

