
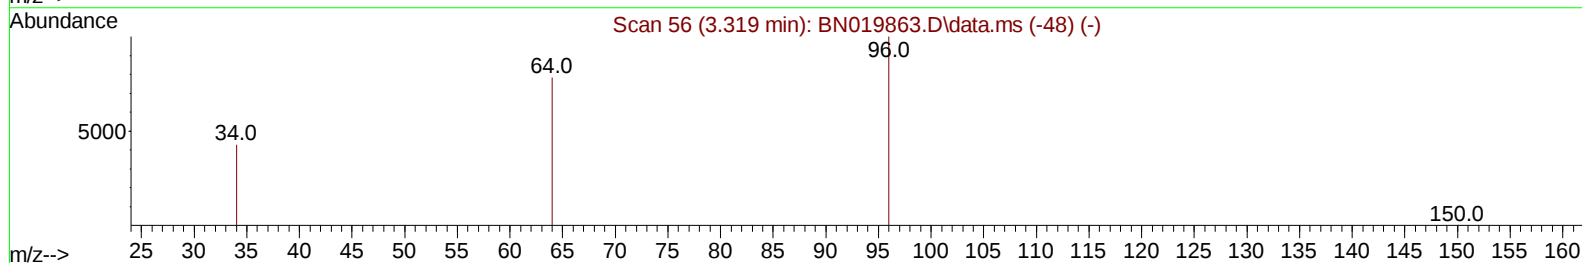
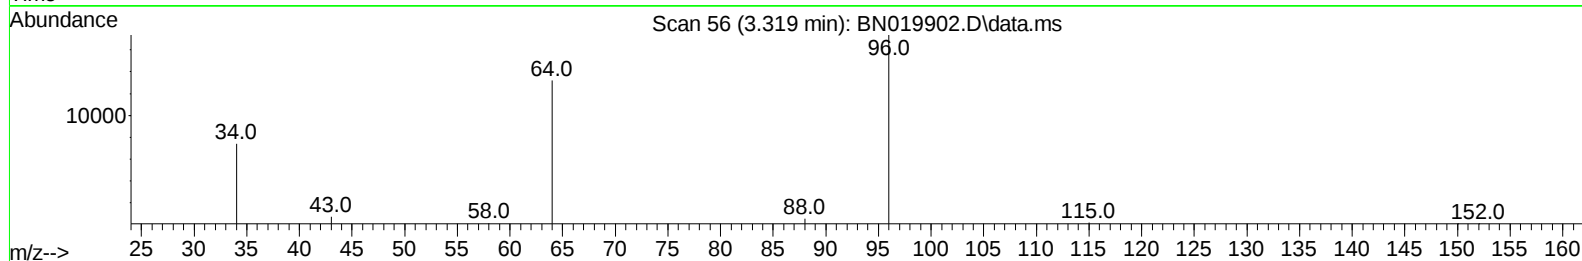


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019902.D
Acq On : 21 May 2022 11:35
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: May 23 09:37:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

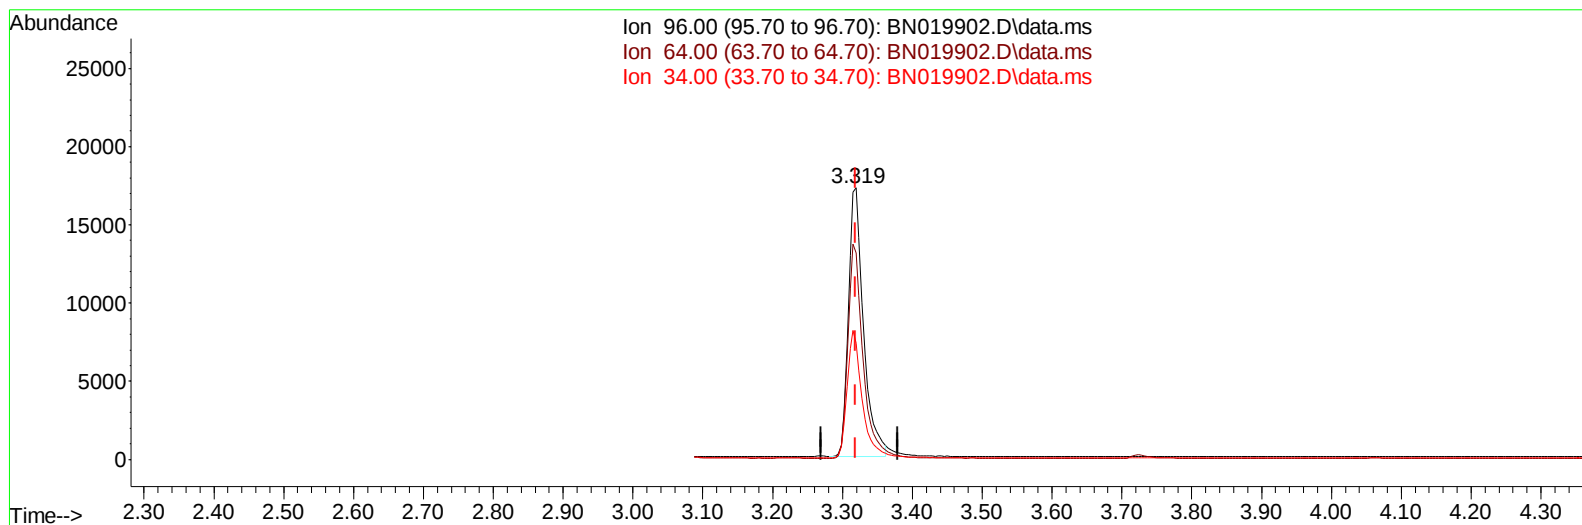




TIC: BN019902.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.319min (+ 0.000) 4.70 ng/u1****response 25711**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.98#
34.00	22.70	42.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019902.D
Acq On : 21 May 2022 11:35
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: May 23 09:37:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

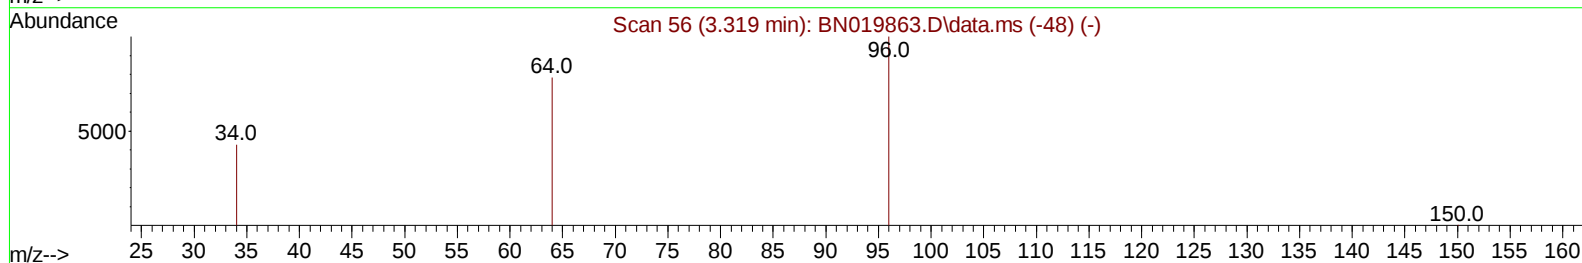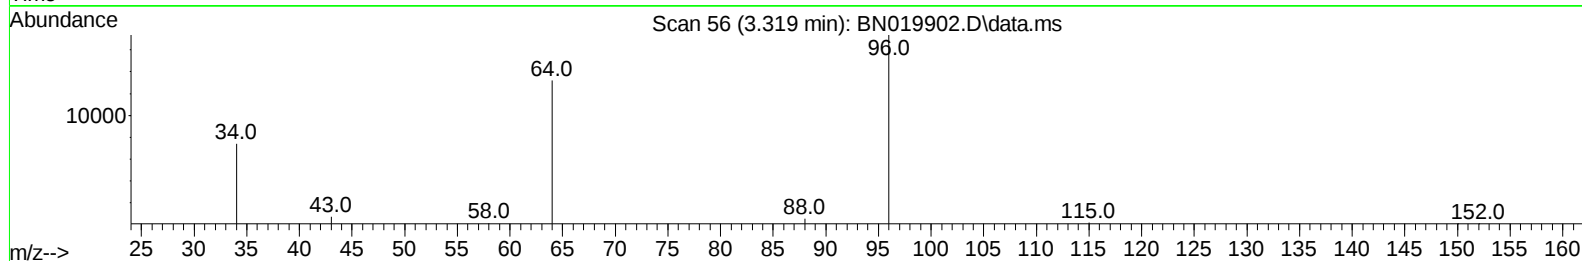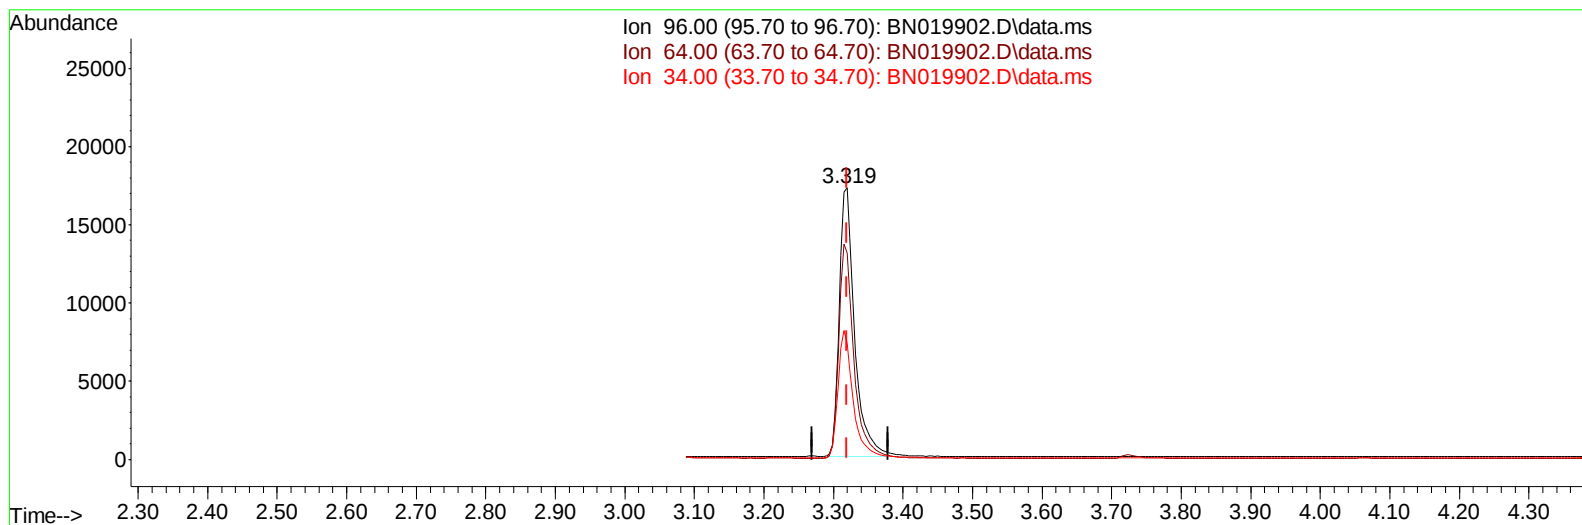

TIC: BN019902.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (+ 0.000) 4.79 ng/ul m

response 26219

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	75.98#
34.00	22.70	42.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019902.D
 Acq On : 21 May 2022 11:35
 Operator : CG/JU
 Sample : N2918-22
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Quant Time: May 23 09:37:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4627	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	15371	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.474	164	9598	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	19634	0.400	ng/ul	0.00
17) Chrysene-d12	21.406	240	15182	0.400	ng/ul	0.00
23) Perylene-d12	23.747	264	11616	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	26219m	4.788	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	10789	0.464	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	24064	0.501	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.689	128	386202	7.760	ng/ul	98
7) 2-Methylnaphthalene	12.306	142	17360	0.573	ng/ul#	100
8) 1-Methylnaphthalene	12.520	142	12205	0.435	ng/ul#	100
10) Acenaphthylene	14.197	152	5013	0.106	ng/ul#	89
11) Acenaphthene	14.539	153	17721	0.464	ng/ul	100
12) Fluorene	15.524	166	32904	0.786	ng/ul	99
14) Pentachlorophenol	16.871	266	9910	2.346	ng/ul	90
15) Phenanthrene	17.255	178	99485	1.377	ng/ul	99
16) Anthracene	17.348	178	5668	0.096	ng/ul	96
19) Fluoranthene	19.272	202	10386	0.149	ng/ul	97
20) Pyrene	19.639	202	4936	0.071	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019902.D
Acq On : 21 May 2022 11:35
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: May 23 09:37:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

