
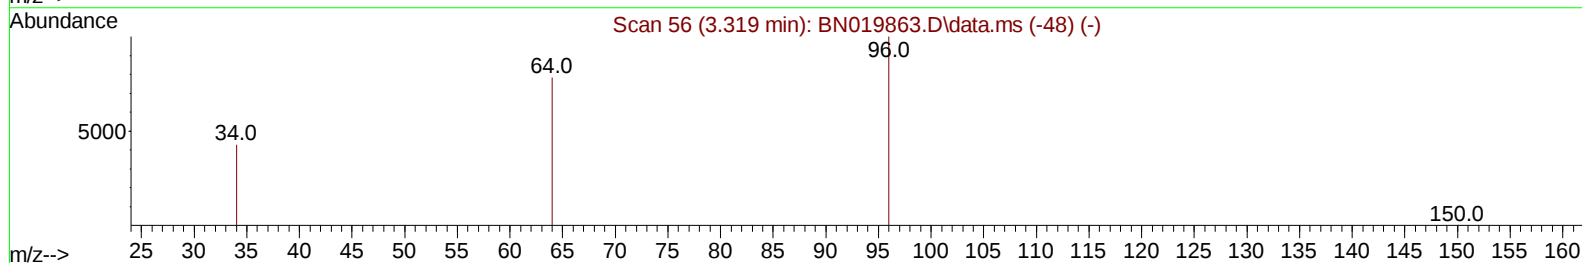
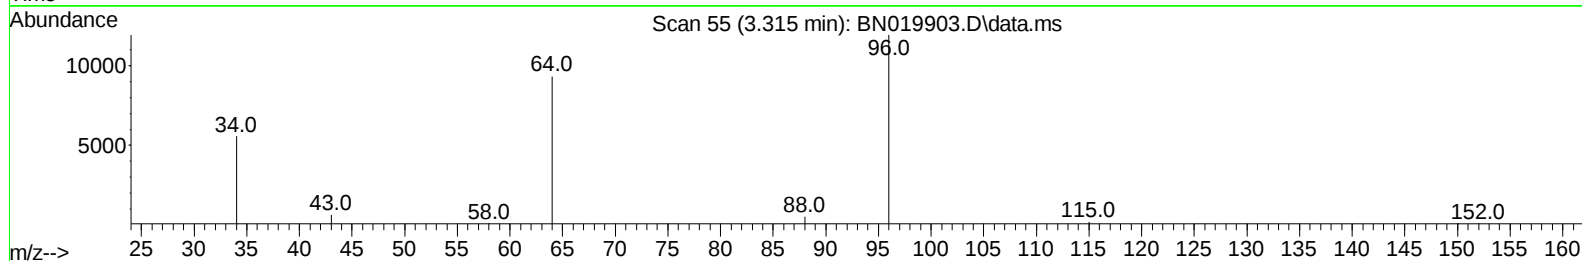


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019903.D
Acq On : 21 May 2022 12:11
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: May 23 09:38:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

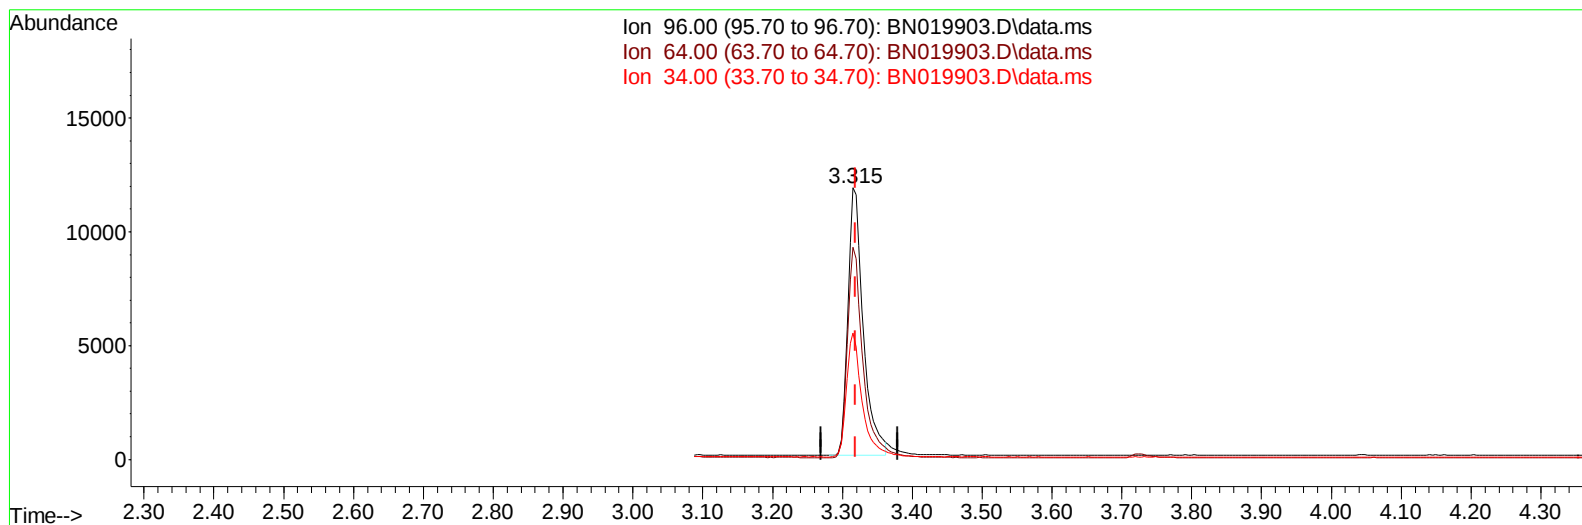




TIC: BN019903.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.315min (-0.004) 3.71 ng/u1****response 17908**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	78.18#
34.00	22.70	46.64#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019903.D
Acq On : 21 May 2022 12:11
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: May 23 09:38:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

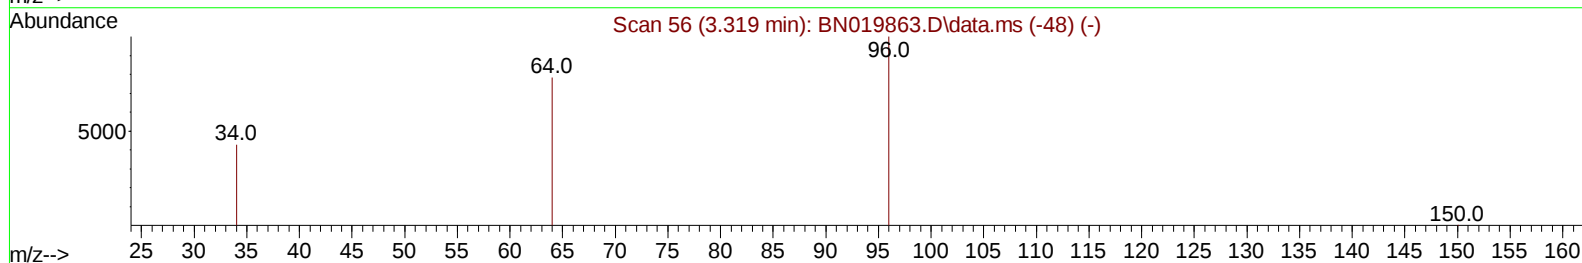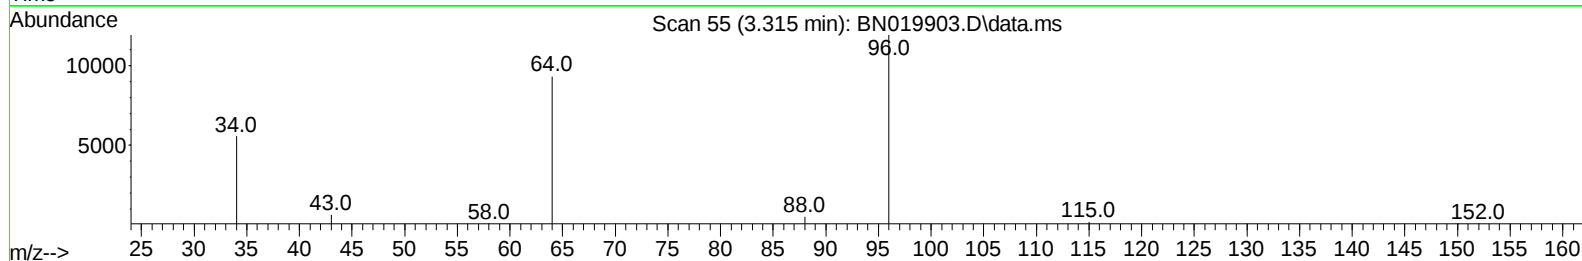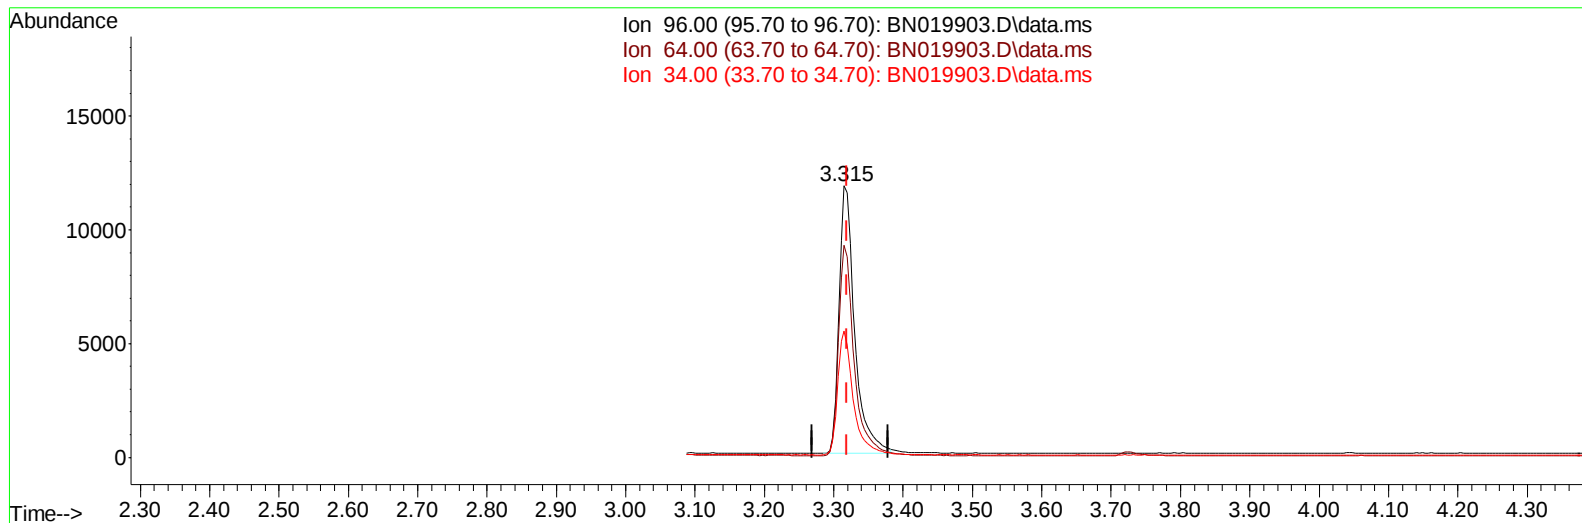

TIC: BN019903.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.315min (-0.004) 3.80 ng/ul m

response 18328

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	78.18#
34.00	22.70	46.64#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019903.D
 Acq On : 21 May 2022 12:11
 Operator : CG/JU
 Sample : N2918-23
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Quant Time: May 23 09:38:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	4079	0.400	ng/ul	0.00
4) Naphthalene-d8	10.644	136	13650	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.477	164	8270	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.216	188	17411	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	14844	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264	11553	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	18328m	3.797	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	8422	0.408	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	21548	0.459	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.693	128	4177	0.095	ng/ul	95
14) Pentachlorophenol	16.870	266	2221	0.593	ng/ul	90
16) Anthracene	17.347	178	1884	0.036	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019903.D
Acq On : 21 May 2022 12:11
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Quant Time: May 23 09:38:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

