

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
 Data File : BN019882.D
 Acq On : 20 May 2022 23:03
 Operator : CG/JU
 Sample : N2843-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4J3

Manual Integrations
 APPROVED

Reviewed By : Jagrut Upadhyay 05/26/2022
 Supervised By : mohammad ahmed 05/27/2022

Quant Time: May 26 04:42:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4403	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	15093	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	9339	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	20224	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	17676	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	14243	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	13335	2.559	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	4325	0.189	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	11699	0.209	ng/ul	0.00
Target Compounds						
					Qvalue	
7) 2-Methylnaphthalene	12.300	142	693	0.023	ng/ul#	100
8) 1-Methylnaphthalene	12.520	142	646	0.023	ng/ul#	100
15) Phenanthrene	17.251	178	8662	0.116	ng/ul	96
16) Anthracene	17.344	178	1246	0.021	ng/ul#	75
19) Fluoranthene	19.267	202	15650	0.193	ng/ul	98
20) Pyrene	19.629	202	14615m	0.181	ng/ul	
21) Benzo(a)anthracene	21.382	228	7341	0.111	ng/ul#	88
22) Chrysene	21.432	228	10416	0.134	ng/ul#	91
24) Benzo(b)fluoranthene	23.031	252	9675m	0.134	ng/ul	
25) Benzo(k)fluoranthene	23.071	252	3428m	0.049	ng/ul	
26) Benzo(a)pyrene	23.633	252	5768	0.094	ng/ul#	86
27) Indeno(1,2,3-cd)pyrene	26.134	276	3882	0.051	ng/ul#	93
29) Benzo(g,h,i)perylene	26.875	276	3523	0.050	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052022\
Data File : BN019882.D
Acq On : 20 May 2022 23:03
Operator : CG/JU
Sample : N2843-13
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW4J3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022


Quant Time: May 26 04:42:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

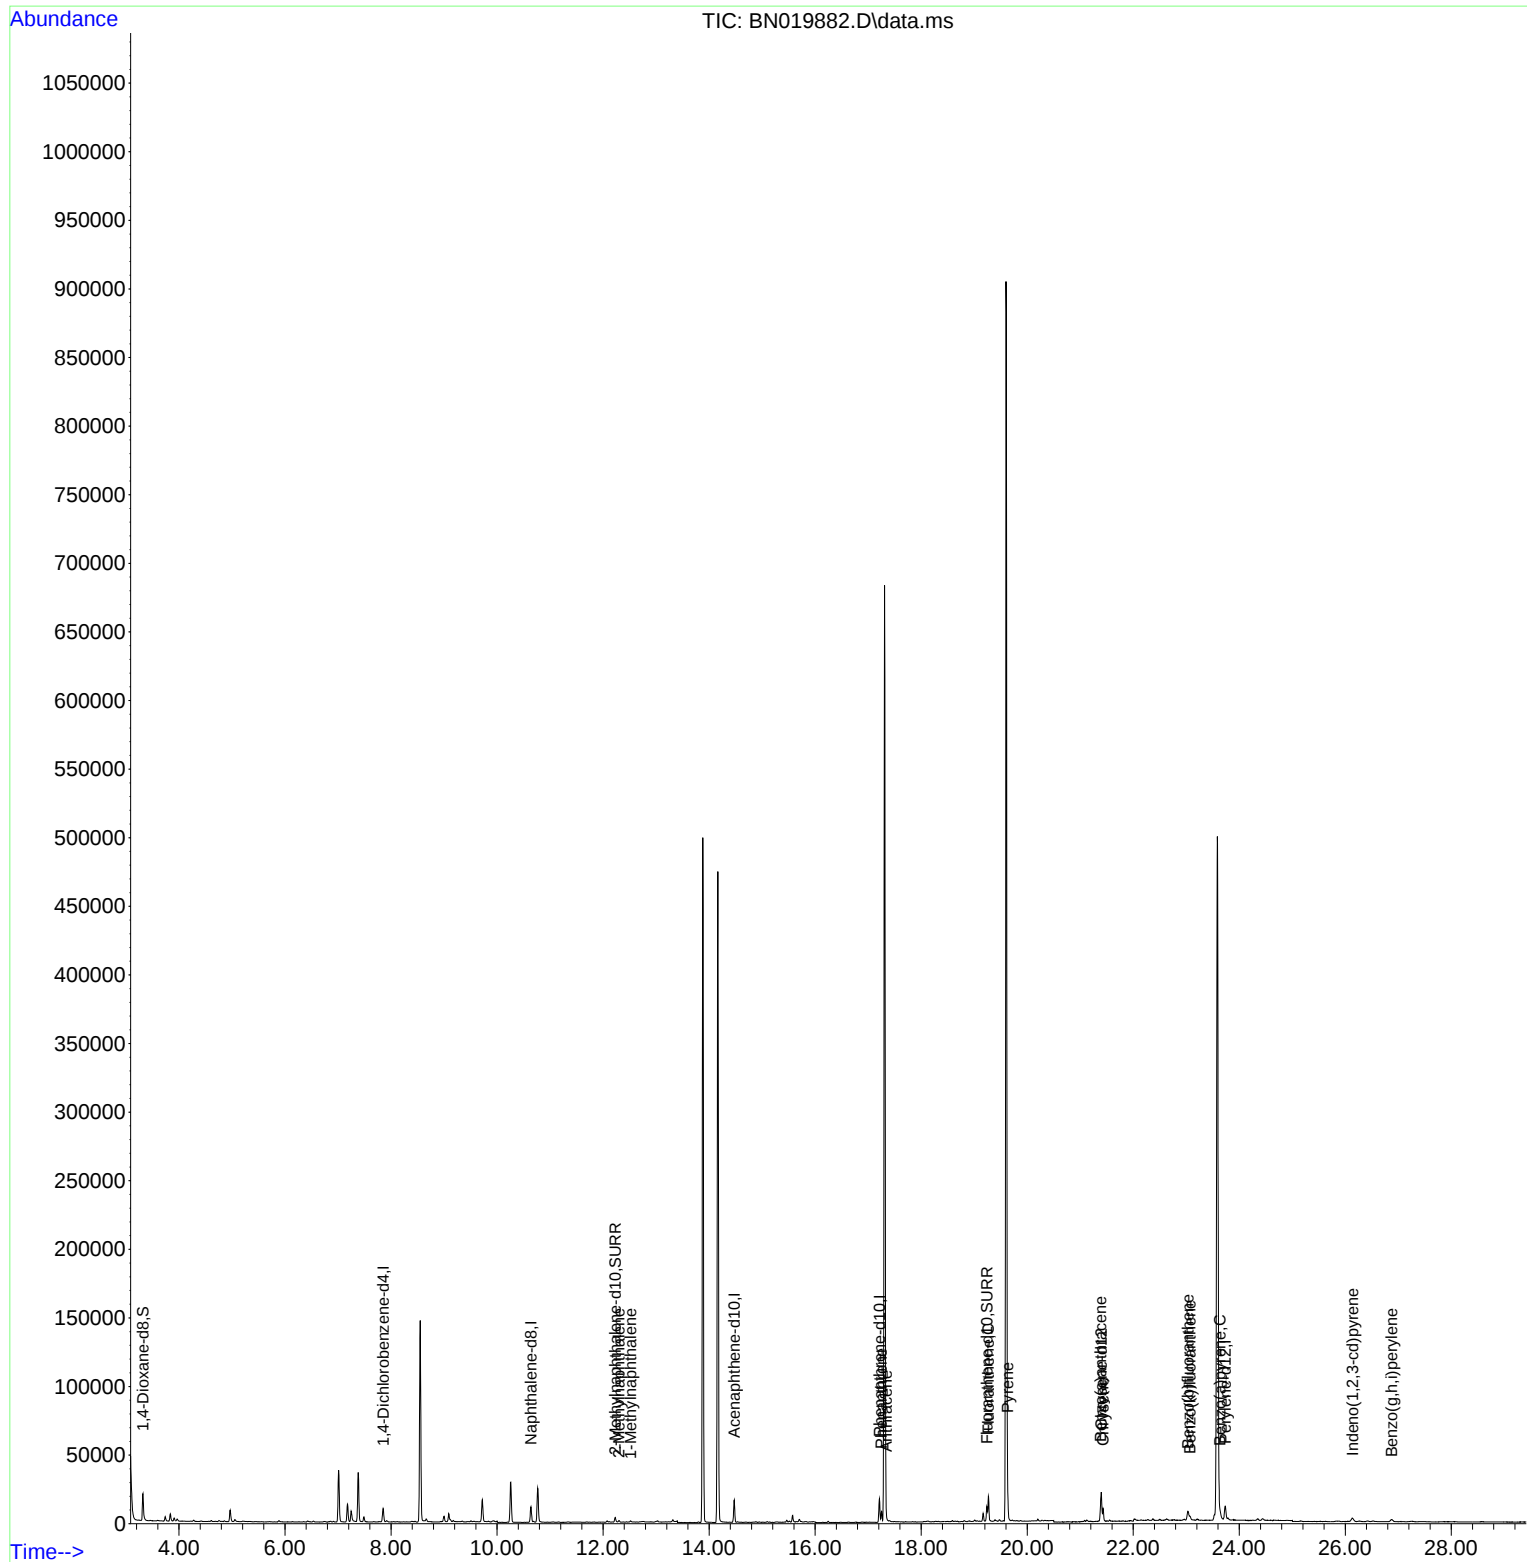



#7
2-Methylnaphthalene
Concen: 0.023 ng/ul
RT: 12.300 min Scan# 2061
Delta R.T. -0.005 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3

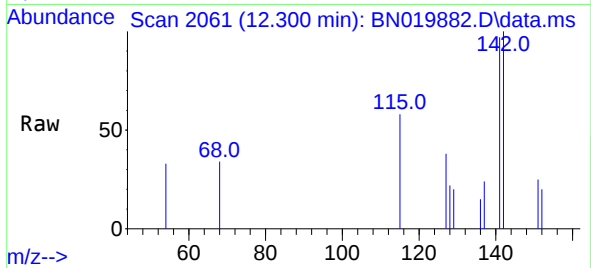


Tgt Ion:142 Resp: 690
Ion Ratio Lower Upper
142 100
141 98.1 0.0 0.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

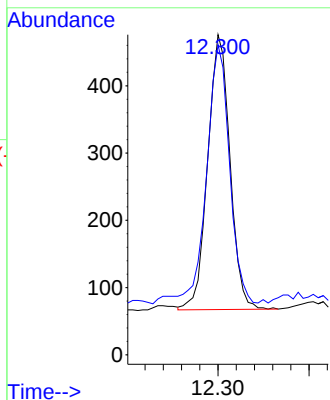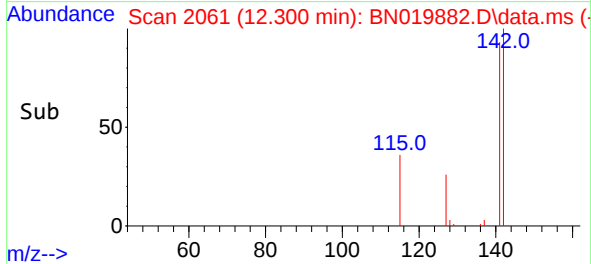


#8
1-Methylnaphthalene
Concen: 0.023 ng/ul
RT: 12.520 min Scan# 2101
Delta R.T. -0.005 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03

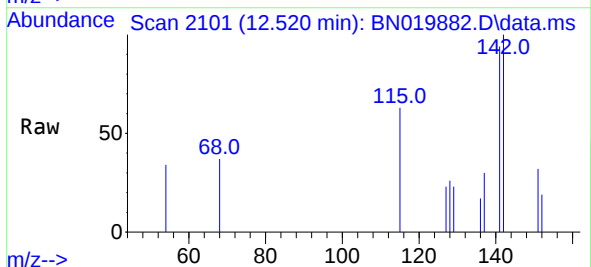


Tgt Ion:142 Resp: 646
Ion Ratio Lower Upper
142 100
141 90.2 0.0 0.0

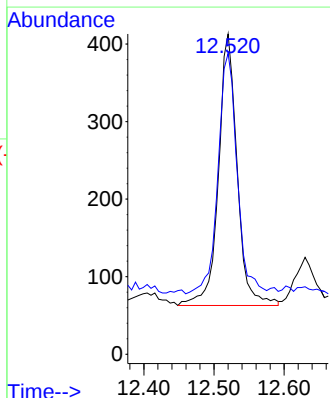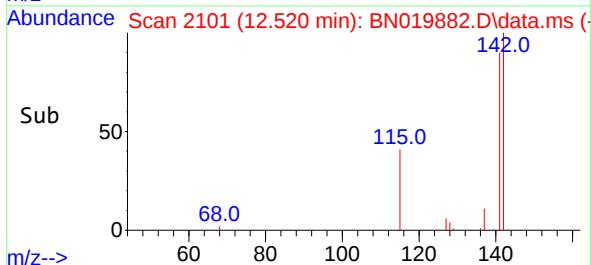



#15
Phenanthrene
Concen: 0.116 ng/u1
RT: 17.251 min Scan# 3119
Delta R.T. -0.004 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3




Tgt Ion:178 Resp: 866
Ion Ratio Lower Upper
178 100
179 18.1 12.9 19.3
176 21.0 15.5 23.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

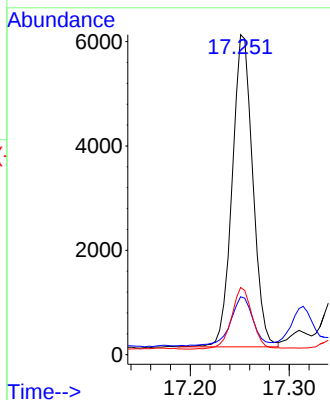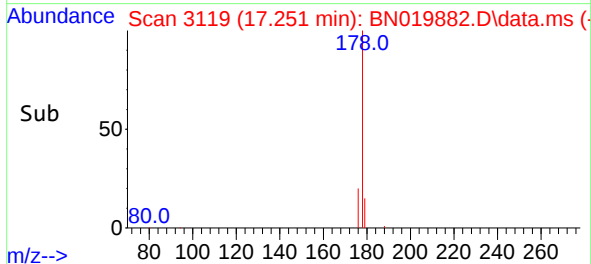


#16
Anthracene
Concen: 0.021 ng/u1
RT: 17.344 min Scan# 3141
Delta R.T. -0.004 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03

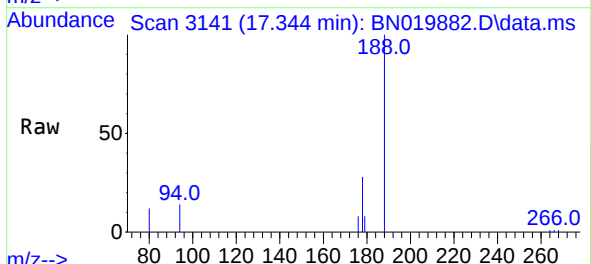


Tgt Ion:178 Resp: 1246
Ion Ratio Lower Upper
178 100
179 29.9 13.1 19.7#
176 27.5 15.3 22.9#

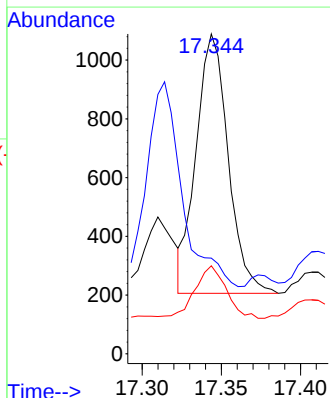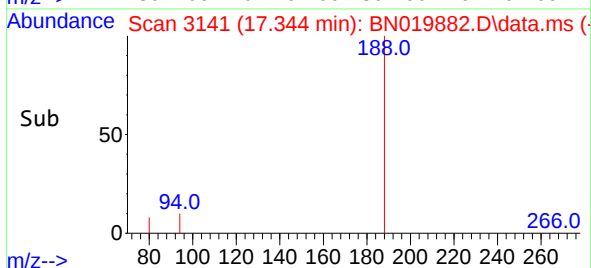



#19
Fluoranthene
Concen: 0.193 ng/ul
RT: 19.267 min Scan# 3580
Delta R.T. -0.005 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3



Tgt Ion:202 Resp: 15650
Ion Ratio Lower Upper
202 100
101 13.3 9.7 14.5
100 9.8 7.4 11.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

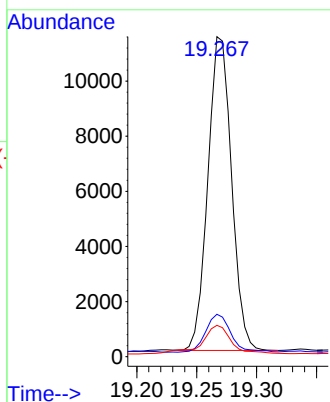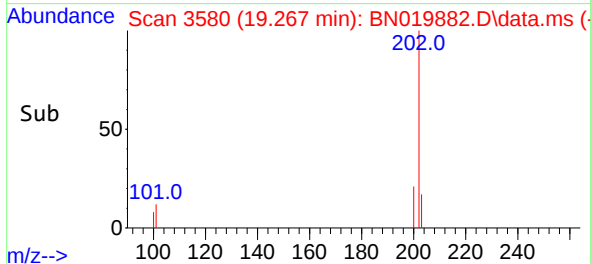

#20
Pyrene
Concen: 0.181 ng/ul m
RT: 19.629 min Scan# 3658
Delta R.T. -0.005 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03


Tgt Ion:202 Resp: 14615
Ion Ratio Lower Upper
202 100
101 15.7 11.4 17.0
100 14.5 9.0 13.4#

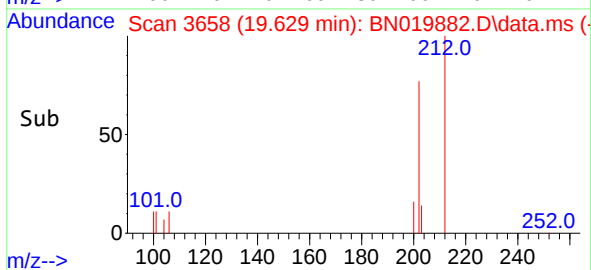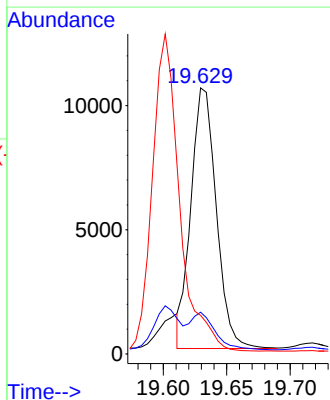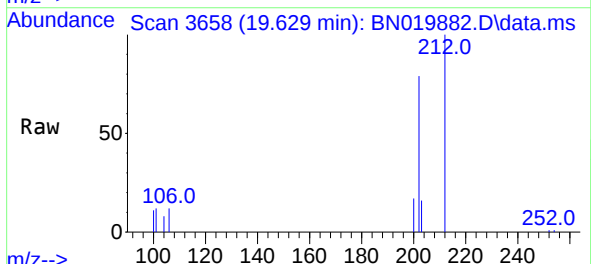



#21
Benzo(a)anthracene
Concen: 0.111 ng/ul
RT: 21.382 min Scan# 4147
Delta R.T. -0.006 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3

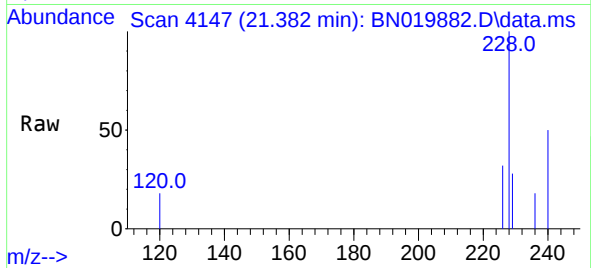


Tgt Ion:228 Resp: 734
Ion Ratio Lower Upper
228 100
229 27.9 16.1 24.1
226 31.8 22.1 33.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

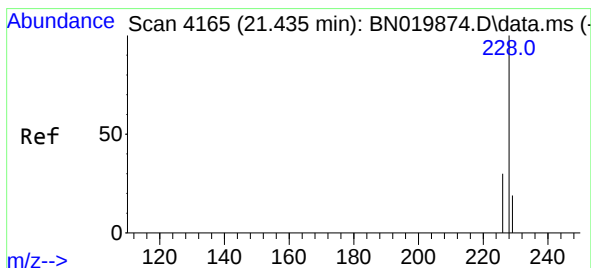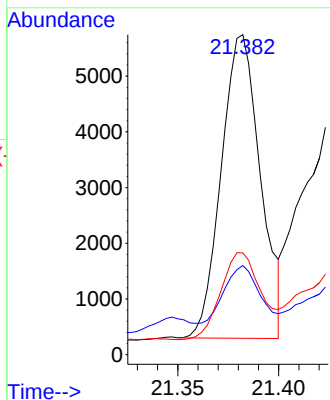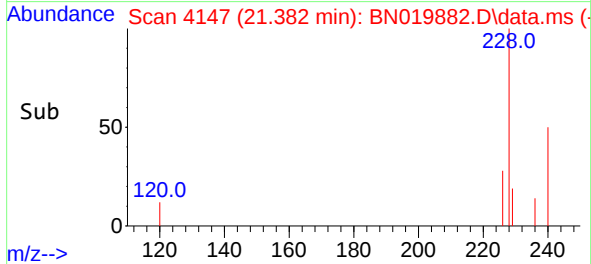


#22
Chrysene
Concen: 0.134 ng/ul
RT: 21.432 min Scan# 4164
Delta R.T. -0.009 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03

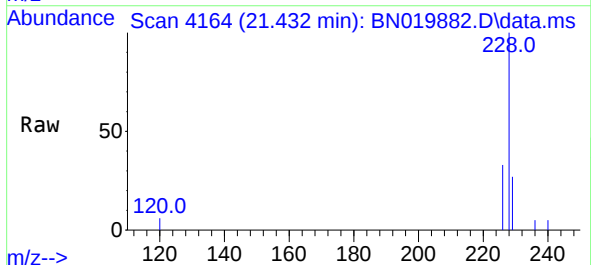


Tgt Ion:228 Resp: 10416
Ion Ratio Lower Upper
228 100
226 32.8 24.2 36.2
229 26.6 16.0 24.0#

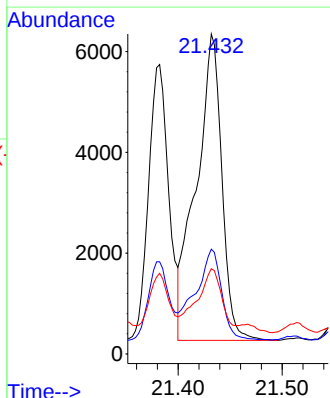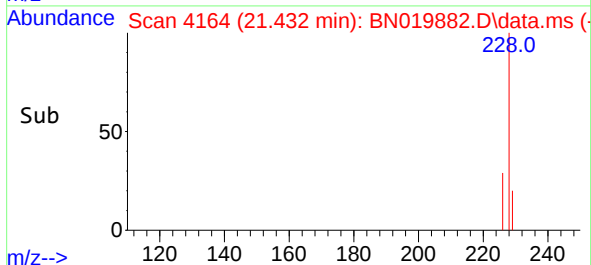



#24
Benzo(b)fluoranthene
Concen: 0.134 ng/ul m
RT: 23.031 min Scan# 4711
Delta R.T. -0.003 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3

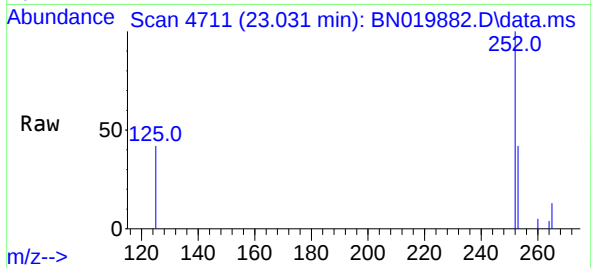


Tgt Ion:252 Resp: 9674
Ion Ratio Lower Upper
252 100
253 41.7 0.0 52.0
125 42.2 0.0 40.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

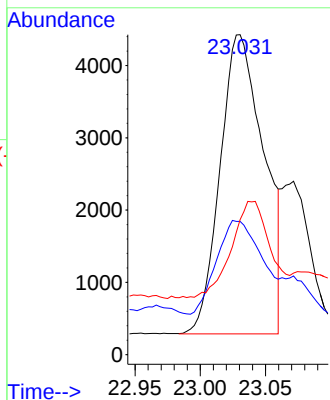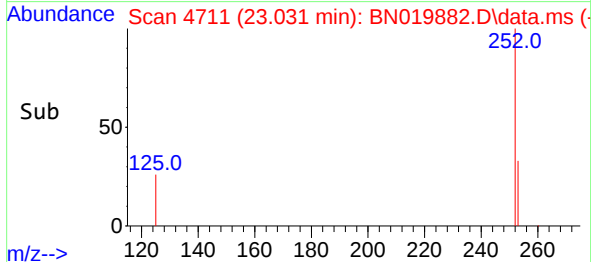


#25
Benzo(k)fluoranthene
Concen: 0.049 ng/ul m
RT: 23.071 min Scan# 4725
Delta R.T. -0.009 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03

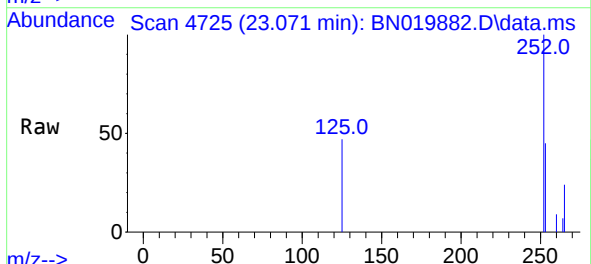


Tgt Ion:252 Resp: 3428
Ion Ratio Lower Upper
252 100
253 45.4 20.2 30.2#
125 47.0 11.0 16.6#

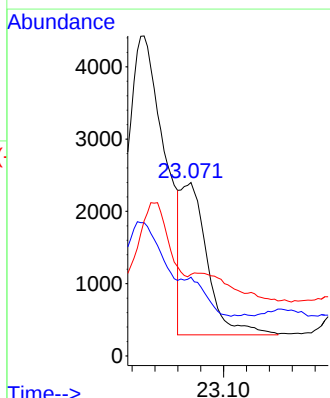



#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.633 min Scan# 4917
Delta R.T. -0.006 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03




Instrument :
BNA_N
ClientSampleId :
EW4J3

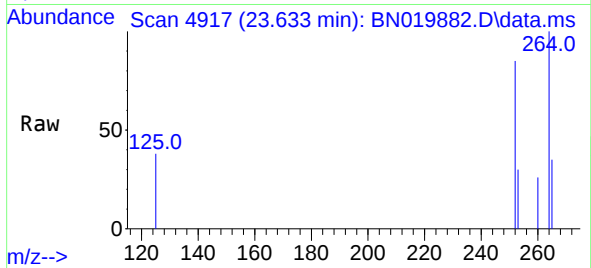

Tgt Ion:252 Resp: 5768
Ion Ratio Lower Upper
252 100
253 35.5 23.4 35.0
125 44.6 28.3 42.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

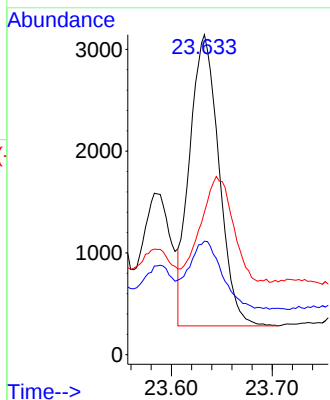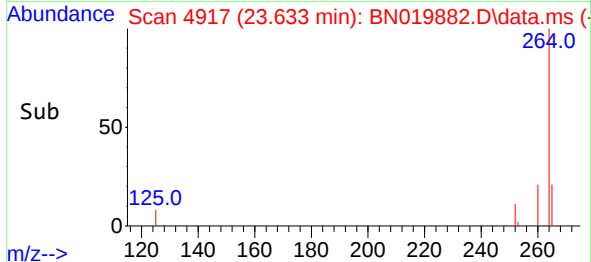

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.051 ng/ul
RT: 26.134 min Scan# 5723
Delta R.T. -0.013 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03


Tgt Ion:276 Resp: 3882
Ion Ratio Lower Upper
276 100
138 33.2 23.6 35.4
227 4.8 0.0 0.0

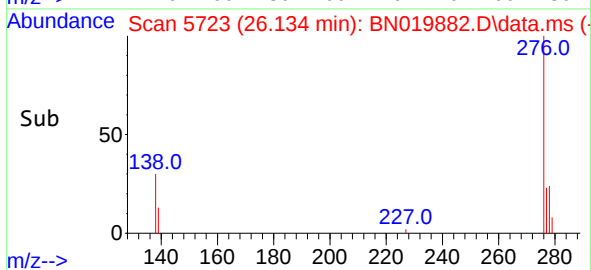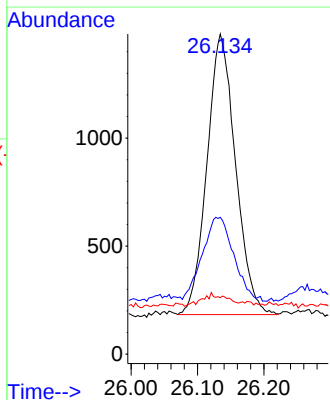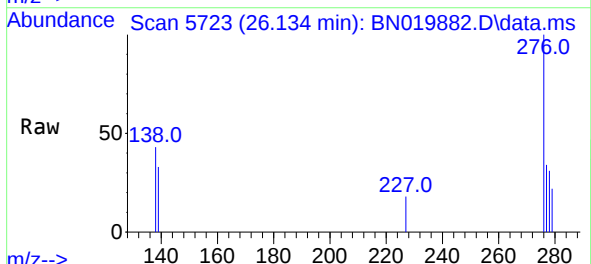

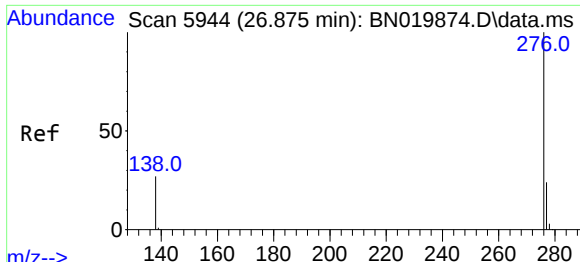

#29
Benzo(g,h,i)perylene
Concen: 0.050 ng/ul
RT: 26.875 min Scan# 5944
Delta R.T. -0.003 min
Lab File: BN019882.D
Acq: 20 May 2022 23:03

Instrument :
BNA_N
ClientSampleId :
EW4J3

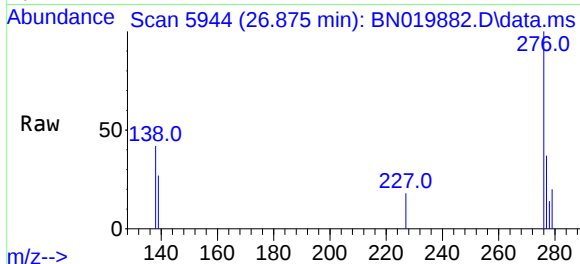

Tgt Ion:276 Resp: 352
Ion Ratio Lower Upper
276 100
138 42.1 20.9 31.3
277 36.6 20.4 30.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/26/2022
Supervised By :mohammad ahmed 05/27/2022

