

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031581.D
 Acq On : 20 May 2024 21:14
 Operator : MA/JU
 Sample : P2484-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q2

Quant Time: May 20 23:09:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 15 02:37:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.698	152	530450	20.000	ng/ul	0.00
20) Naphthalene-d8	10.481	136	2350279	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.333	164	1456716	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.074	188	2884176	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1785655	20.000	ng/ul	0.00
88) Perylene-d12	24.239	264	1716897	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	58979	4.579	ng/uL	0.00
4) Pyridine-d5	3.605	84	591672	15.027	ng/ul	0.00
7) Phenol-d5	6.857	99	1223648	27.181	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	748545	25.398	ng/ul	0.00
11) 2-Chlorophenol-d4	7.228	132	917646	29.736	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	1009306	29.197	ng/ul	0.00
21) Nitrobenzene-d5	8.851	128	477160	30.805	ng/ul	0.00
24) 2-Nitrophenol-d4	9.569	143	412826	35.315	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.092	165	877304	30.208	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	1443635	27.947	ng/ul	0.00
46) Dimethylphthalate-d6	13.745	166	2893562	31.405	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	3459800	30.734	ng/ul	0.00
54) 4-Nitrophenol-d4	14.533	143	315051	17.828	ng/ul	0.00
60) Fluorene-d10	15.327	176	2516276	29.861	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	106415	10.305	ng/ul	0.00
73) Anthracene-d10	17.174	188	3780312	30.653	ng/ul	0.00
81) Pyrene-d10	19.468	212	3758155	42.391	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.039	264	2465697	32.356	ng/ul	-0.01
Target Compounds						
					Qvalue	
55) 4-Nitrophenol	14.569	109	222094	15.556	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031581.D
Acq On : 20 May 2024 21:14
Operator : MA/JU
Sample : P2484-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9Q2

Quant Time: May 20 23:09:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 15 02:37:21 2024
Response via : Initial Calibration

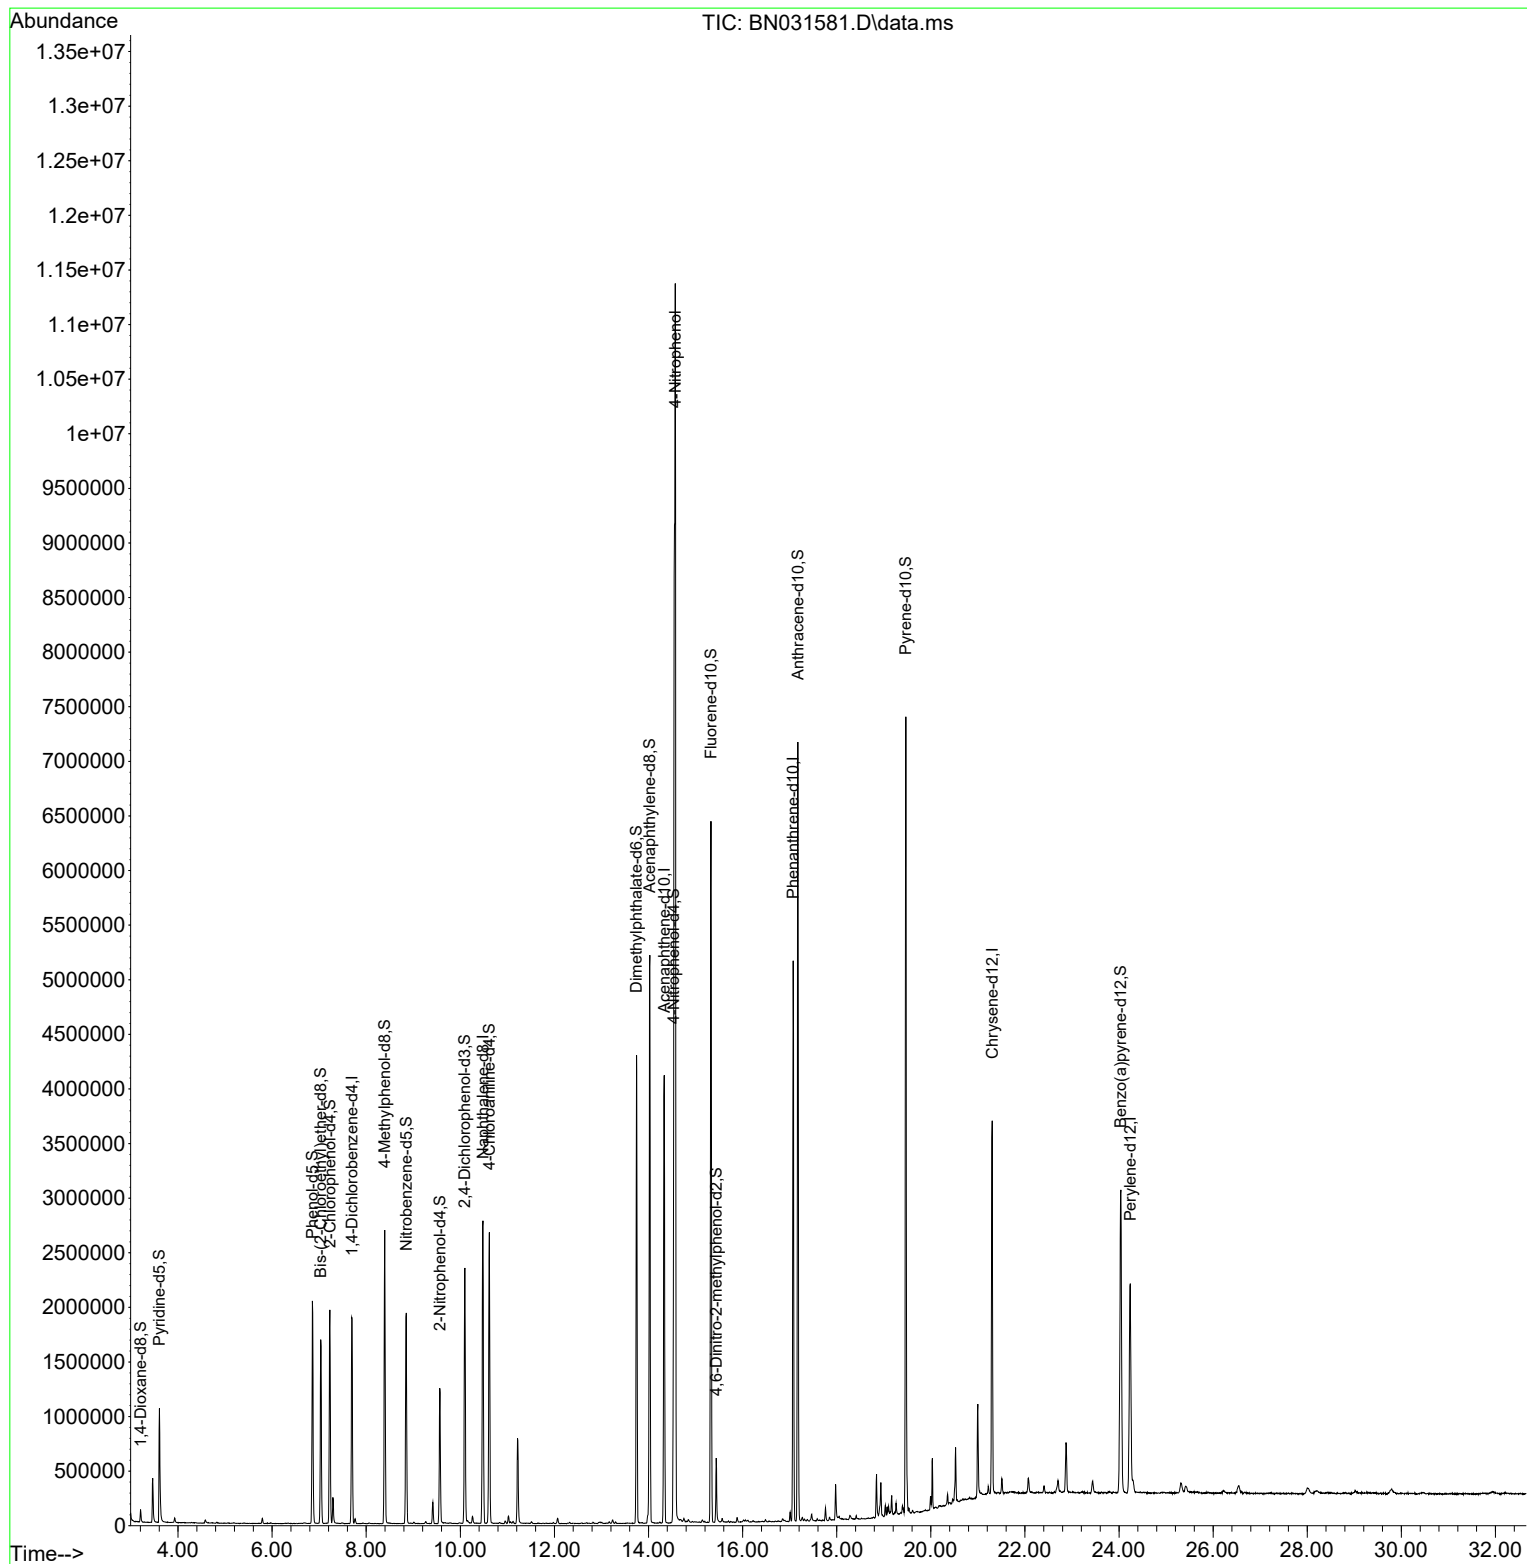

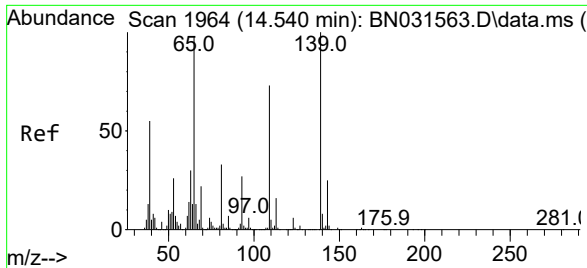

#55
 4-Nitrophenol
 Concen: 15.556 ng/ul
 RT: 14.569 min Scan# 1969
 Delta R.T. 0.029 min
 Lab File: BN031581.D
 Acq: 20 May 2024 21:14

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q2

Tgt Ion:109 Resp: 222094
 Ion Ratio Lower Upper
 109 100
 139 10.6 104.0 156.0#
 65 15.1 110.2 165.2#

