

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031589.D
 Acq On : 21 May 2024 04:27
 Operator : MA/JU
 Sample : P2484-21
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q0

Quant Time: May 21 06:08:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 15 02:37:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	522229	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	2322557	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.328	164	1477442	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.075	188	2973206	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1944192	20.000	ng/u1	-0.01
88) Perylene-d12	24.233	264	1706547	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	51902	4.093	ng/uL	0.00
4) Pyridine-d5	3.605	84	464768	11.990	ng/u1	0.00
7) Phenol-d5	6.858	99	1124617	25.374	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	677802	23.360	ng/u1	0.00
11) 2-Chlorophenol-d4	7.222	132	860203	28.314	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	770552	22.641	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	440295	28.764	ng/u1	0.00
24) 2-Nitrophenol-d4	9.563	143	410047	35.496	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	804660	28.038	ng/u1	0.00
31) 4-Chloroaniline-d4	10.610	131	1097863	21.507	ng/u1	0.00
46) Dimethylphthalate-d6	13.746	166	2608039	27.909	ng/u1	0.00
49) Acenaphthylene-d8	14.022	160	3086186	27.030	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	411619	22.966	ng/u1	0.00
60) Fluorene-d10	15.322	176	2282233	26.704	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.440	200	212639	19.974	ng/u1	0.00
73) Anthracene-d10	17.169	188	3462019	27.232	ng/u1	-0.01
81) Pyrene-d10	19.469	212	3646728	37.780	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.033	264	2311307	30.514	ng/u1	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.511	105	84414	1.459	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031589.D
Acq On : 21 May 2024 04:27
Operator : MA/JU
Sample : P2484-21
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9Q0


Quant Time: May 21 06:08:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 15 02:37:21 2024
Response via : Initial Calibration

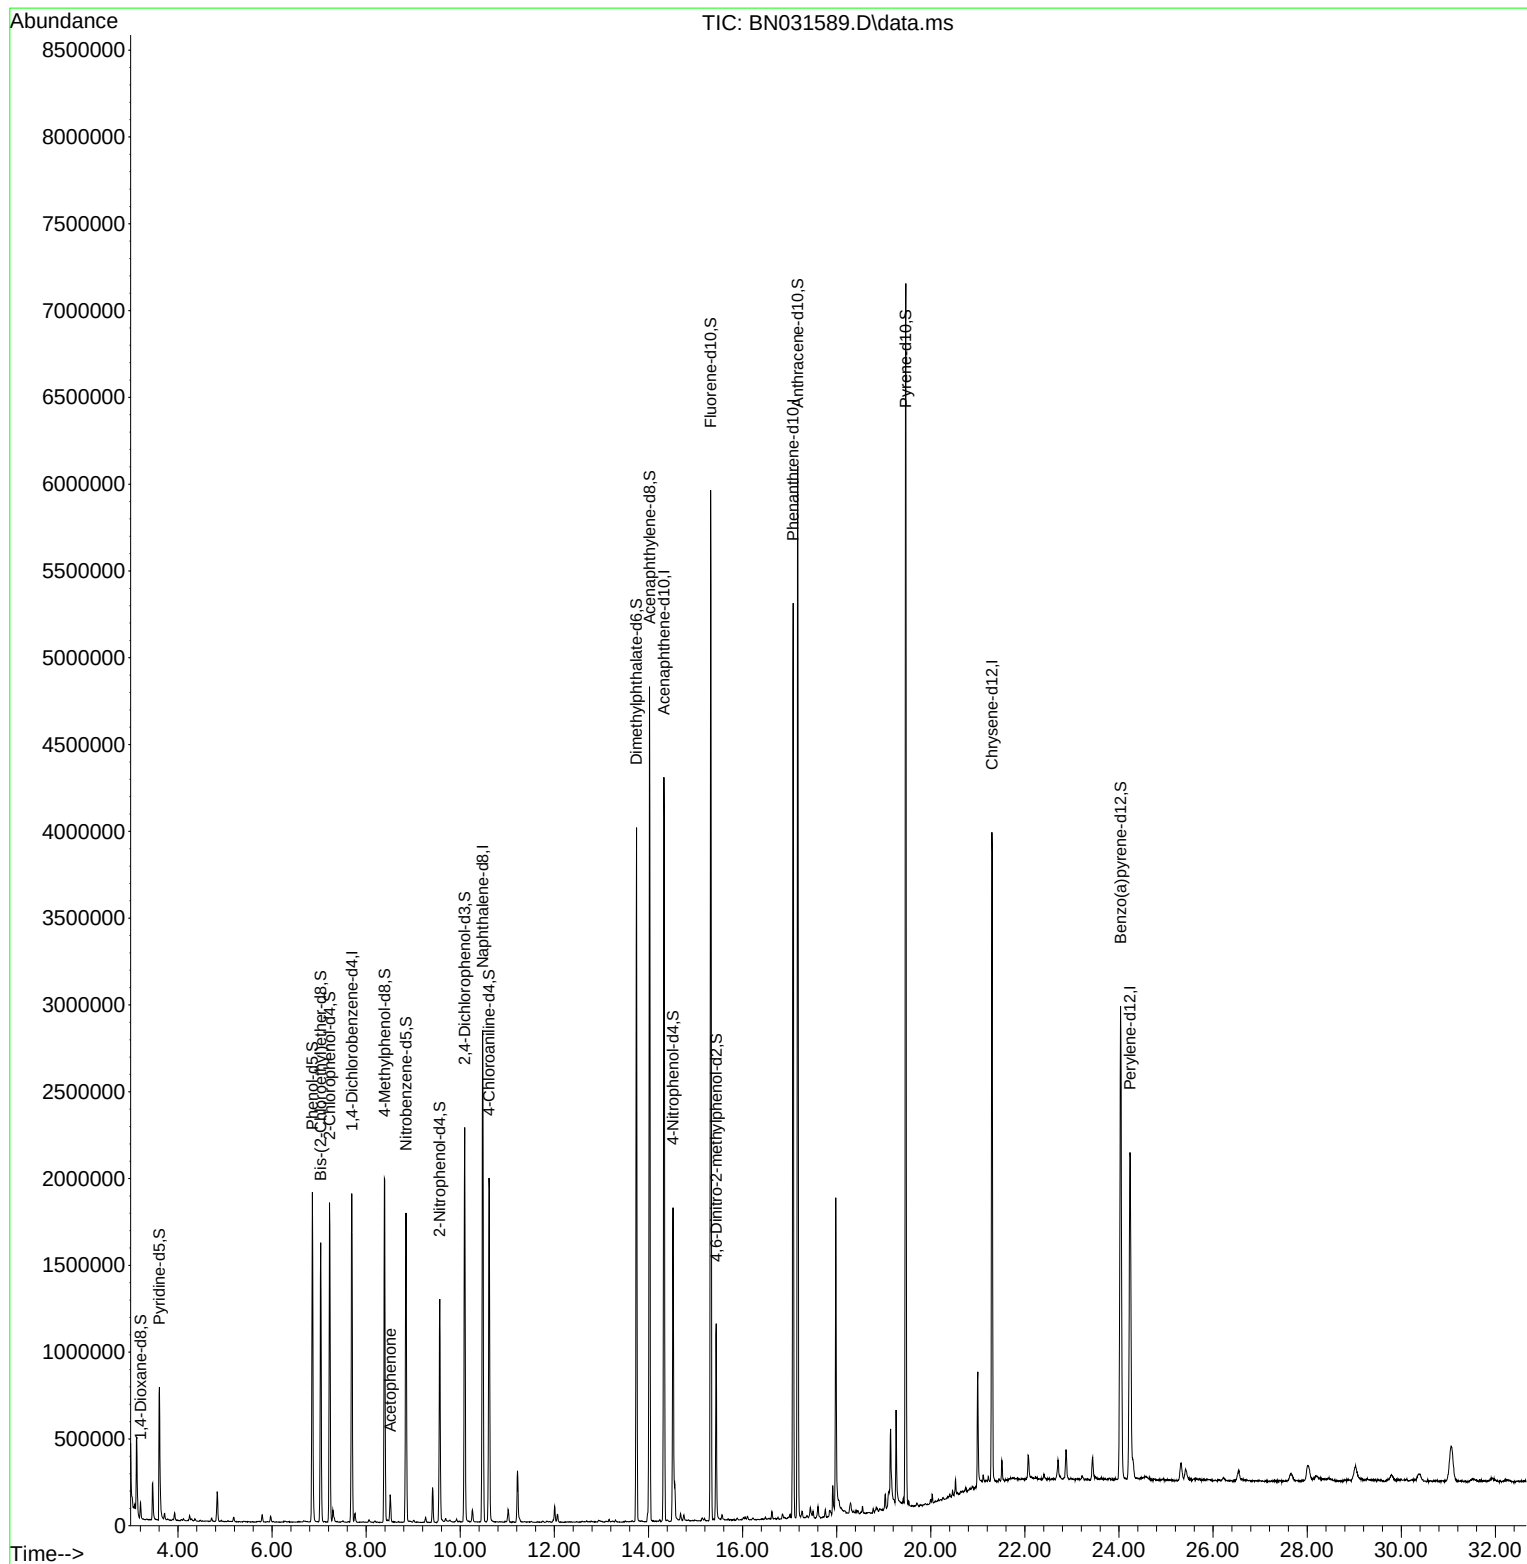

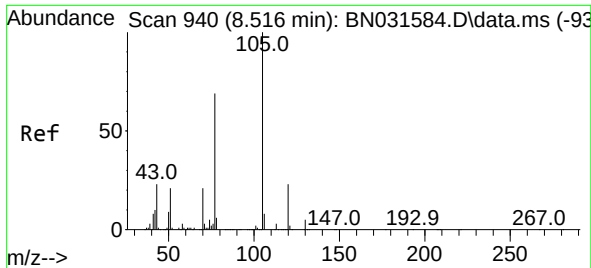

#16
 Acetophenone
 Concen: 1.459 ng/ul
 RT: 8.511 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN031589.D
 Acq: 21 May 2024 04:27

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q0

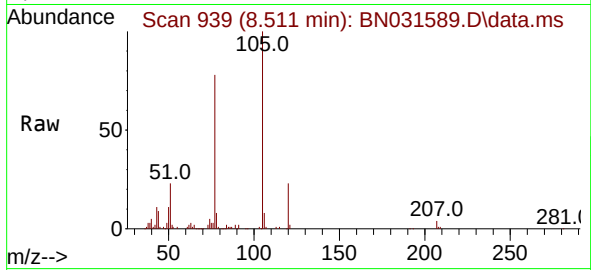

Tgt Ion:105 Resp: 84414
 Ion Ratio Lower Upper
 105 100
 77 78.0 63.7 95.5
 51 23.0 20.6 31.0

