

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031564.D
 Acq On : 20 May 2024 09:35
 Operator : MA/JU
 Sample : PB160893BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK893

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	33	37	44	rBV	120499	177468	1.44%	0.133%
2	3.599	101	104	124	rBV	1671373	2752441	22.30%	2.056%
3	3.928	156	160	165	rBV	33113	48505	0.39%	0.036%
4	4.140	192	196	203	rVB6	11823	18840	0.15%	0.014%
5	6.857	651	658	668	rBV	2163804	3323392	26.93%	2.483%
6	7.034	681	688	699	rVB	1913723	2958144	23.97%	2.210%
7	7.222	711	720	736	rBV	2014173	3323935	26.94%	2.483%
8	7.692	791	800	810	rBV	1984882	3171280	25.70%	2.369%
9	8.392	909	919	933	rBV	2612646	4210088	34.12%	3.145%
10	8.845	988	996	1008	rBV	2075713	3402664	27.57%	2.542%
11	9.563	1108	1118	1131	rBV	1328224	2152312	17.44%	1.608%
12	10.092	1199	1208	1223	rBV	2439764	4016486	32.55%	3.000%
13	10.475	1265	1273	1284	rBV	2846741	4908810	39.78%	3.667%
14	10.610	1287	1296	1308	rBV	2764106	4707509	38.15%	3.517%
15	12.069	1539	1544	1550	rVB	48262	77994	0.63%	0.058%
16	13.745	1822	1829	1840	rBV	4976267	6745644	54.66%	5.039%
17	14.022	1868	1876	1890	rBV2	5523937	8225404	66.65%	6.144%
18	14.327	1921	1928	1939	rBV	4699807	6818421	55.25%	5.093%
19	14.521	1954	1961	1977	rBV	2237934	3114340	25.24%	2.326%
20	15.321	2090	2097	2106	rBV	6951952	10050857	81.45%	7.508%
21	15.439	2110	2117	2130	rVV	1433169	2014345	16.32%	1.505%
22	15.563	2134	2138	2145	rVB	30308	52774	0.43%	0.039%
23	16.757	2337	2341	2344	rVB5	8303	12362	0.10%	0.009%
24	16.863	2355	2359	2362	rBV2	12489	16270	0.13%	0.012%
25	17.074	2388	2395	2404	rBV	5752949	8096723	65.61%	6.048%
26	17.174	2405	2412	2424	rBV2	7491701	10789199	87.43%	8.060%
27	17.968	2544	2547	2553	rBV6	12497	17767	0.14%	0.013%
28	19.033	2723	2728	2733	rBV2	80366	115677	0.94%	0.086%
29	19.098	2735	2739	2745	rVV	81625	116213	0.94%	0.087%
30	19.415	2790	2793	2795	rBV3	18297	20358	0.16%	0.015%
31	19.468	2796	2802	2818	rVB	9433634	12340553	100.00%	9.218%
32	21.303	3108	3114	3126	rVB2	5602603	7958665	64.49%	5.945%
33	24.039	3569	3579	3593	rBV2	4482463	10388777	84.18%	7.760%
34	24.239	3603	3613	3637	rVB	3020756	7724095	62.59%	5.770%

Sum of corrected areas: 133868312

Instrument :

BNA_N

ClientSampleId :




SBLK893

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031564.D
Acq On : 20 May 2024 09:35
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

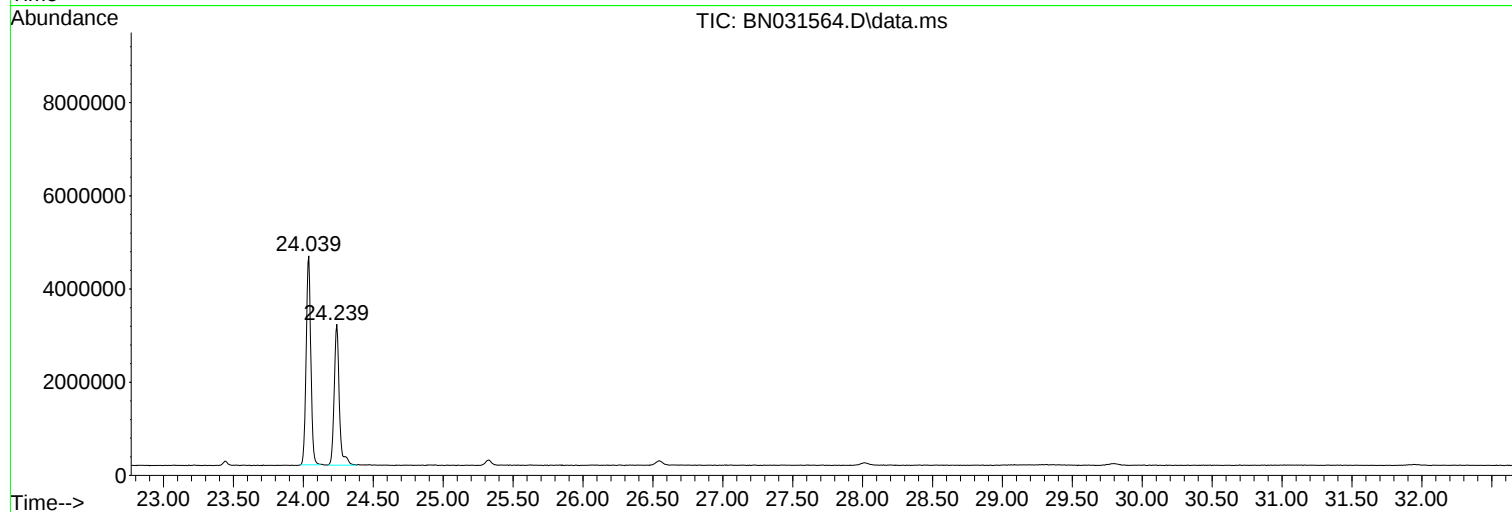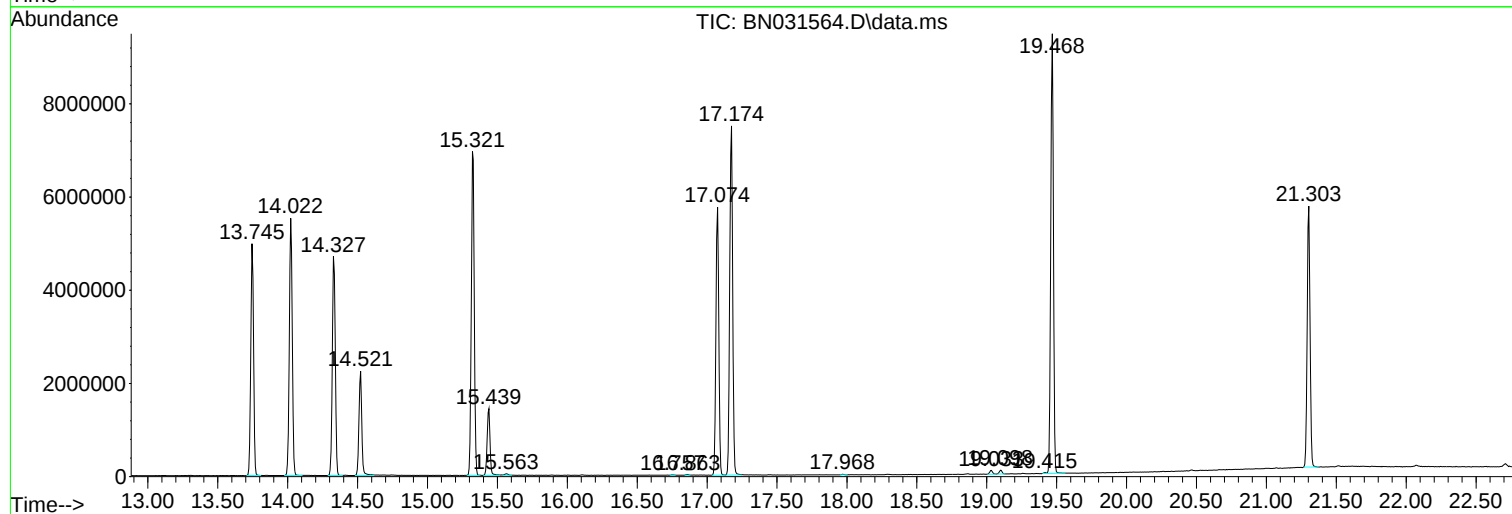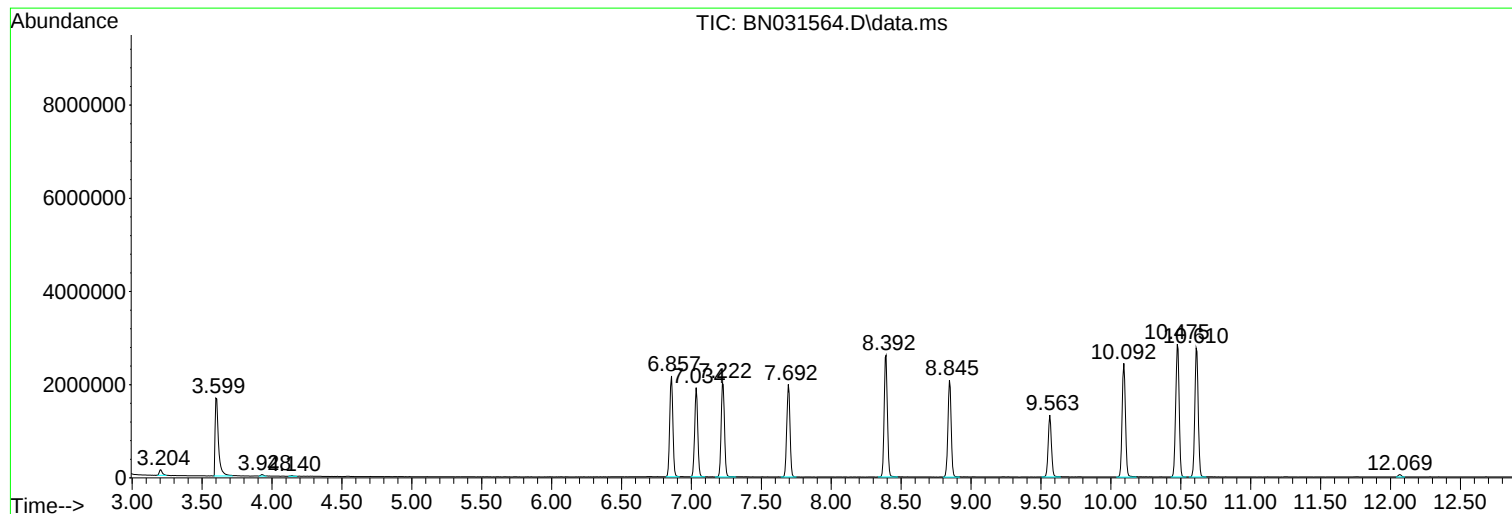

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031564.D
Acq On : 20 May 2024 09:35
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031564.D
Acq On : 20 May 2024 09:35
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc