

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031569.D
 Acq On : 20 May 2024 12:57
 Operator : MA/JU
 Sample : PB160897BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	32	37	44	rVB	128560	168877	1.65%	0.142%
2	3.599	101	104	127	rBV	1786202	2647597	25.84%	2.226%
3	3.928	156	160	165	rVB	40745	56060	0.55%	0.047%
4	4.140	192	196	202	rVB4	13753	20544	0.20%	0.017%
5	4.546	259	265	271	rVB5	7434	13166	0.13%	0.011%
6	6.858	651	658	672	rBV	2086399	3187327	31.11%	2.680%
7	7.034	681	688	700	rVB	1820229	2824884	27.57%	2.375%
8	7.222	709	720	737	rBV	1940745	3156900	30.81%	2.654%
9	7.693	792	800	810	rVB	1981029	3183632	31.07%	2.676%
10	8.393	910	919	931	rBV	2535837	4025348	39.29%	3.384%
11	8.846	987	996	1006	rBV	1975319	3228964	31.52%	2.715%
12	9.563	1110	1118	1131	rBV	1236475	2022738	19.74%	1.700%
13	10.093	1199	1208	1222	rBV	2328734	3830344	37.39%	3.220%
14	10.475	1265	1273	1282	rBV	2928969	4965527	48.47%	4.174%
15	10.616	1288	1297	1308	rBV	2609777	4494511	43.87%	3.778%
16	11.252	1401	1405	1410	rBV8	6917	11862	0.12%	0.010%
17	12.069	1537	1544	1551	rBV	45612	76777	0.75%	0.065%
18	13.293	1750	1752	1758	rVB5	6432	11486	0.11%	0.010%
19	13.746	1821	1829	1839	rBV	4488932	6270325	61.20%	5.271%
20	14.022	1869	1876	1885	rBV2	5332508	7721643	75.37%	6.491%
21	14.328	1921	1928	1939	rBV	4666417	6805736	66.43%	5.721%
22	14.522	1953	1961	1977	rBV	2102005	2856077	27.88%	2.401%
23	14.745	1996	1999	2005	rVB7	9053	13665	0.13%	0.011%
24	15.322	2090	2097	2104	rBV	6473467	9407428	91.82%	7.909%
25	15.440	2110	2117	2133	rBV	1263025	1767888	17.26%	1.486%
26	15.563	2133	2138	2145	rVB3	31163	52903	0.52%	0.044%
27	16.110	2226	2231	2236	rVB7	7500	12186	0.12%	0.010%
28	16.751	2337	2340	2344	rBV3	8832	12712	0.12%	0.011%
29	16.857	2355	2358	2362	rVB3	9600	11888	0.12%	0.010%
30	17.075	2388	2395	2403	rBV	5561140	7771678	75.85%	6.533%
31	17.175	2405	2412	2426	rVV2	6694694	9787644	95.53%	8.228%
32	17.451	2455	2459	2461	rBV3	6820	10290	0.10%	0.009%
33	18.863	2697	2699	2705	rVB5	11777	13267	0.13%	0.011%
34	19.033	2723	2728	2733	rBV	66736	96437	0.94%	0.081%
35	19.098	2735	2739	2745	rVV	67956	95519	0.93%	0.080%
36	19.469	2795	2802	2810	rBV	7585088	10245515	100.00%	8.613%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031569.D
Acq On : 20 May 2024 12:57
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK897

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Title : SVOA CALIBRATION

37	21.304	3108	3114	3126	rVB	4218594	6058360	59.13%	5.093%
38	24.033	3569	3578	3594	rBV	2885716	6877373	67.13%	5.782%
39	24.233	3604	3612	3621	rBV2	2081294	5136488	50.13%	4.318%




Sum of corrected areas: 118951566

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031569.D
Acq On : 20 May 2024 12:57
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

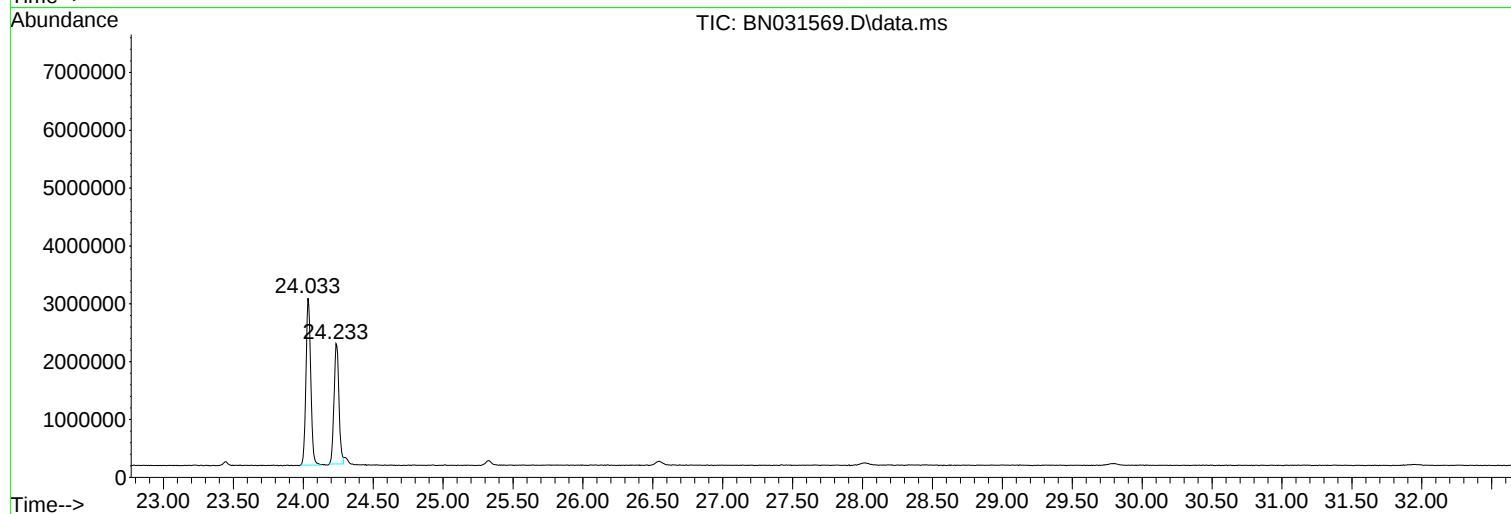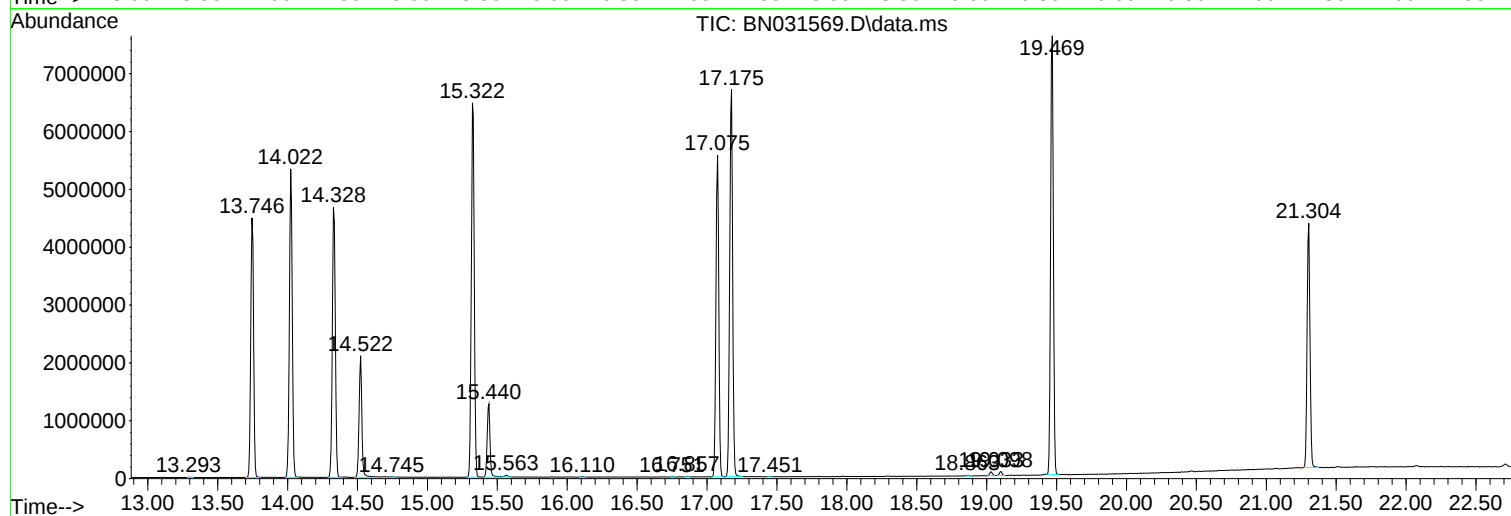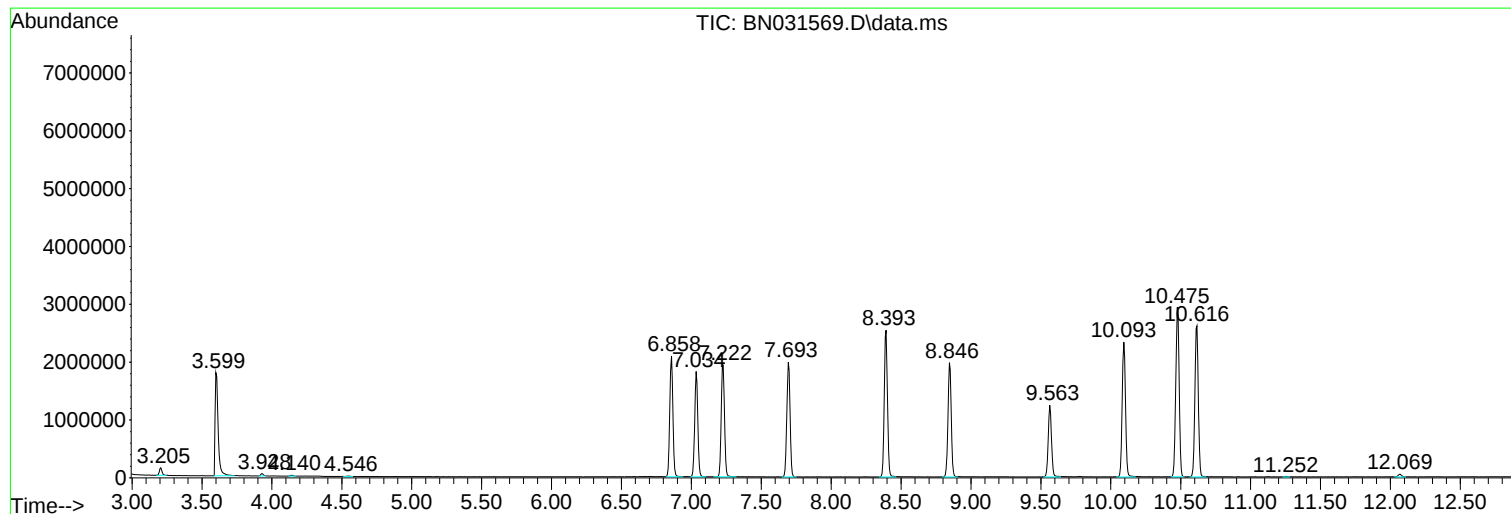

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031569.D
Acq On : 20 May 2024 12:57
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031569.D
Acq On : 20 May 2024 12:57
Operator : MA/JU
Sample : PB160897BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc