

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031571.D
 Acq On : 20 May 2024 14:20
 Operator : MA/JU
 Sample : PB160987BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK987

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	4	7	14	rBV8	10350	18405	0.18%	0.017%
2	3.122	19	23	30	rVB	45253	68505	0.65%	0.062%
3	3.199	33	36	46	rVB	111601	153128	1.46%	0.138%
4	3.599	100	104	122	rBV	1564081	2373112	22.61%	2.137%
5	3.928	155	160	169	rVB	57806	87628	0.83%	0.079%
6	6.857	650	658	671	rBV	1758547	2741933	26.12%	2.469%
7	7.034	681	688	699	rVB	1562876	2424063	23.09%	2.183%
8	7.222	713	720	733	rBV	1709077	2713561	25.85%	2.444%
9	7.693	792	800	809	rVB	1761507	2789327	26.57%	2.512%
10	8.387	909	918	930	rBV	2143202	3462681	32.99%	3.118%
11	8.846	988	996	1004	rBV	1735622	2782761	26.51%	2.506%
12	9.563	1111	1118	1130	rBV	1087861	1737510	16.55%	1.565%
13	10.093	1200	1208	1225	rBV	2027891	3311853	31.55%	2.983%
14	10.475	1266	1273	1283	rVB	2587909	4403782	41.96%	3.966%
15	10.610	1288	1296	1307	rBV	2307862	3900147	37.16%	3.512%
16	12.063	1537	1543	1551	rVB	38776	63143	0.60%	0.057%
17	13.745	1822	1829	1839	rBV	4085670	5665766	53.98%	5.102%
18	14.022	1869	1876	1888	rBV	4645093	6792369	64.71%	6.117%
19	14.328	1921	1928	1936	rBV	4165755	6085932	57.98%	5.481%
20	14.522	1953	1961	1980	rBV	1857150	2698542	25.71%	2.430%
21	15.322	2090	2097	2110	rBV	5784325	8433872	80.35%	7.595%
22	15.439	2110	2117	2134	rBV	1154764	1681017	16.02%	1.514%
23	15.563	2134	2138	2145	rVB2	28813	47235	0.45%	0.043%
24	16.751	2337	2340	2346	rBV5	8817	12440	0.12%	0.011%
25	16.857	2354	2358	2365	rVB2	11586	19535	0.19%	0.018%
26	17.075	2388	2395	2404	rBV	5054673	7096456	67.61%	6.391%
27	17.175	2405	2412	2428	rVV	6630946	9335190	88.94%	8.407%
28	19.033	2723	2728	2733	rBV	68183	97675	0.93%	0.088%
29	19.098	2735	2739	2744	rVV	64813	89091	0.85%	0.080%
30	19.469	2796	2802	2811	rBV	7478791	10496441	100.00%	9.453%
31	21.304	3108	3114	3126	rVB2	4495024	6581580	62.70%	5.927%
32	24.033	3570	3578	3601	rVB2	3105555	7404599	70.54%	6.668%
33	24.233	3604	3612	3633	rVB	2111106	5472154	52.13%	4.928%




Sum of corrected areas: 111041433

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031571.D
Acq On : 20 May 2024 14:20
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

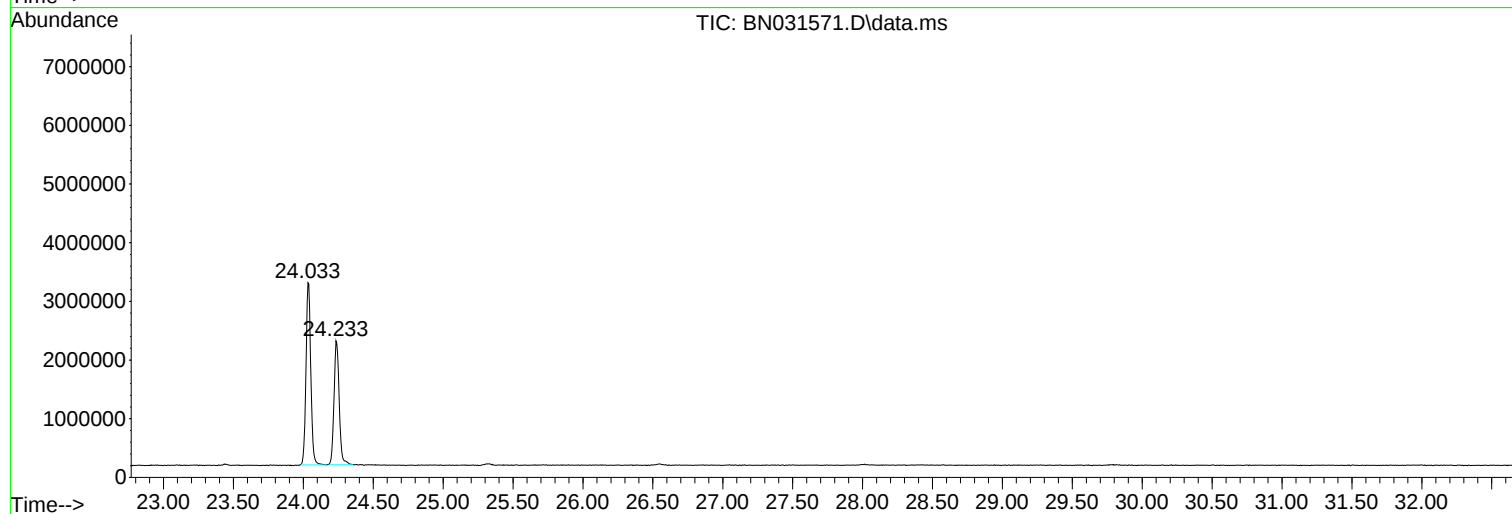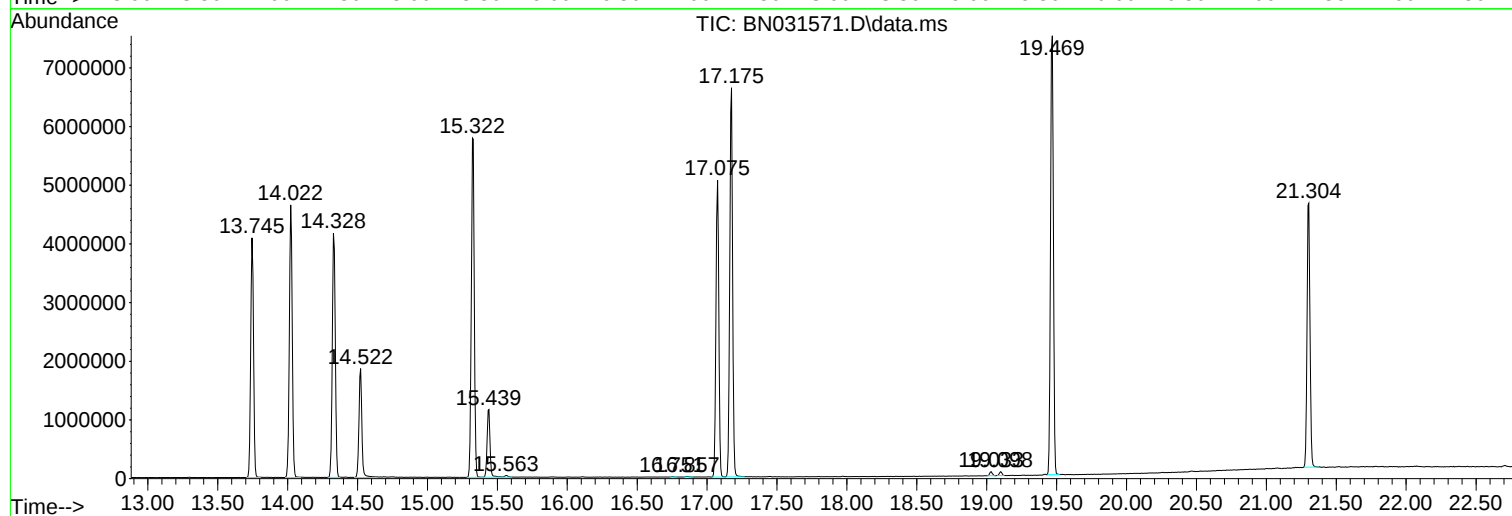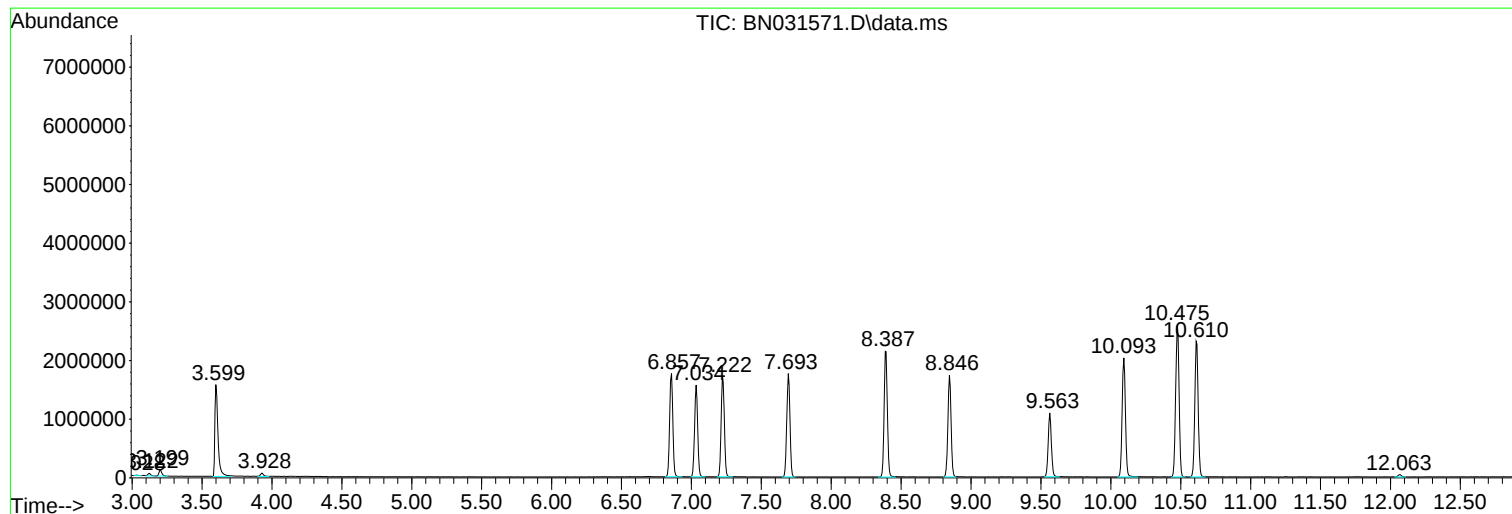

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031571.D
Acq On : 20 May 2024 14:20
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031571.D
Acq On : 20 May 2024 14:20
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc