

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031585.D
 Acq On : 21 May 2024 01:50
 Operator : MA/JU
 Sample : PB160987BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK987

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	5	7	14	rVB5	12384	19706	0.18%	0.014%
2	3.122	19	23	32	rVB	53004	84697	0.76%	0.061%
3	3.205	32	37	45	rVB	151640	203165	1.82%	0.146%
4	3.599	101	104	129	rVB	2060729	3028194	27.11%	2.183%
5	3.928	155	160	166	rVB	72646	105978	0.95%	0.076%
6	6.858	650	658	670	rBV	2457583	3846215	34.43%	2.773%
7	7.034	680	688	698	rVB	2060763	3229123	28.91%	2.328%
8	7.222	713	720	734	rBV	2370711	3860528	34.56%	2.783%
9	7.693	793	800	810	rVB	2433759	3848071	34.45%	2.774%
10	8.393	910	919	937	rBV	3077731	4915904	44.01%	3.544%
11	8.846	988	996	1012	rBV	2331796	3839919	34.38%	2.768%
12	9.563	1110	1118	1127	rBV	1782943	2814629	25.20%	2.029%
13	10.093	1199	1208	1224	rBV	2902159	4838094	43.31%	3.488%
14	10.475	1264	1273	1284	rVB	3535726	5954993	53.31%	4.293%
15	10.616	1287	1297	1311	rBV	3048969	5264220	47.13%	3.795%
16	12.069	1536	1544	1552	rVB	58928	99657	0.89%	0.072%
17	13.298	1749	1753	1758	rVB3	7998	11823	0.11%	0.009%
18	13.745	1821	1829	1839	rBV	5373682	7360913	65.90%	5.307%
19	14.022	1869	1876	1885	rBV	5856004	8943987	80.07%	6.448%
20	14.334	1920	1929	1939	rBV	5157688	7957236	71.24%	5.737%
21	14.522	1954	1961	1977	rBV	2468851	3642354	32.61%	2.626%
22	14.698	1985	1991	1994	rVB7	7391	13942	0.12%	0.010%
23	14.751	1994	2000	2005	rVB6	11559	17514	0.16%	0.013%
24	15.328	2091	2098	2106	rBV	7165186	10712867	95.91%	7.723%
25	15.439	2110	2117	2134	rBV	1684266	2382064	21.33%	1.717%
26	15.563	2134	2138	2143	rVB2	36518	54356	0.49%	0.039%
27	16.104	2227	2230	2238	rBV7	10108	18243	0.16%	0.013%
28	16.857	2352	2358	2366	rBV2	15627	29074	0.26%	0.021%
29	17.075	2388	2395	2404	rVB	6171754	8626984	77.24%	6.219%
30	17.175	2404	2412	2425	rBV	7863289	11169741	100.00%	8.053%
31	17.316	2431	2436	2443	rBV5	10414	18049	0.16%	0.013%
32	17.445	2454	2458	2464	rBV3	8905	15669	0.14%	0.011%
33	19.033	2723	2728	2733	rBV	87809	119665	1.07%	0.086%
34	19.098	2735	2739	2744	rVV	83352	109209	0.98%	0.079%
35	19.416	2789	2793	2795	rBV3	36753	40258	0.36%	0.029%
36	19.469	2796	2802	2810	rVV	8014799	10712635	95.91%	7.723%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031585.D
Acq On : 21 May 2024 01:50
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Title : SVOA CALIBRATION

37	20.463	2968	2971	2976	rBV3	41130	51341	0.46%	0.037%
38	21.304	3107	3114	3125	rBV2	4117049	6113097	54.73%	4.407%
39	24.039	3569	3579	3594	rBV2	3420363	8446624	75.62%	6.089%
40	24.239	3603	3613	3622	rBV2	2423224	6188442	55.40%	4.461%




Sum of corrected areas: 138709180

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031585.D
Acq On : 21 May 2024 01:50
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

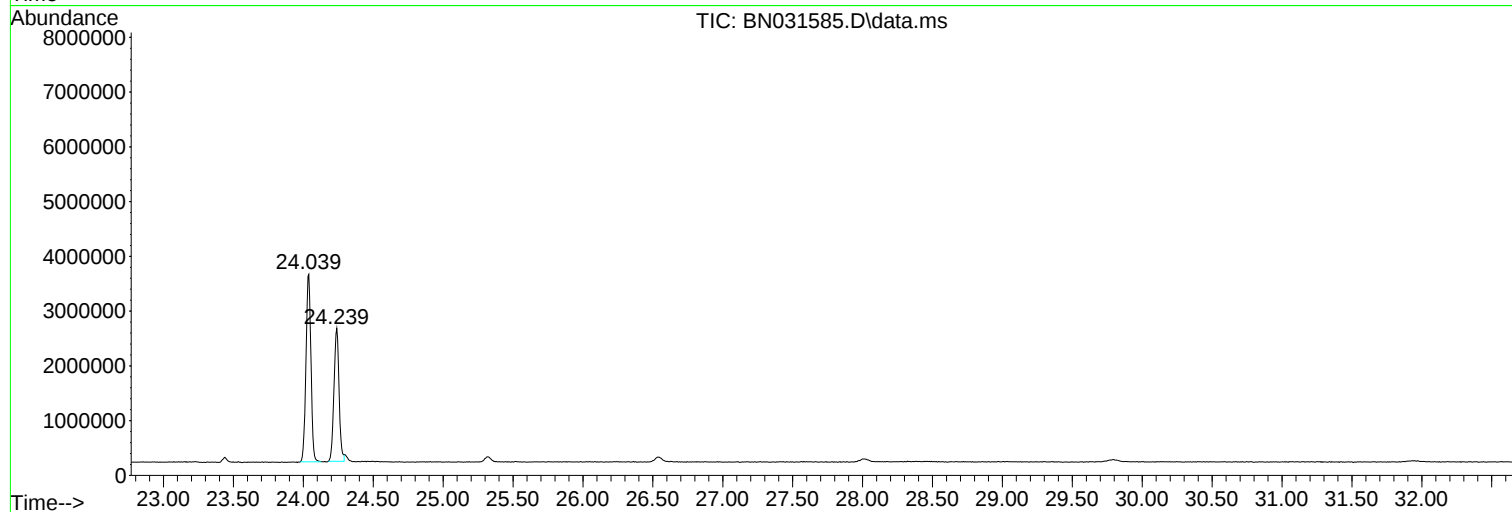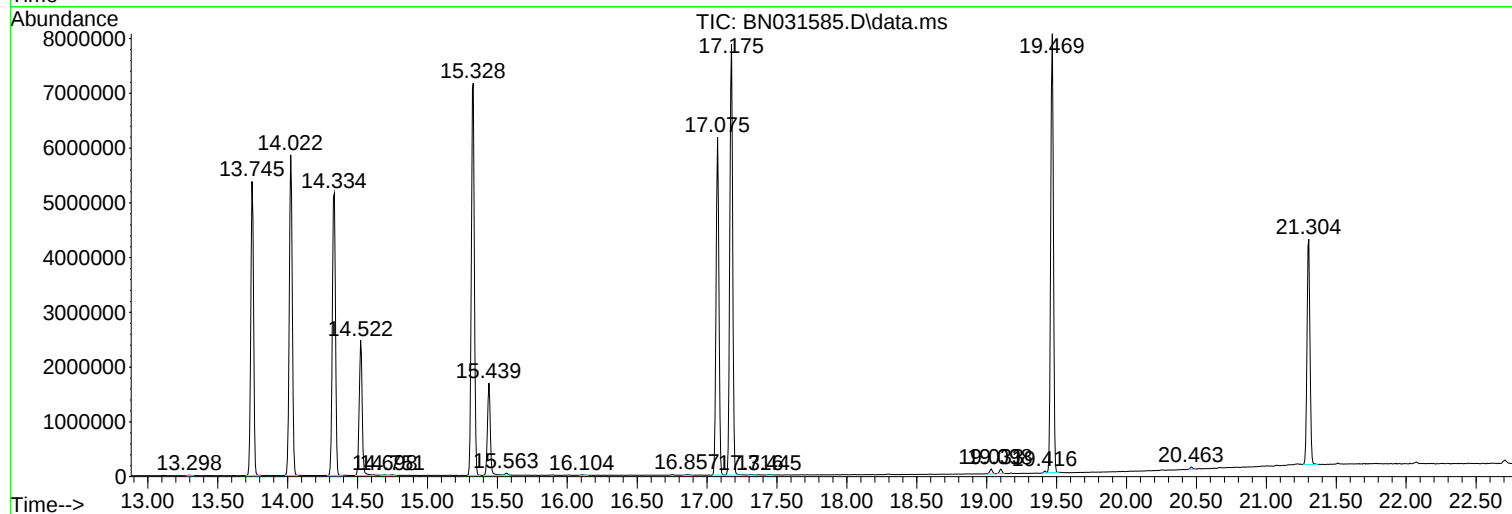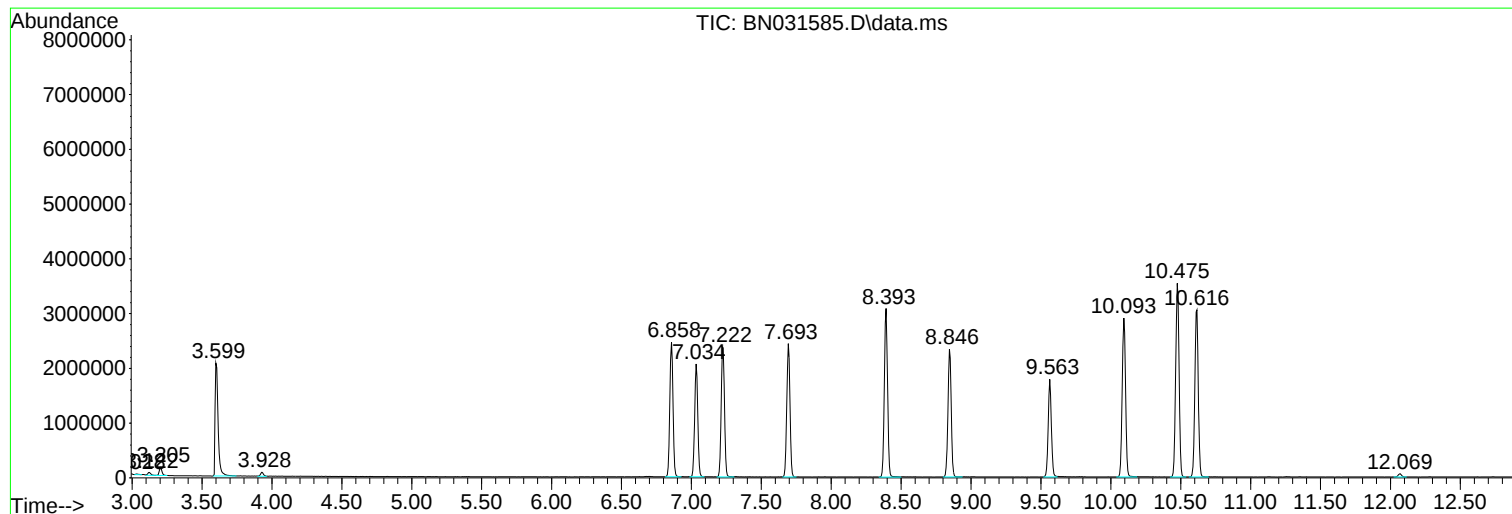

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031585.D
Acq On : 21 May 2024 01:50
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031585.D
Acq On : 21 May 2024 01:50
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------