

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031592.D
 Acq On : 21 May 2024 06:24
 Operator : MA/JU
 Sample : P2484-24
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	33	37	46	rVB	86498	128021	1.59%	0.124%
2	3.463	77	81	93	rBV	165105	250130	3.10%	0.243%
3	3.604	102	105	119	rBV	847343	1307332	16.21%	1.270%
4	3.928	155	160	168	rBV	33891	53910	0.67%	0.052%
5	4.246	211	214	219	rBV	29510	39401	0.49%	0.038%
6	4.840	309	315	320	rBV	100282	153836	1.91%	0.149%
7	5.193	370	375	379	rVB6	4993	8354	0.10%	0.008%
8	5.793	471	477	484	rVB	35333	58441	0.72%	0.057%
9	5.975	501	508	512	rVB10	6739	13470	0.17%	0.013%
10	6.857	651	658	669	rVB	1572544	2478906	30.74%	2.407%
11	7.034	681	688	703	rVB	1367840	2081721	25.81%	2.022%
12	7.222	713	720	728	rBV	1530179	2452305	30.41%	2.381%
13	7.293	728	732	740	rVB	43299	73862	0.92%	0.072%
14	7.693	791	800	807	rBV	2073236	3343044	41.45%	3.246%
15	7.763	807	812	818	rVB2	42652	69853	0.87%	0.068%
16	8.392	911	919	927	rBV	1962813	3166674	39.27%	3.075%
17	8.845	988	996	1007	rBV	1496913	2459522	30.50%	2.388%
18	9.010	1019	1024	1032	rVB	7345	15574	0.19%	0.015%
19	9.263	1063	1067	1073	rVB2	18392	27747	0.34%	0.027%
20	9.410	1087	1092	1100	rVB	165971	255234	3.16%	0.248%
21	9.563	1110	1118	1129	rBV	1043080	1701282	21.10%	1.652%
22	9.787	1148	1156	1161	rBV8	6686	13457	0.17%	0.013%
23	10.092	1201	1208	1221	rBV	1887970	3114069	38.61%	3.024%
24	10.257	1230	1236	1243	rBV	59158	95502	1.18%	0.093%
25	10.475	1264	1273	1282	rBV	3148913	5211438	64.62%	5.061%
26	10.610	1288	1296	1305	rBV	1990055	3367554	41.76%	3.270%
27	11.022	1360	1366	1372	rVB	52643	80710	1.00%	0.078%
28	11.216	1391	1399	1411	rBV	255741	444924	5.52%	0.432%
29	11.351	1417	1422	1426	rBV5	6224	9978	0.12%	0.010%
30	12.063	1537	1543	1550	rVB2	38661	73594	0.91%	0.071%
31	13.116	1717	1722	1726	rBV8	5210	9093	0.11%	0.009%
32	13.163	1726	1730	1736	rVV4	13065	19576	0.24%	0.019%
33	13.228	1736	1741	1744	rVV6	6084	8654	0.11%	0.008%
34	13.298	1748	1753	1759	rVB6	9647	15769	0.20%	0.015%
35	13.551	1790	1796	1799	rBV7	7373	9108	0.11%	0.009%
36	13.745	1822	1829	1839	rBV	3447114	4624608	57.34%	4.491%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
 Data File : BN031592.D
 Acq On : 21 May 2024 06:24
 Operator : MA/JU
 Sample : P2484-24
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
 Title : SVOA CALIBRATION

37	14.022	1865	1876	1887	rBV	4080534	6084151	75.44%	5.908%
38	14.239	1910	1913	1917	rVB3	8176	9885	0.12%	0.010%
39	14.327	1920	1928	1938	rVV	4764994	7165764	88.85%	6.959%
40	14.522	1953	1961	1966	rBV	1360863	2125261	26.35%	2.064%
41	14.686	1987	1989	1996	rVB8	7306	9438	0.12%	0.009%
42	14.751	1996	2000	2006	rBV5	17687	29051	0.36%	0.028%
43	15.139	2061	2066	2071	rBV4	14653	25555	0.32%	0.025%
44	15.192	2071	2075	2082	rVB4	9402	14124	0.18%	0.014%
45	15.322	2090	2097	2105	rBV	4972089	7167914	88.88%	6.961%
46	15.439	2110	2117	2132	rBV	750494	1076768	13.35%	1.046%
47	15.563	2134	2138	2143	rVV3	21351	29989	0.37%	0.029%
48	15.886	2189	2193	2199	rBV7	10709	21001	0.26%	0.020%
49	16.051	2219	2221	2224	rBV3	8590	11452	0.14%	0.011%
50	16.480	2290	2294	2300	rVB8	10179	14828	0.18%	0.014%
51	16.751	2338	2340	2345	rVB4	7236	8770	0.11%	0.009%
52	16.851	2352	2357	2362	rBV3	19676	36672	0.45%	0.036%
53	17.004	2380	2383	2387	rVB5	16197	20808	0.26%	0.020%
54	17.074	2387	2395	2402	rBV	5685248	8064653	100.00%	7.832%
55	17.174	2405	2412	2423	rVV	5202975	7444979	92.32%	7.230%
56	17.268	2423	2428	2432	rVV5	28531	49164	0.61%	0.048%
57	17.310	2432	2435	2441	rVV6	17179	31653	0.39%	0.031%
58	17.368	2442	2445	2452	rVB4	10718	19915	0.25%	0.019%
59	17.580	2479	2481	2486	rVB5	8423	9975	0.12%	0.010%
60	17.757	2507	2511	2516	rVB2	28264	40373	0.50%	0.039%
61	17.845	2522	2526	2529	rBV6	12847	19285	0.24%	0.019%
62	17.916	2534	2538	2542	rBV7	8243	17700	0.22%	0.017%
63	17.974	2543	2548	2558	rBV	432632	599462	7.43%	0.582%
64	18.292	2596	2602	2609	rBV10	19919	43084	0.53%	0.042%
65	18.415	2619	2623	2626	rVB5	15942	20894	0.26%	0.020%
66	18.845	2692	2696	2700	rBV6	20651	29225	0.36%	0.028%
67	19.027	2723	2727	2733	rVB	59183	81707	1.01%	0.079%
68	19.098	2735	2739	2744	rBV	62241	107832	1.34%	0.105%
69	19.262	2763	2767	2773	rBV	132632	185712	2.30%	0.180%
70	19.415	2790	2793	2795	rBV2	43703	41218	0.51%	0.040%
71	19.462	2795	2801	2810	rVV	5297657	7395723	91.71%	7.182%
72	20.033	2895	2898	2900	rVB2	31060	31244	0.39%	0.030%
73	20.462	2968	2971	2974	rBV2	45268	48062	0.60%	0.047%
74	20.527	2979	2982	2985	rVB2	59042	68667	0.85%	0.067%
75	20.992	3057	3061	3071	rBV2	340446	561001	6.96%	0.545%
76	21.298	3107	3113	3123	rVB2	3931470	5963738	73.95%	5.791%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031592.D
Acq On : 21 May 2024 06:24
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Title : SVOA CALIBRATION

77	22.874	3376	3381	3387	rVB	220369	380786	4.72%	0.370%
78	24.033	3569	3578	3589	rBV2	2168731	5027010	62.33%	4.882%
79	24.233	3603	3612	3630	rVB	2207941	5605551	69.51%	5.444%




Sum of corrected areas: 102976697

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031592.D
Acq On : 21 May 2024 06:24
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

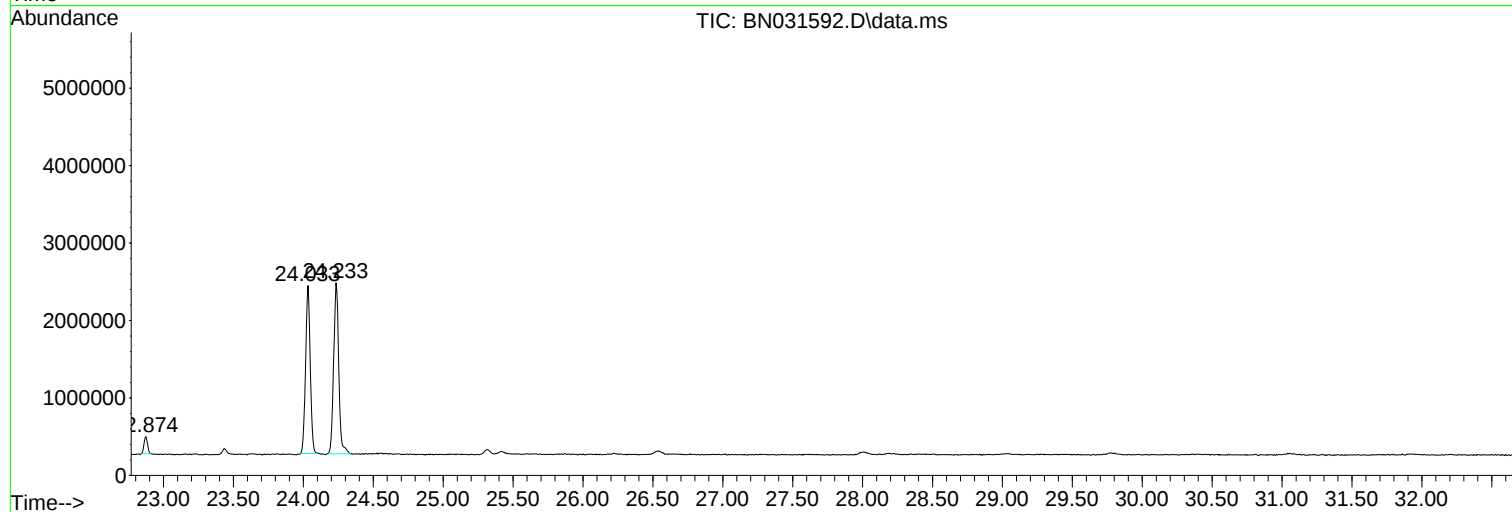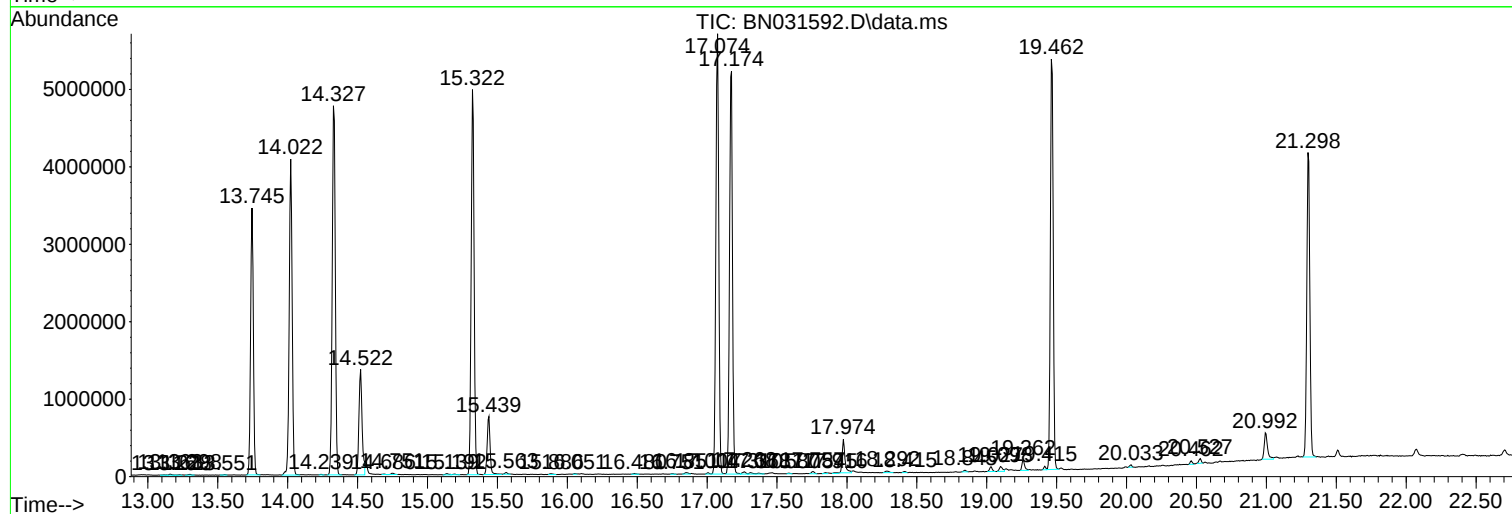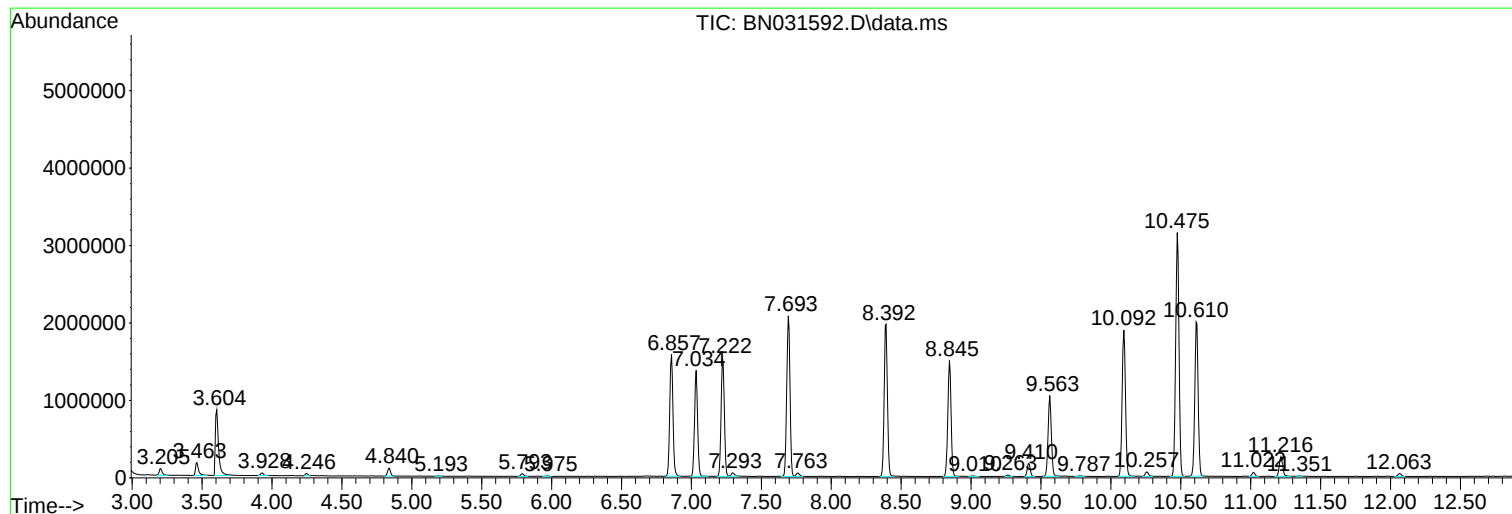

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031592.D
Acq On : 21 May 2024 06:24
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052024\
Data File : BN031592.D
Acq On : 21 May 2024 06:24
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN051524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc