
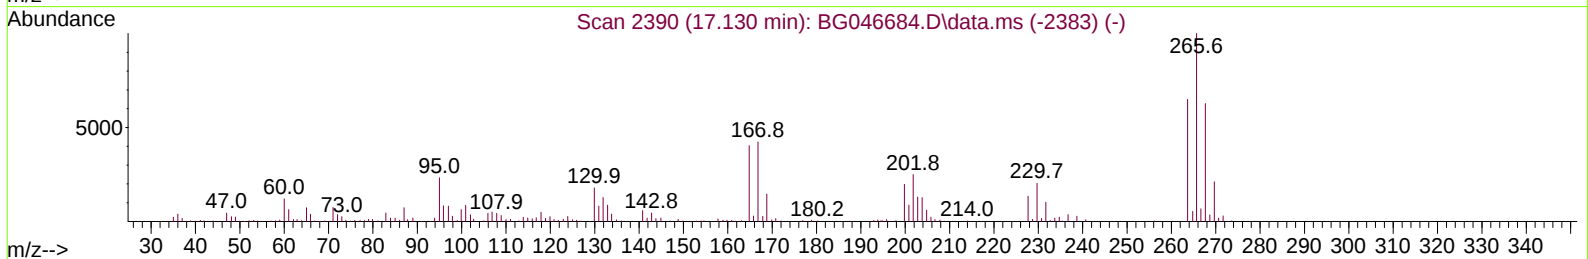
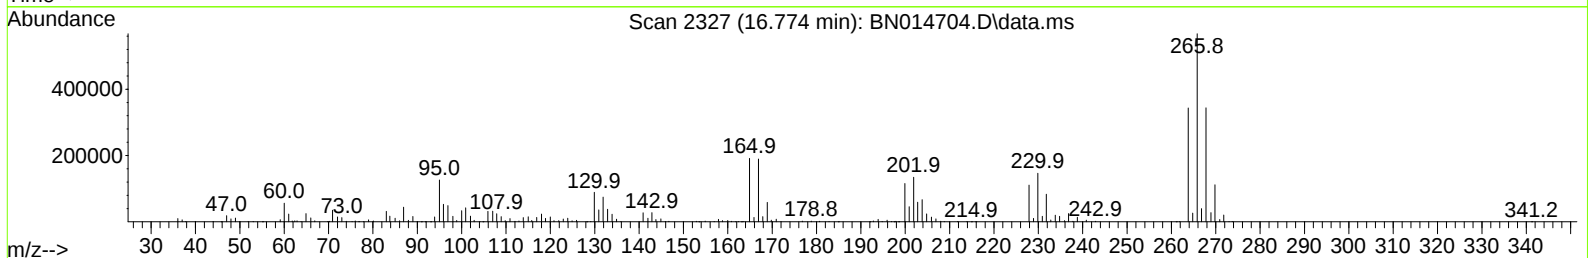


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014704.D
 Acq On : 21 May 2021 22:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 07:55:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

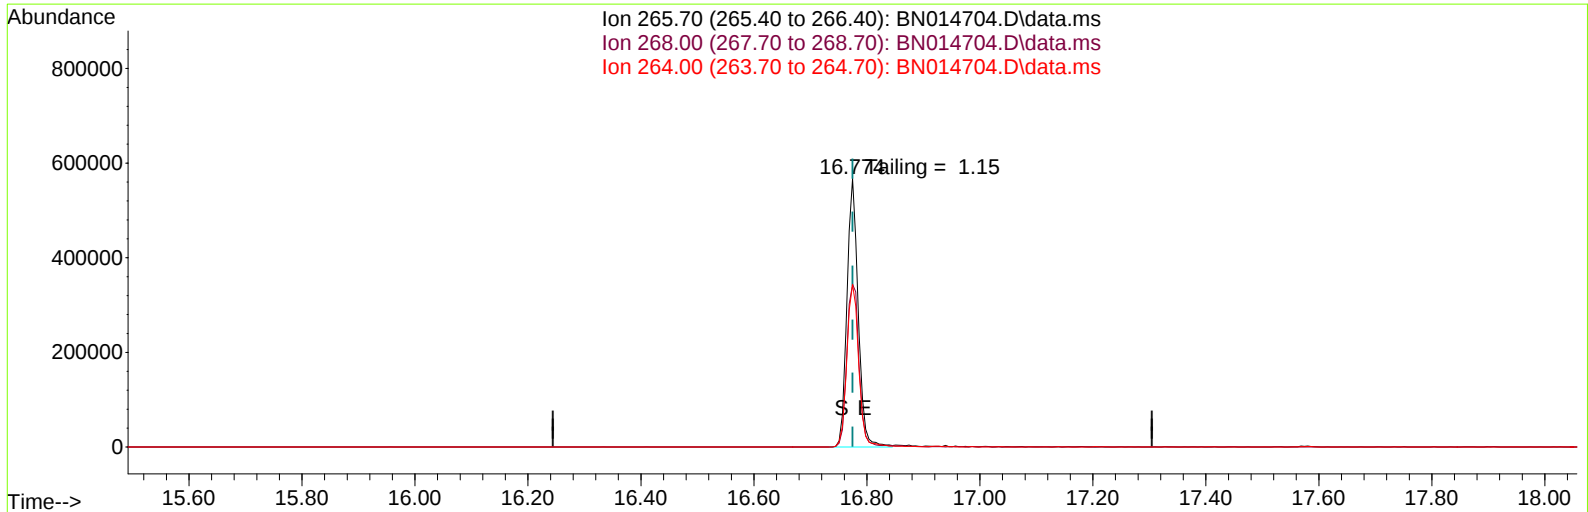

TIC: BN014704.D\data.ms

(70) Pentachlorophenol (C)




16.774min (0.000) 21212.87 ng

response 785088

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.66
264.00	61.60	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
Data File : BN014704.D
Acq On : 21 May 2021 22:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 22 07:55:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

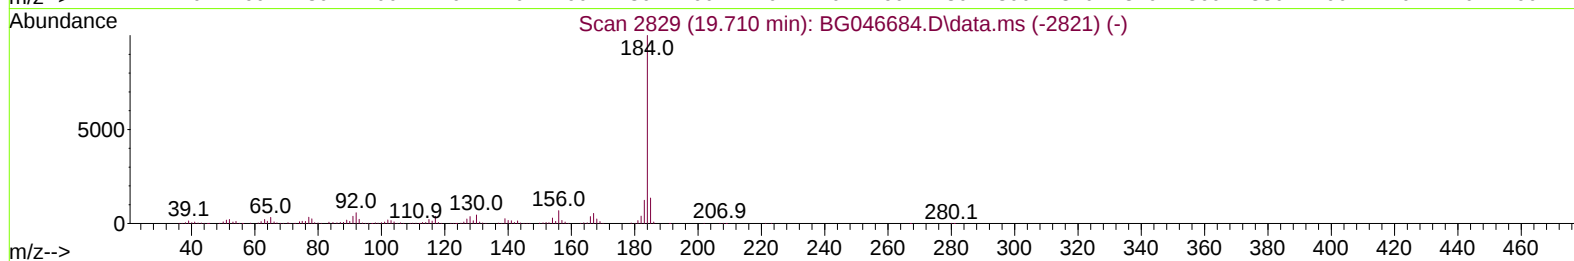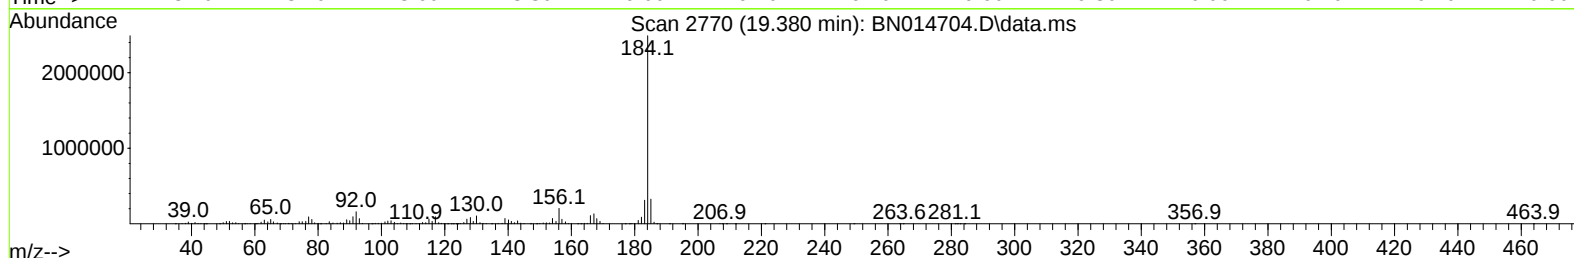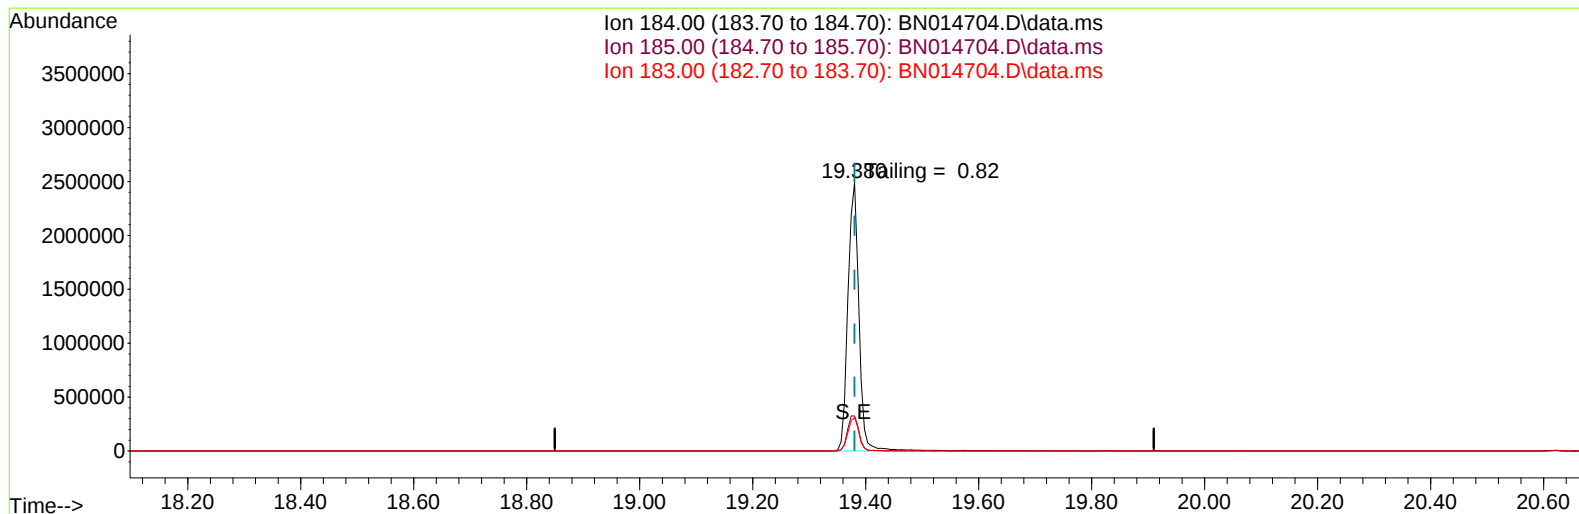

TIC: BN014704.D\data.ms

(77) Benzidine

19.380min (0.000) 0.00 ng

response 3372513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.09
183.00	13.20	12.50
0.00	0.00	0.00