

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014712.D
 Acq On : 22 May 2021 04:06
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

mohammad
 5/24/2021 2:37:22 PM

Quant Time: May 22 04:37:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 21 11:30:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.724	152	860	0.40	ng	# 0.00
7) Naphthalene-d8	10.505	136	3102	0.40	ng	# 0.00
13) Acenaphthene-d10	14.371	164	2047	0.40	ng	0.00
19) Phenanthrene-d10	17.116	188	4472	0.40	ng	# 0.00
29) Chrysene-d12	21.321	240	5380	0.40	ng	# 0.00
35) Perylene-d12	23.582	264	5784	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.324	112	1085	0.48	ng	0.00
5) Phenol-d6	6.895	99	1464	0.48	ng	0.00
8) Nitrobenzene-d5	8.870	82	1227	0.46	ng	0.00
11) 2-Methylnaphthalene-d10	12.102	152	3084	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.869	330	496	0.52	ng	0.00
15) 2-Fluorobiphenyl	12.989	172	3329	0.44	ng	0.00
27) Fluoranthene-d10	19.156	212	7807	0.39	ng	0.00
31) Terphenyl-d14	19.761	244	5447	0.43	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.279	88	527	0.40	ng	92
3) n-Nitrosodimethylamine	3.649	42	155m	0.36	ng	
6) bis(2-Chloroethyl)ether	7.153	93	1142	0.45	ng	# 87
9) Naphthalene	10.556	128	3454	0.42	ng	# 93
10) Hexachlorobutadiene	10.847	225	920	0.47	ng	# 100
12) 2-Methylnaphthalene	12.177	142	2437	0.41	ng	# 91
16) Acenaphthylene	14.080	152	3302	0.44	ng	98
17) Acenaphthene	14.422	154	2310	0.41	ng	99
18) Fluorene	15.425	166	3056	0.41	ng	99
20) 4,6-Dinitro-2-methylph...	15.501	198	225	0.46	ng	# 1
21) 4-Bromophenyl-phenylether	16.312	248	1248	0.46	ng	# 78
22) Hexachlorobenzene	16.434	284	1379	0.48	ng	91
23) Atrazine	16.580	200	751	0.43	ng	# 91
24) Pentachlorophenol	16.775	266	459	0.48	ng	# 51
25) Phenanthrene	17.164	178	5093	0.42	ng	98
26) Anthracene	17.249	178	4325	0.42	ng	100
28) Fluoranthene	19.185	202	6265	0.39	ng	98
30) Pyrene	19.553	202	6346	0.43	ng	98
32) Benzo(a)anthracene	21.300	228	6722	0.43	ng	98
33) Chrysene	21.353	228	7240	0.44	ng	98
34) Bis(2-ethylhexyl)phtha...	21.236	149	2196	0.51	ng	# 78
36) Indeno(1,2,3-cd)pyrene	25.869	276	9503	0.41	ng	# 88
37) Benzo(b)fluoranthene	22.901	252	8029	0.41	ng	97
38) Benzo(k)fluoranthene	22.946	252	8213m	0.40	ng	
39) Benzo(a)pyrene	23.483	252	7530	0.45	ng	# 92
40) Dibenzo(a,h)anthracene	25.882	278	8061	0.41	ng	# 93
41) Benzo(g,h,i)perylene	26.564	276	8048	0.42	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
Data File : BN014712.D
Acq On : 22 May 2021 04:06
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM


Quant Time: May 22 04:37:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 21 11:30:28 2021
Response via : Initial Calibration

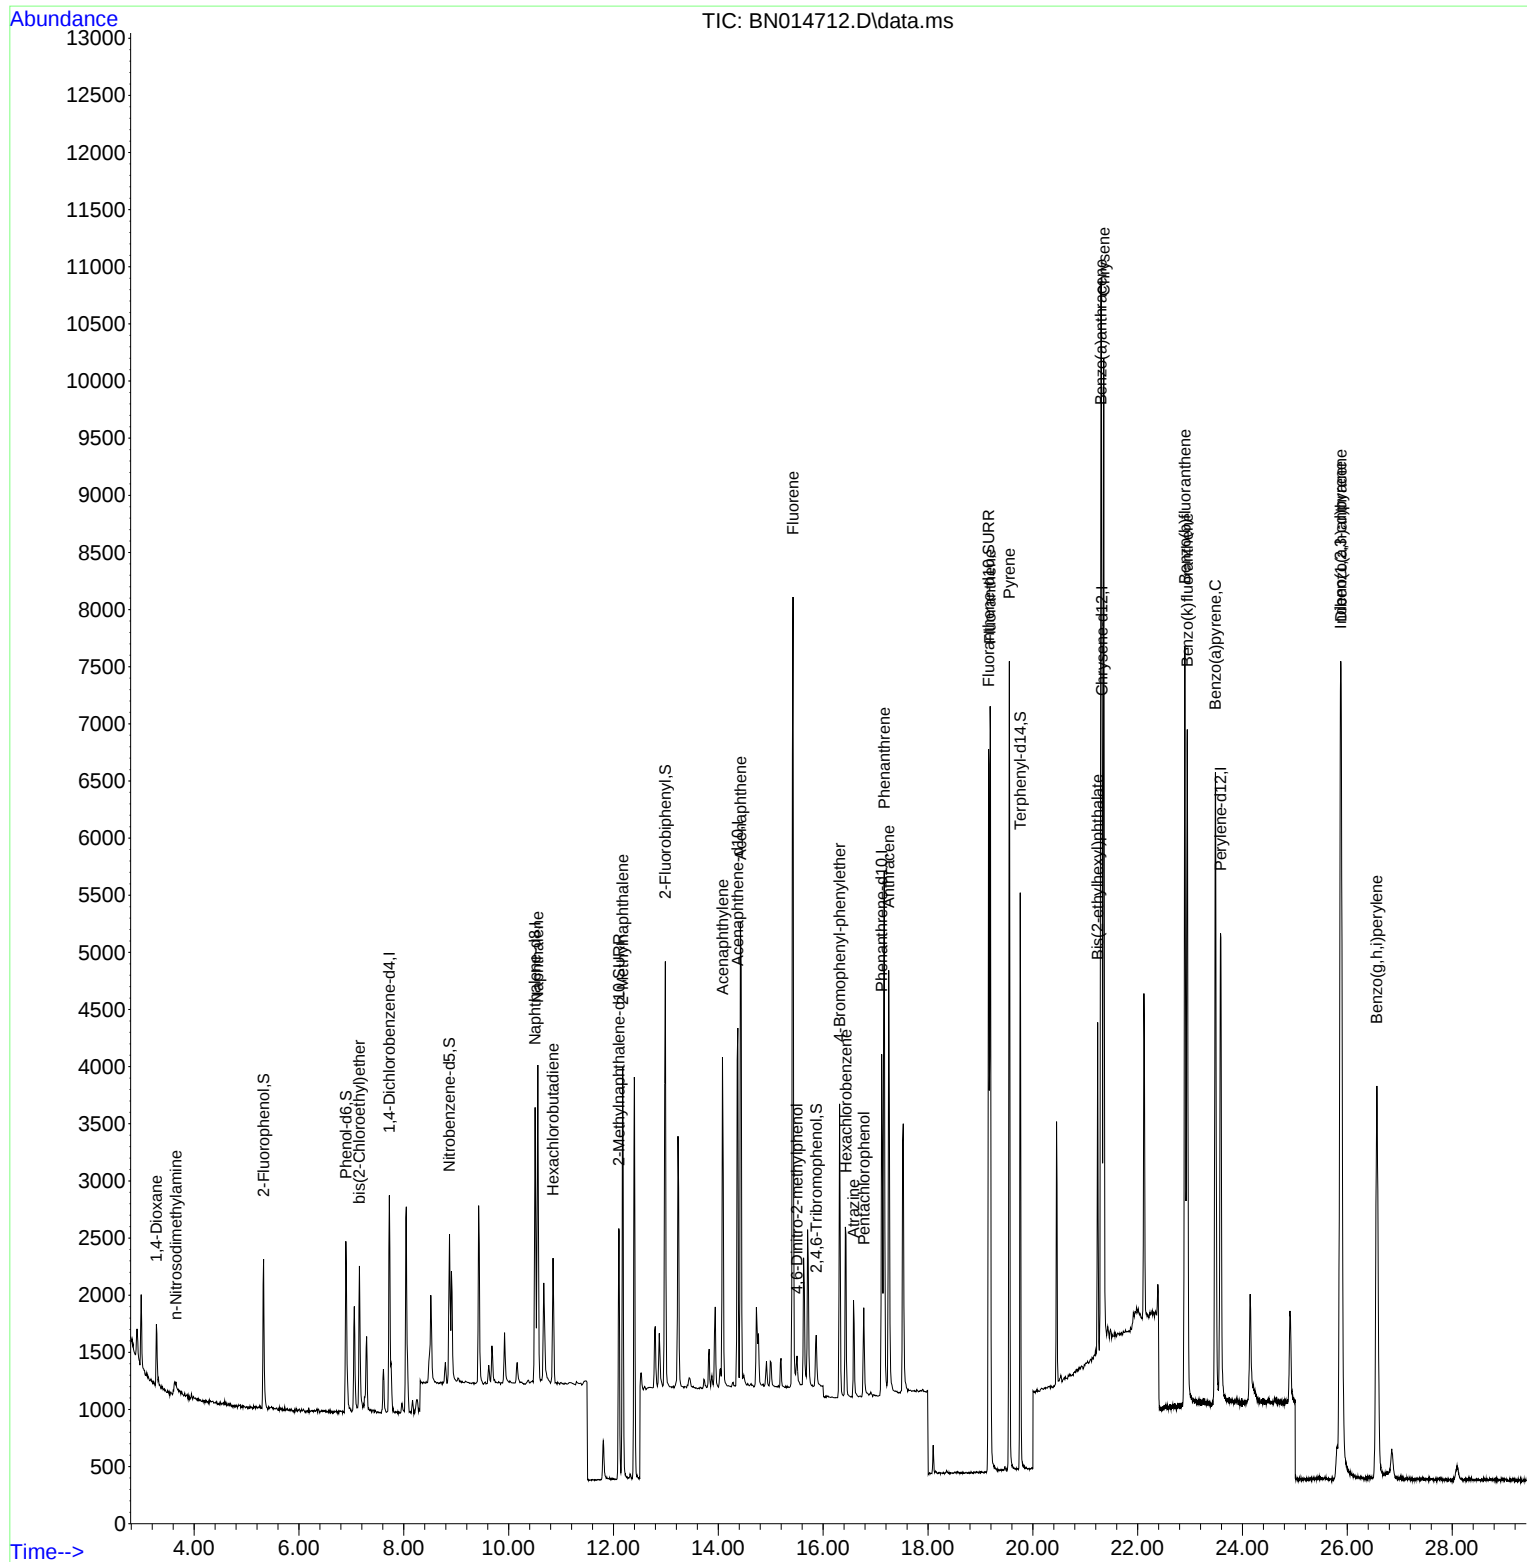



#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.724 min Scan# 614
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

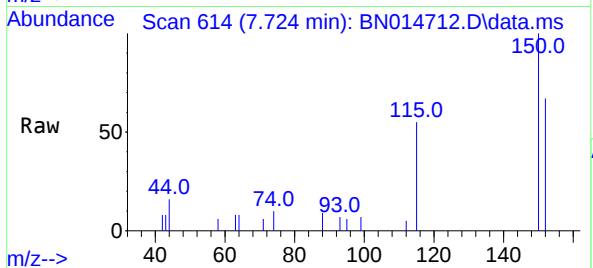


Tgt Ion: 152 Resp: 860
Ion Ratio Lower Upper
152 100
150 148.7 123.8 185.8
115 81.5 47.0 70.4#

Manual Integrations
APPROVED



mohammad
5/24/2021 2:37:22 PM

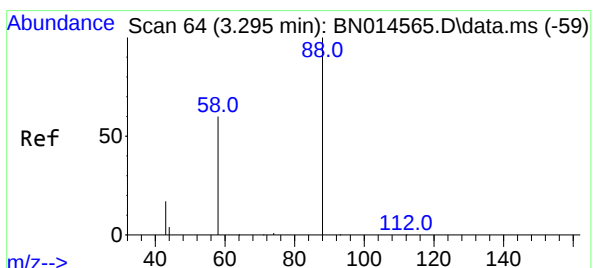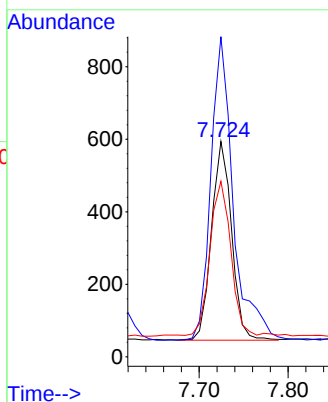


#2
1,4-Dioxane
Concen: 0.40 ng
RT: 3.279 min Scan# 62
Delta R.T. -0.008 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06



Tgt Ion: 88 Resp: 527
Ion Ratio Lower Upper
88 100
58 49.5 44.4 66.6
43 16.3 15.9 23.9

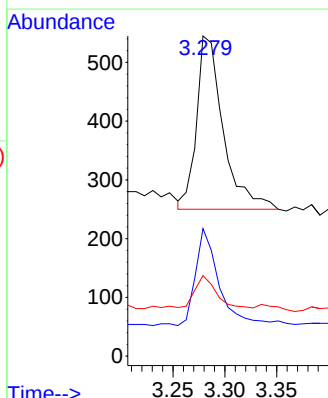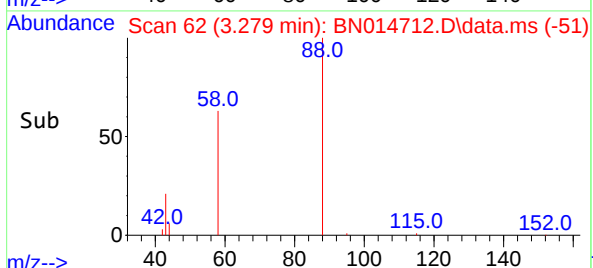

Abundance Scan 107 (3.641 min): BN014565.D\data.ms (-10

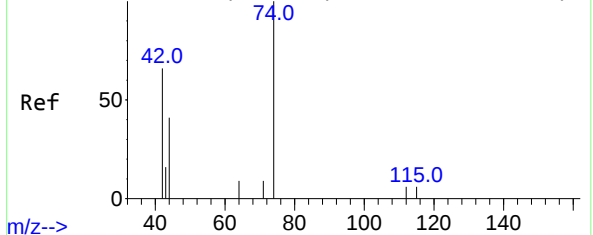





#3
n-Nitrosodimethylamine
Concen: 0.36 ng m
RT: 3.649 min Scan# 108
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	42	Resp:	155
Ion	Ratio	Lower	Upper
42	100		
74	220.0	175.1	262.7
44	18.1	7.5	11.3#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM

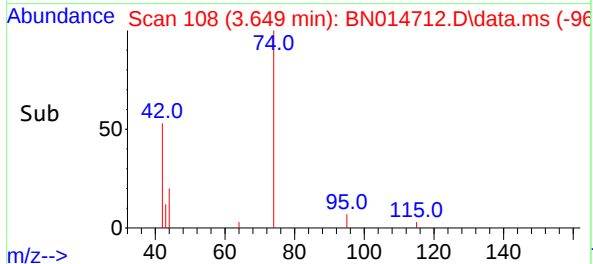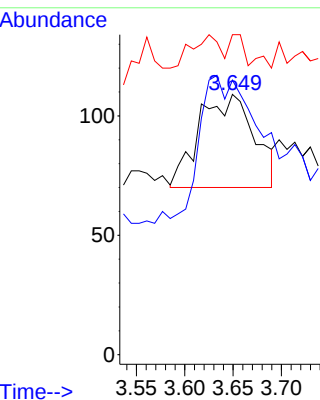

#4
2-Fluorophenol
Concen: 0.48 ng
RT: 5.324 min Scan# 316
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	112	Resp:	1085
Ion	Ratio	Lower	Upper
112	100		
64	57.6	41.8	62.6
63	29.9	22.0	33.0

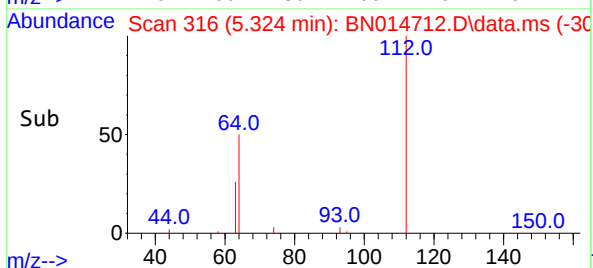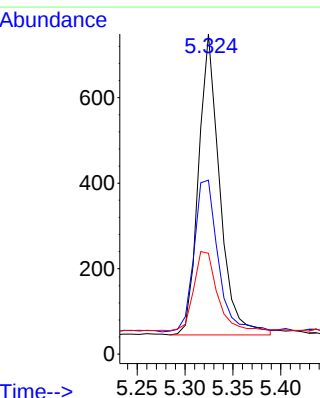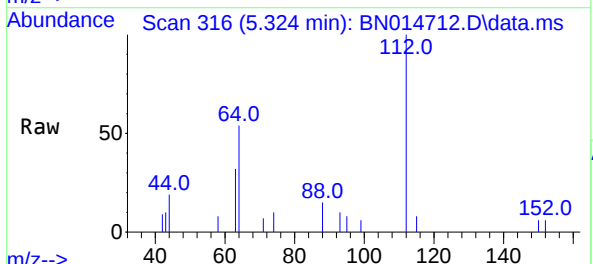







#5
Phenol-d6
Concen: 0.48 ng
RT: 6.895 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	99	Resp:	1464
Ion	Ratio	Lower	Upper
99	100		
42	12.4	13.2	19.8#
71	46.8	26.2	39.2#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM



#6
bis(2-Chloroethyl)ether
Concen: 0.45 ng
RT: 7.153 min Scan# 543
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	93	Resp:	1142
Ion	Ratio	Lower	Upper
93	100		
63	57.4	58.0	87.0#
95	33.4	27.0	40.6

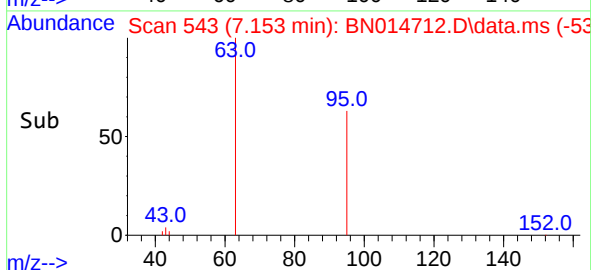

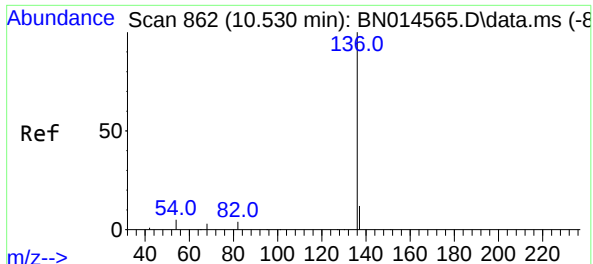





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.505 min Scan# 860
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	136	Resp:	3102
Ion	Ratio	Lower	Upper
136	100		
137	13.4	8.9	13.3#
54	8.6	3.8	5.8#
68	8.0	3.8	5.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM



#8
Nitrobenzene-d5
Concen: 0.46 ng
RT: 8.870 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	82	Resp:	1227
Ion	Ratio	Lower	Upper
82	100		
128	34.7	29.5	44.3
54	42.5	36.9	55.3

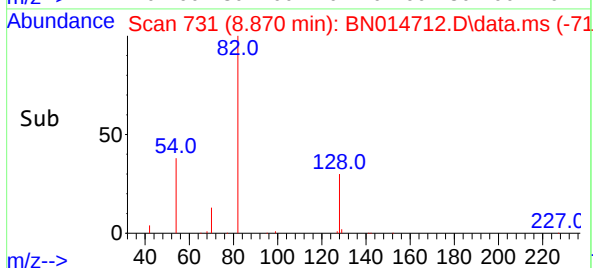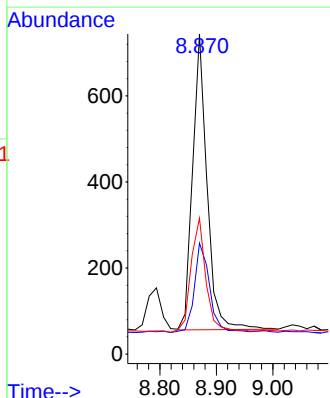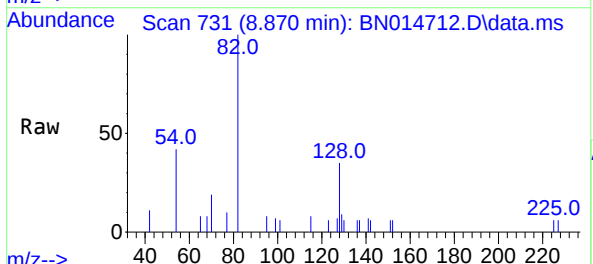

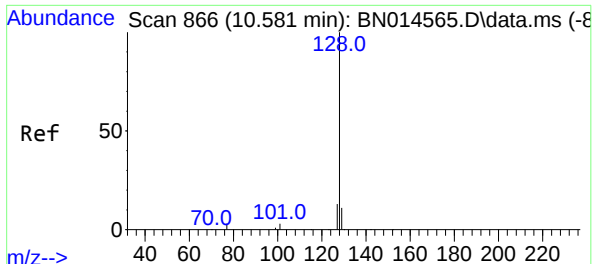





#9
Naphthalene
Concen: 0.42 ng
RT: 10.556 min Scan# 864
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	128	Resp:	3454
Ion Ratio	Lower	Upper	
128	100		
129	13.3	9.0	13.4
127	16.1	10.4	15.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM

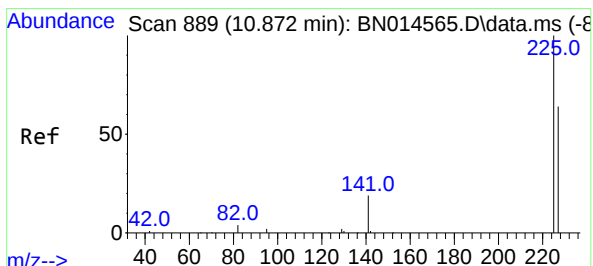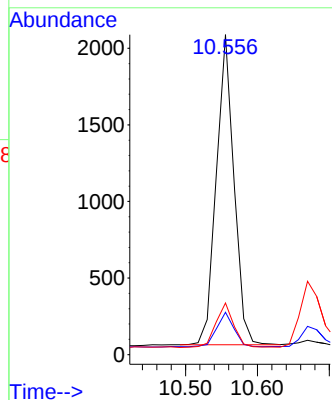

#10
Hexachlorobutadiene
Concen: 0.47 ng
RT: 10.847 min Scan# 887
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	225	Resp:	920
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.4	50.9	76.3

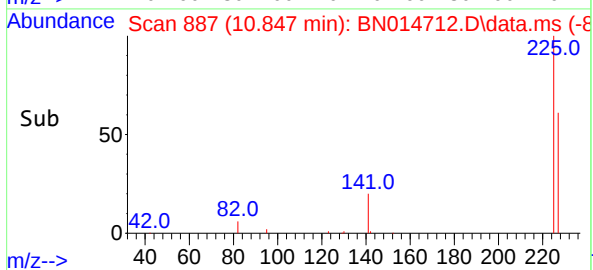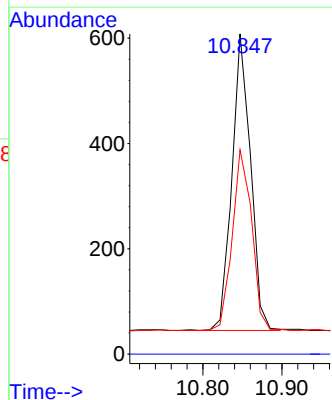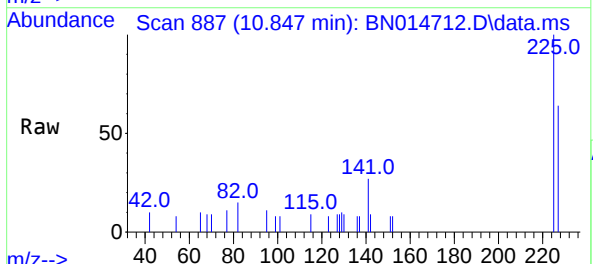







#11
2-Methylnaphthalene-d10
Concen: 0.41 ng
RT: 12.102 min Scan# 1073
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:152 Resp: 3084
Ion Ratio Lower Upper
152 100
151 21.1 16.2 24.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM



#12
2-Methylnaphthalene
Concen: 0.41 ng
RT: 12.177 min Scan# 1090
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:142 Resp: 2437
Ion Ratio Lower Upper
142 100
141 87.8 70.2 105.4
115 51.3 26.7 40.1#

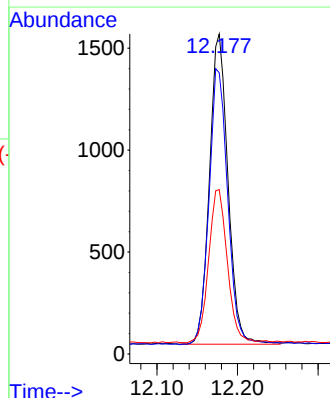







#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.371 min Scan# 1311
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:164 Resp: 2047
Ion Ratio Lower Upper
164 100
162 102.9 78.6 118.0
160 47.2 35.8 53.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM

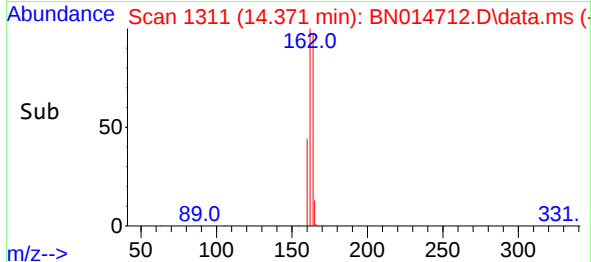


#14
2,4,6-Tribromophenol
Concen: 0.52 ng
RT: 15.869 min Scan# 1429
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:330 Resp: 496
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 23.6 27.0 40.4#

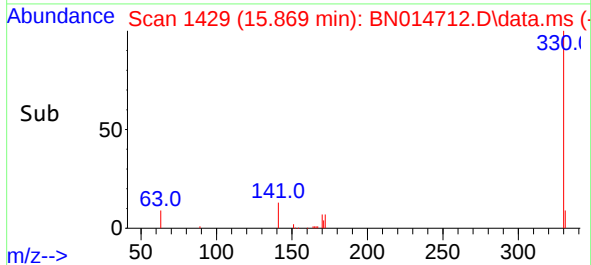

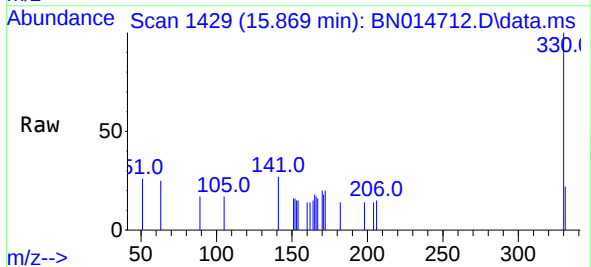


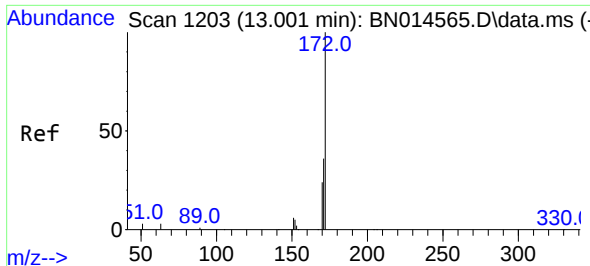


#15
2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.989 min Scan# 1202
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

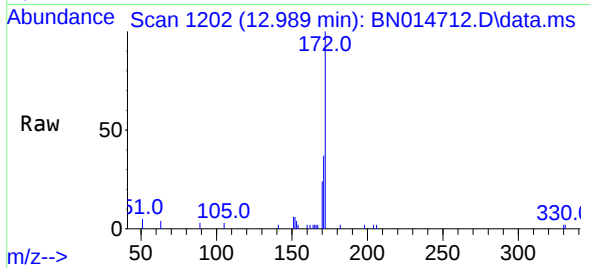



Tgt Ion:172 Resp: 3329
Ion Ratio Lower Upper
172 100
171 37.0 27.1 40.7
170 24.4 18.3 27.5

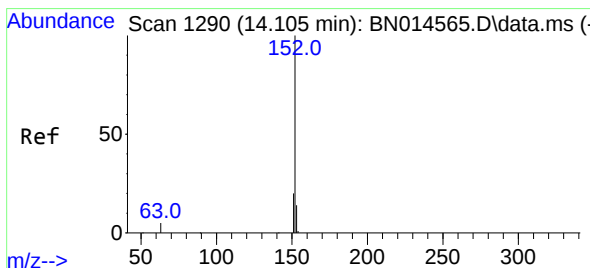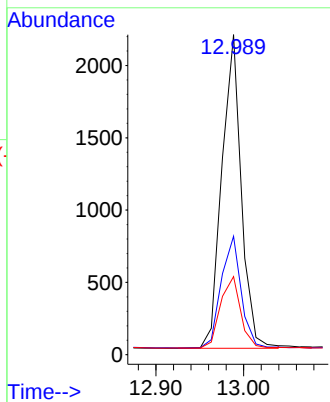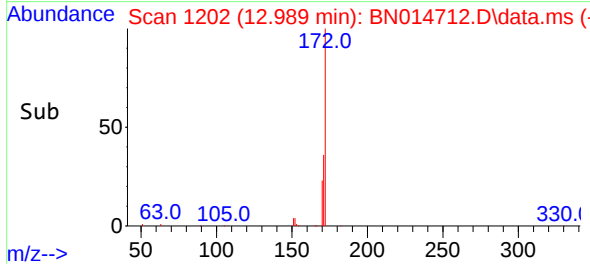

#16
Acenaphthylene
Concen: 0.44 ng
RT: 14.080 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

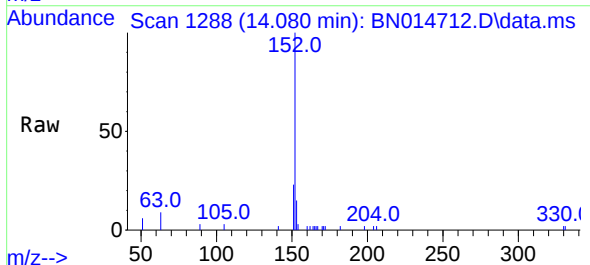


Tgt Ion:152 Resp: 3302
Ion Ratio Lower Upper
152 100
151 20.8 15.6 23.4
153 13.2 10.5 15.7

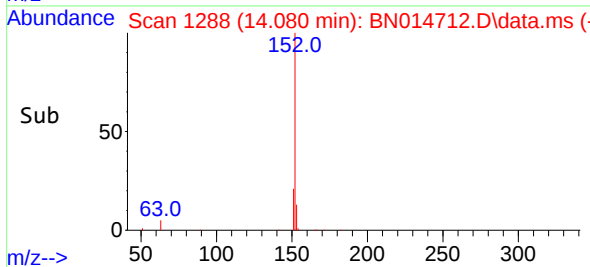

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM

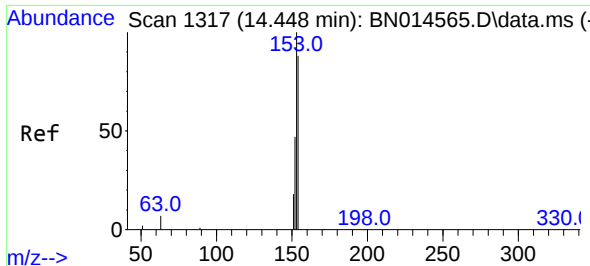

#17
Acenaphthene
Concen: 0.41 ng
RT: 14.422 min Scan# 1315
Delta R.T. -0.013 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

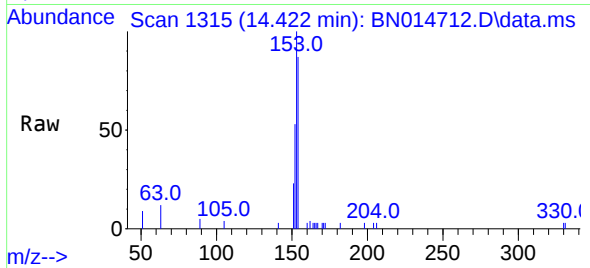


Tgt Ion:154 Resp: 2310
Ion Ratio Lower Upper
154 100
153 113.8 90.2 135.4
152 57.2 46.2 69.2

Manual Integrations
APPROVED



mohammad
5/24/2021 2:37:22 PM

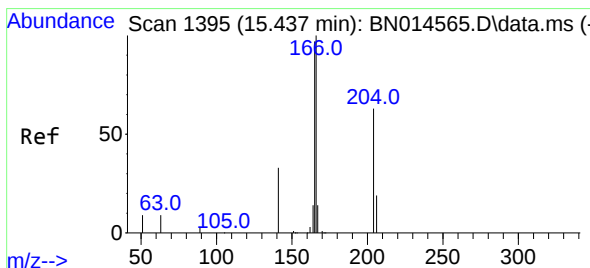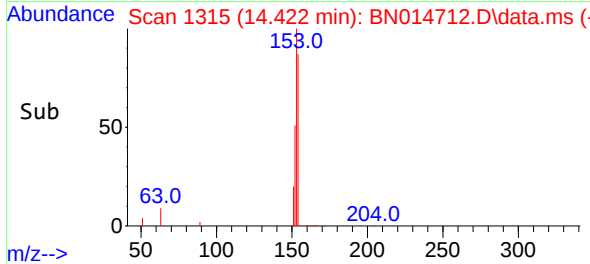


#18
Fluorene
Concen: 0.41 ng
RT: 15.425 min Scan# 1394
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

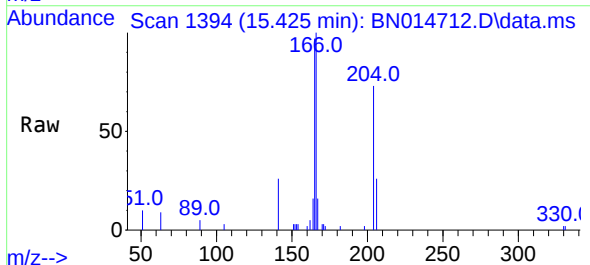


Tgt Ion:166 Resp: 3056
Ion Ratio Lower Upper
166 100
165 98.9 78.4 117.6
167 13.3 10.7 16.1

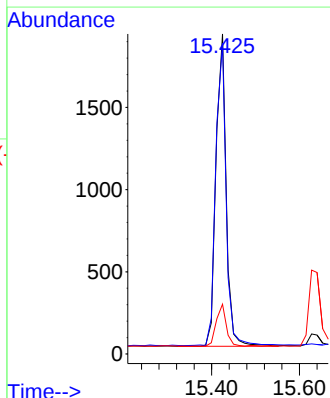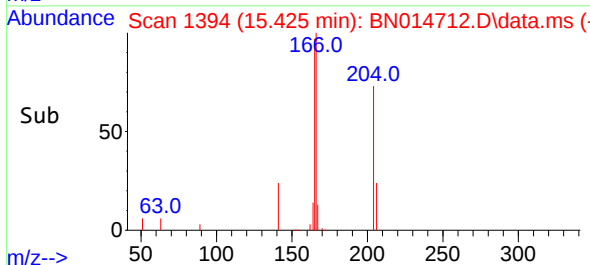



#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.116 min Scan# 1531
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:188 Resp: 4472
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.2 5.2 7.8#

Manual Integrations
APPROVED



mohammad
5/24/2021 2:37:22 PM

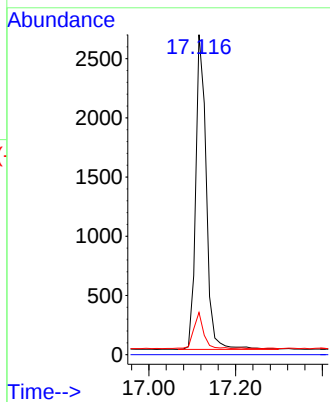


#20
4,6-Dinitro-2-methylphenol
Concen: 0.46 ng
RT: 15.501 min Scan# 1400
Delta R.T. -0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

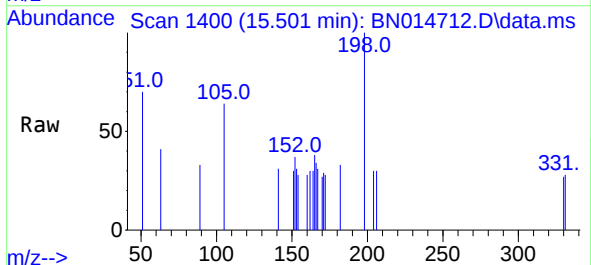


Tgt Ion:198 Resp: 225
Ion Ratio Lower Upper
198 100
51 69.9 865.3 1297.9#
105 64.5 93.6 140.4#



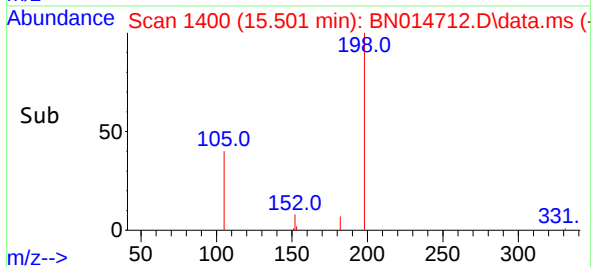


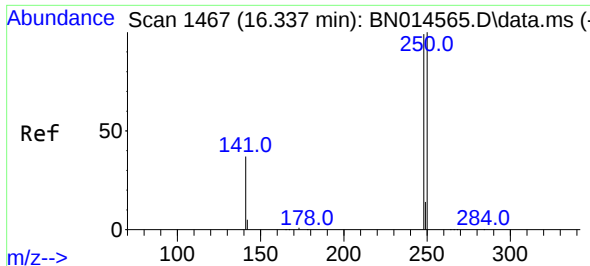


#21
4-Bromophenyl-phenylether
Concen: 0.46 ng
RT: 16.312 min Scan# 1465
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

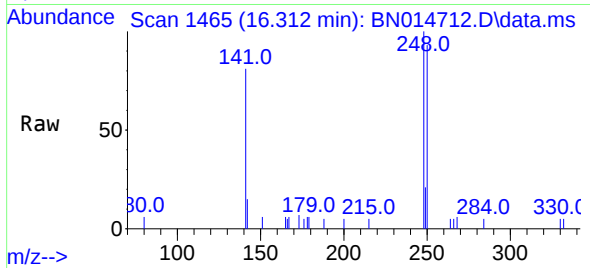



Tgt Ion:248 Resp: 1248
Ion Ratio Lower Upper
248 100
250 93.3 80.5 120.7
141 81.5 37.2 55.8#

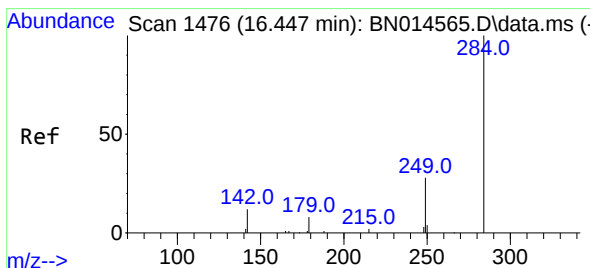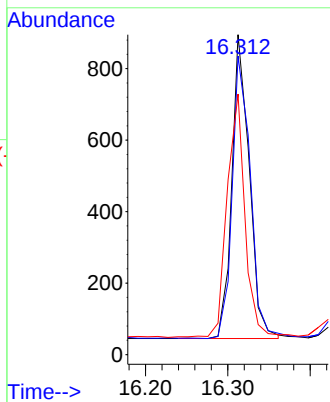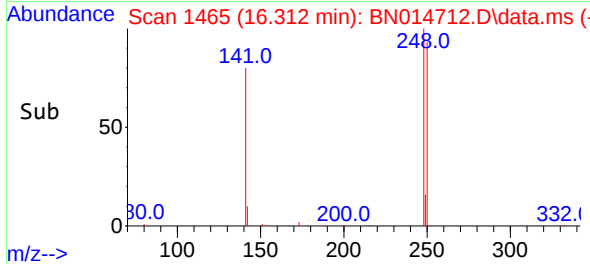

#22
Hexachlorobenzene
Concen: 0.48 ng
RT: 16.434 min Scan# 1475
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

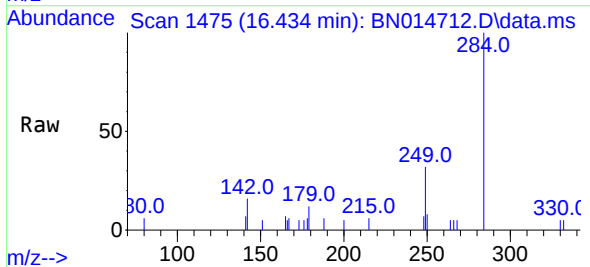


Tgt Ion:284 Resp: 1379
Ion Ratio Lower Upper
284 100
142 27.0 26.6 39.8
249 33.3 23.6 35.4

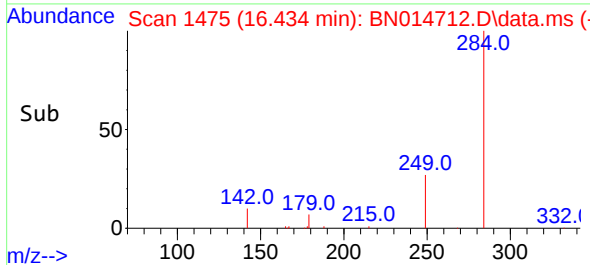

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM







#23
Atrazine
Concen: 0.43 ng
RT: 16.580 min Scan# 1487
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	200	Resp:	751
Ion Ratio	Lower	Upper	
200	100		
173	36.7	23.0	34.6#
215	52.2	38.6	57.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM




#24
Pentachlorophenol
Concen: 0.48 ng
RT: 16.775 min Scan# 1503
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	266	Resp:	459
Ion Ratio	Lower	Upper	
266	100		
264	57.5	24.2	36.4#
268	58.6	25.2	37.8#

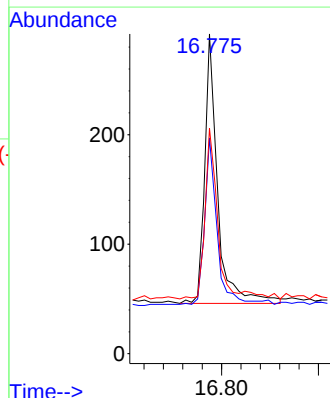



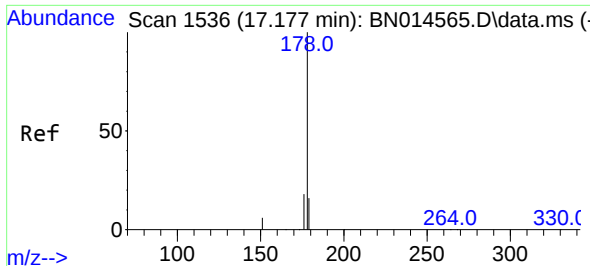


#25
Phenanthrene
Concen: 0.42 ng
RT: 17.164 min Scan# 1535
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

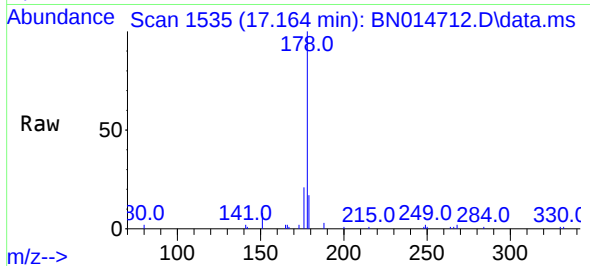


Tgt Ion:178 Resp: 5093

Ion	Ratio	Lower	Upper
178	100		
176	20.2	15.2	22.8
179	15.9	12.4	18.6

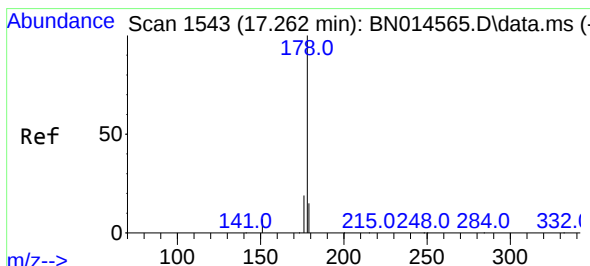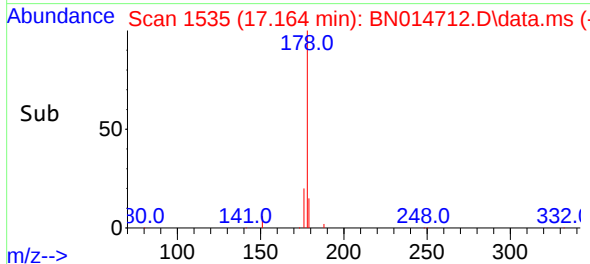
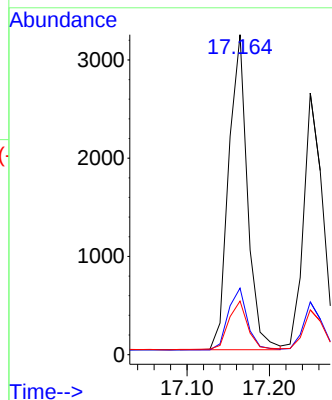


#26
Anthracene
Concen: 0.42 ng
RT: 17.249 min Scan# 1542
Delta R.T. -0.001 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

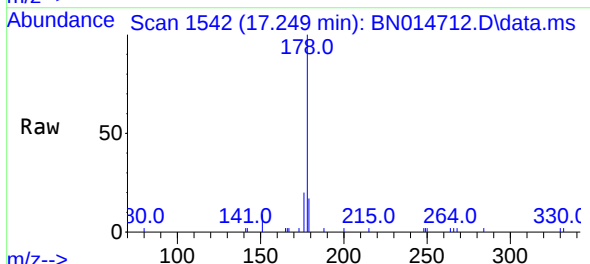

Tgt Ion:178 Resp: 4325


Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.8	22.2
179	15.5	12.2	18.2

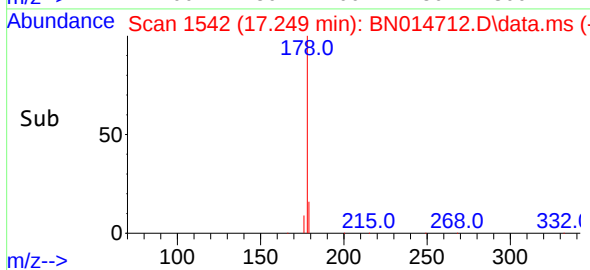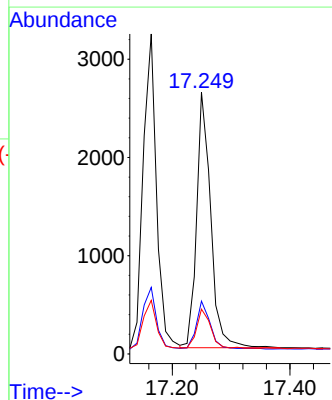

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM







#27
Fluoranthene-d10
Concen: 0.39 ng
RT: 19.156 min Scan# 1836
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion	Ratio	Lower	Upper
212	100		
106	9.8	10.1	15.1#
104	5.7	5.4	8.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM

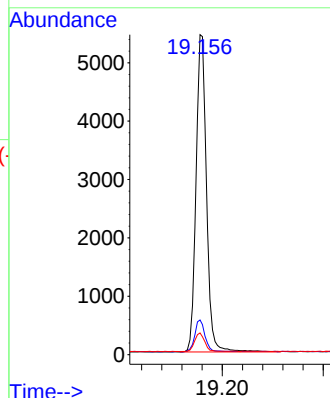


#28
Fluoranthene
Concen: 0.39 ng
RT: 19.185 min Scan# 1842
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.6	8.4	12.6
203	17.5	13.5	20.3









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.321 min Scan# 2131
Delta R.T. 0.008 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06





Tgt Ion:240 Resp: 5380
Ion Ratio Lower Upper
240 100
120 4.9 5.8 8.8#
236 26.7 20.6 30.8

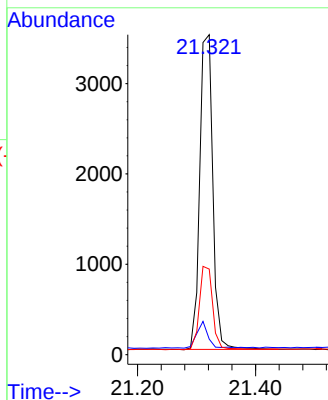

#30
Pyrene
Concen: 0.43 ng
RT: 19.553 min Scan# 1916
Delta R.T. 0.002 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Tgt Ion:202 Resp: 6346
Ion Ratio Lower Upper
202 100
200 21.5 16.3 24.5
203 18.2 14.0 21.0

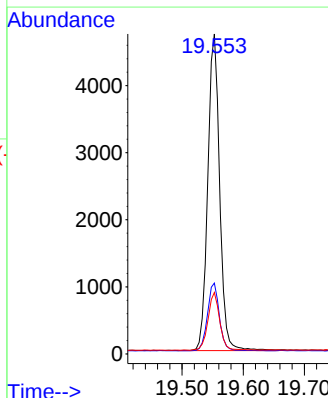


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
5/24/2021 2:37:22 PM




#31
Terphenyl-d14
Concen: 0.43 ng
RT: 19.761 min Scan# 1958
Delta R.T. 0.002 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06





Tgt Ion:244 Resp: 5447
Ion Ratio Lower Upper
244 100
212 8.1 6.0 9.0
122 8.6 9.3 13.9#

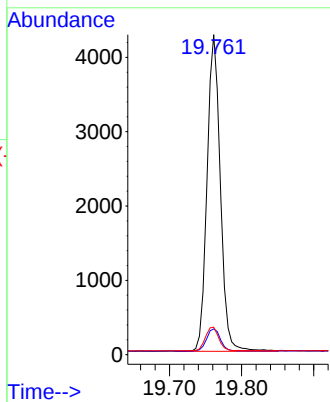

#32
Benzo(a)anthracene
Concen: 0.43 ng
RT: 21.300 min Scan# 2129
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Tgt Ion:228 Resp: 6722
Ion Ratio Lower Upper
228 100
226 28.1 21.7 32.5
229 20.6 15.7 23.5

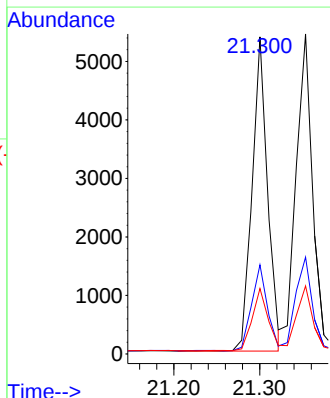

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM

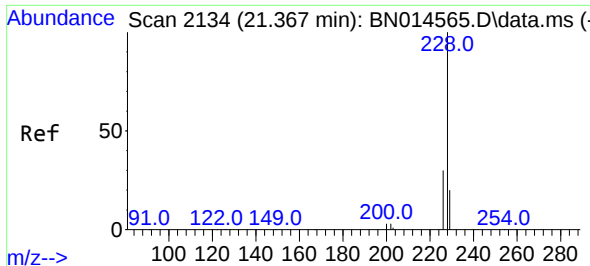





#33
Chrysene
Concen: 0.44 ng
RT: 21.353 min Scan# 2134
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	23.8	35.6
229	21.2	15.6	23.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
5/24/2021 2:37:22 PM

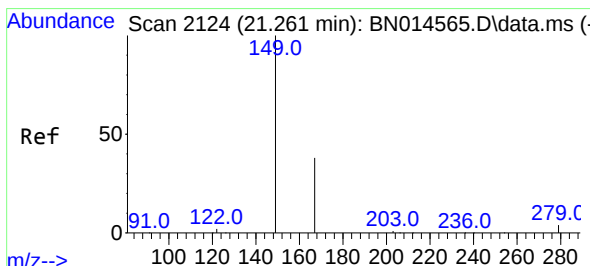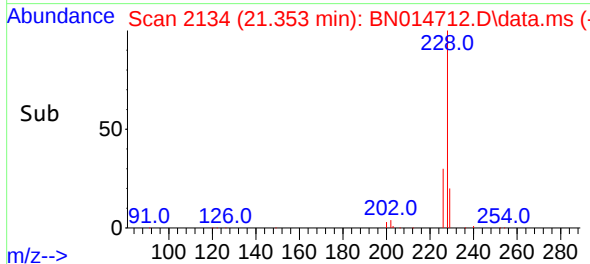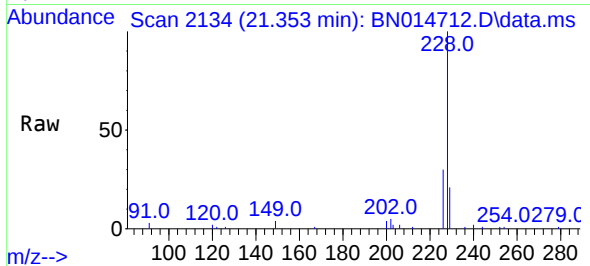

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.51 ng
RT: 21.236 min Scan# 2123
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06


Tgt Ion	Ratio	Lower	Upper
149	100		
167	37.4	20.5	30.7#
279	8.4	2.9	4.3#

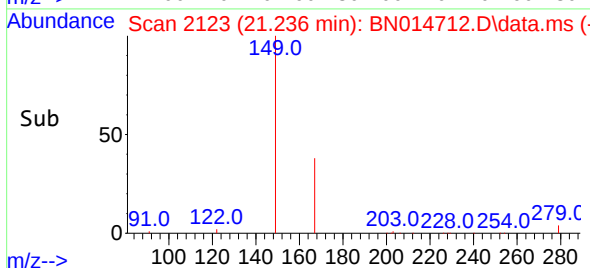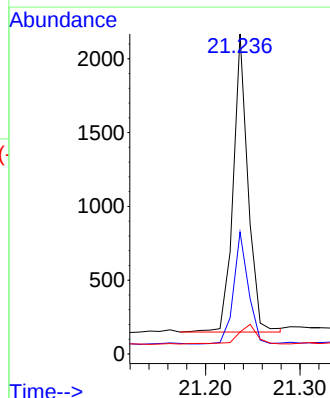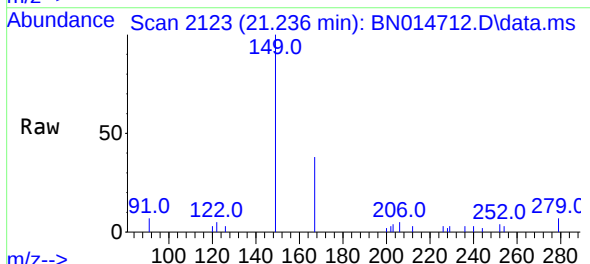

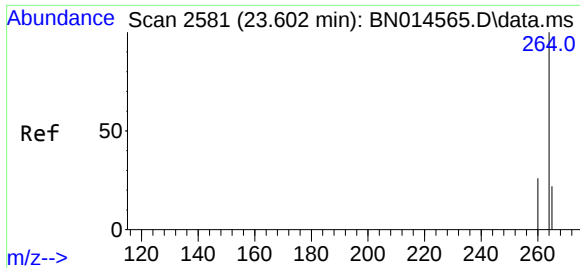

#35
Perylene-d12
Concen: 0.40 ng
RT: 23.582 min Scan# 2577
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

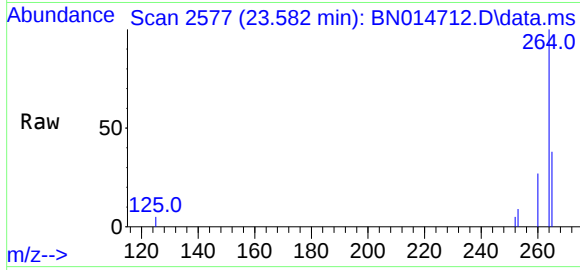


Tgt Ion:264 Resp: 5784
Ion Ratio Lower Upper
264 100
260 26.7 19.5 29.3
265 37.9 35.4 53.0

Manual Integrations
APPROVED



mohammad
5/24/2021 2:37:22 PM

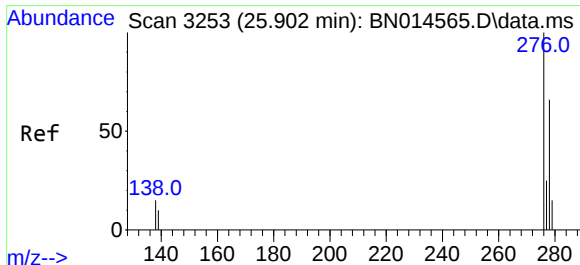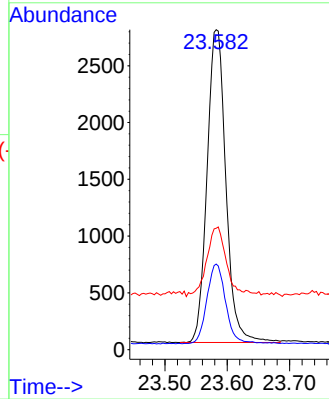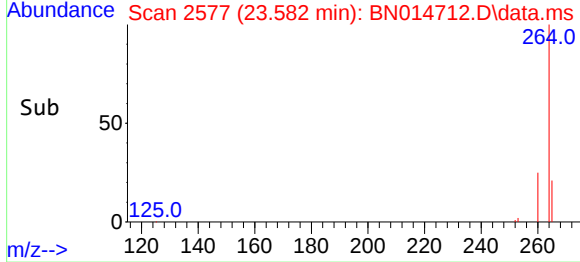


#36
Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.869 min Scan# 3245
Delta R.T. 0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

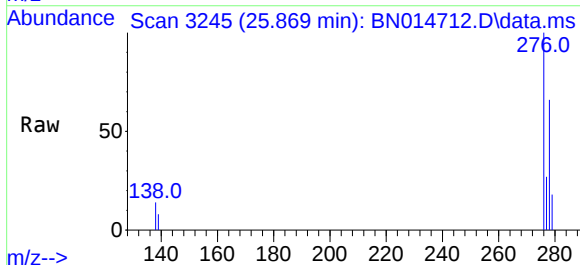


Tgt Ion:276 Resp: 9503
Ion Ratio Lower Upper
276 100
138 12.1 18.8 28.2#
277 25.7 19.8 29.8


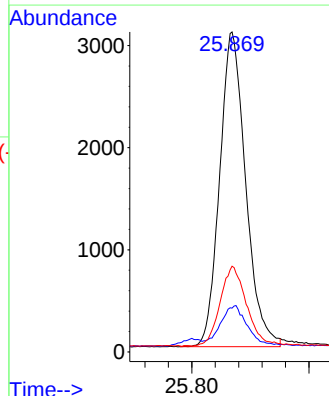
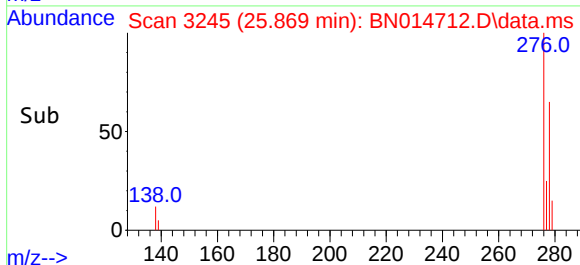





#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.901 min Scan# 2378
Delta R.T. 0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06





Tgt Ion:252 Resp: 8029
Ion Ratio Lower Upper
252 100
253 26.7 19.6 29.4
125 12.9 10.3 15.5

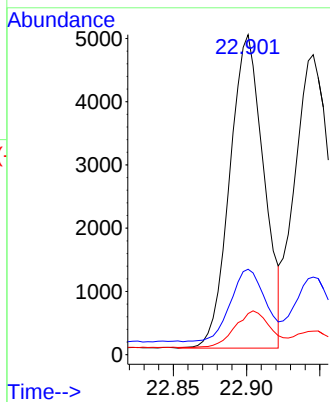

#38
Benzo(k)fluoranthene
Concen: 0.40 ng m
RT: 22.946 min Scan# 2391
Delta R.T. 0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

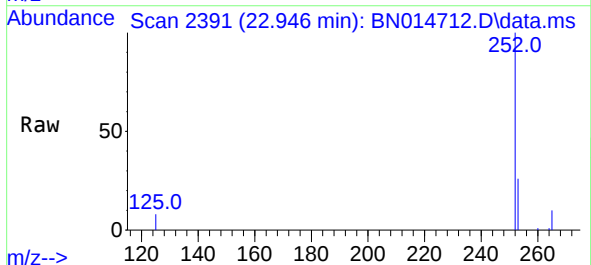


Tgt Ion:252 Resp: 8213
Ion Ratio Lower Upper
252 100
253 25.8 19.7 29.5
125 7.9 9.7 14.5#

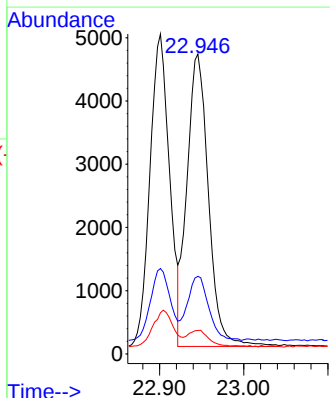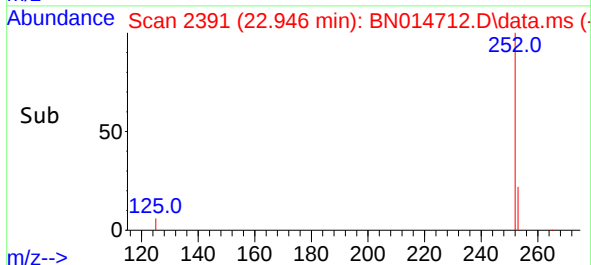


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
5/24/2021 2:37:22 PM




#39
Benzo(a)pyrene
Concen: 0.45 ng
RT: 23.483 min Scan# 2548
Delta R.T. 0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06





Tgt Ion: 252 Resp: 7530
Ion Ratio Lower Upper
252 100
253 30.9 21.8 32.6
125 22.6 14.9 22.3#

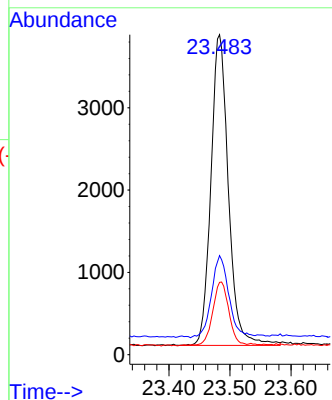

#40
Dibenzo(a,h)anthracene
Concen: 0.41 ng
RT: 25.882 min Scan# 3249
Delta R.T. 0.000 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06




Tgt Ion: 278 Resp: 8061
Ion Ratio Lower Upper
278 100
139 10.3 13.9 20.9#
279 25.1 20.7 31.1

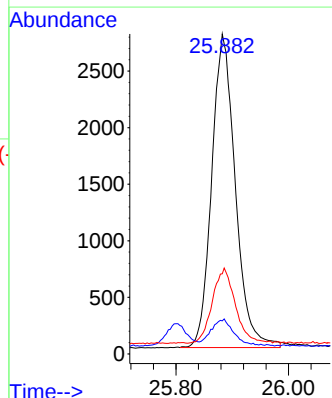

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM

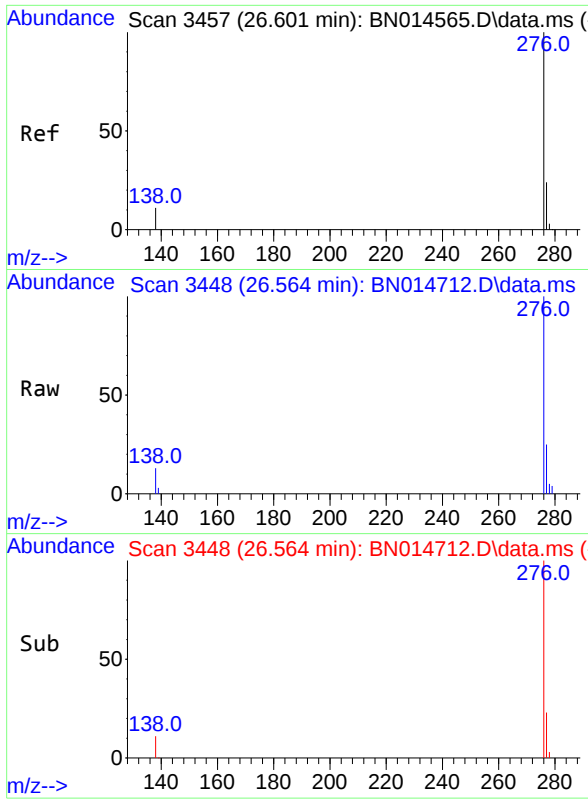

#41
Benzo(g,h,i)perylene
Concen: 0.42 ng
RT: 26.564 min Scan# 3448
Delta R.T. -0.003 min
Lab File: BN014712.D
Acq: 22 May 2021 04:06

Tgt Ion:	276	Resp:	8048
Ion Ratio	Lower	Upper	
276	100		
277	25.3	19.6	29.4
138	13.0	17.5	26.3#

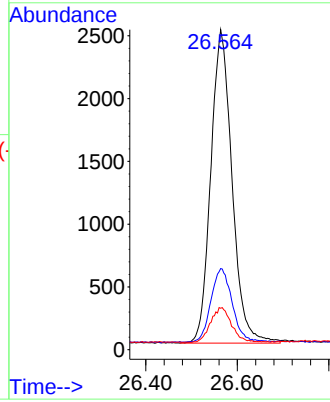

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
5/24/2021 2:37:22 PM