


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014687.D
 Acq On : 21 May 2021 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 21 11:30:28 2021

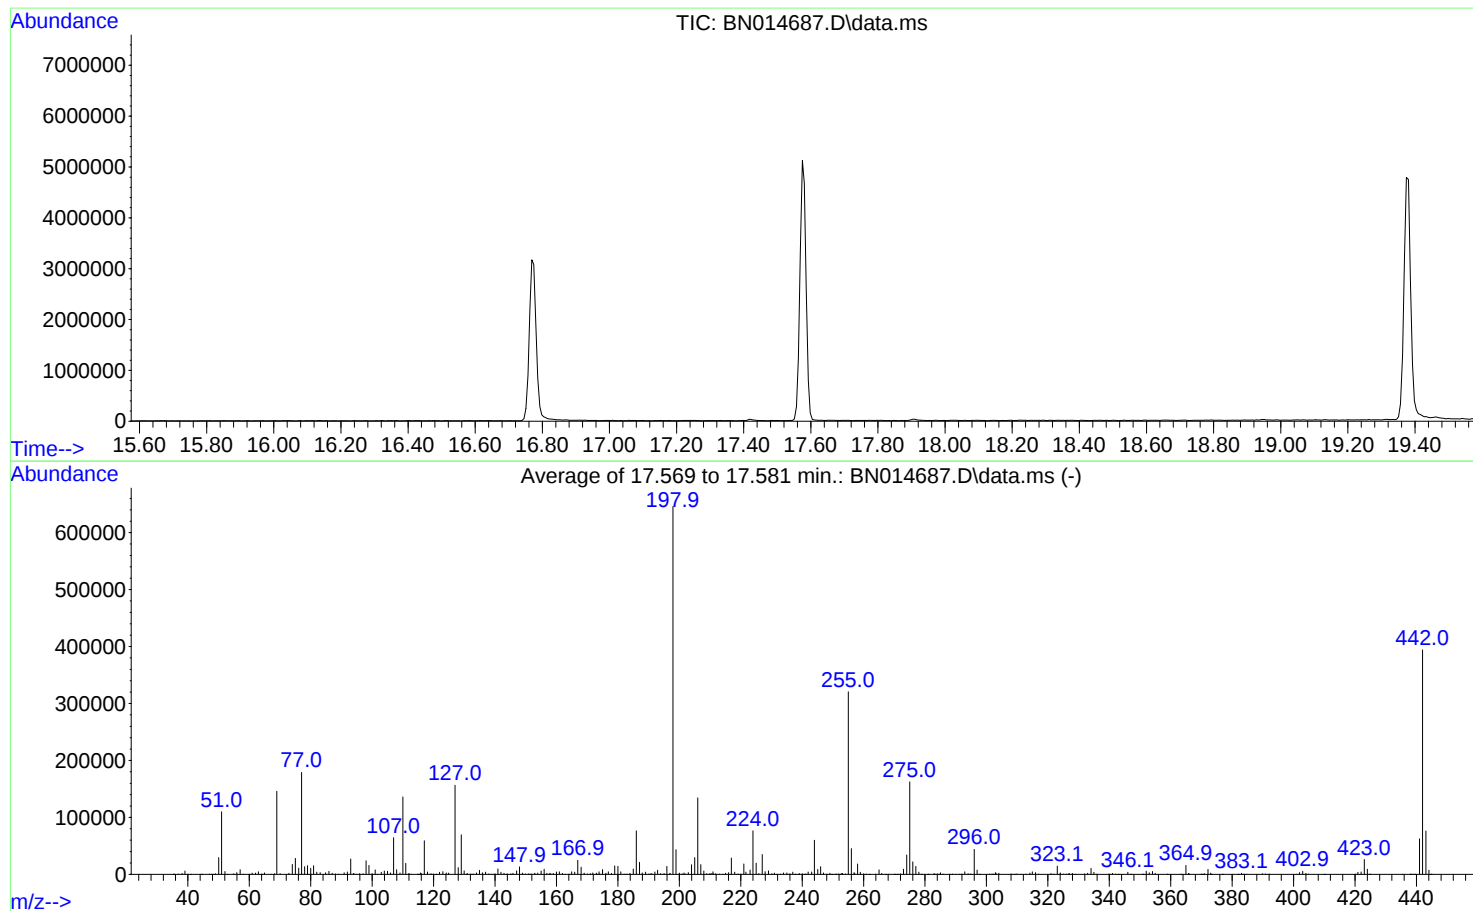




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.0	109859	PASS
68	69	0.00	2	0.7	1038	PASS
69	198	0.00	100	22.6	145851	PASS
70	69	0.00	2	0.8	1145	PASS
127	198	10	80	24.2	156565	PASS
197	198	0.00	2	0.3	1968	PASS
198	198	100	100	100.0	645909	PASS
199	198	5	9	6.7	43416	PASS
275	198	10	60	25.1	162363	PASS
365	198	1	100	2.4	15760	PASS
441	198	0.01	100	9.6	62253	PASS
442	442	50	100	100.0	394112	PASS
443	442	15	24	19.3	76101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014687.D
 Acq On : 21 May 2021 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 21 11:27:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

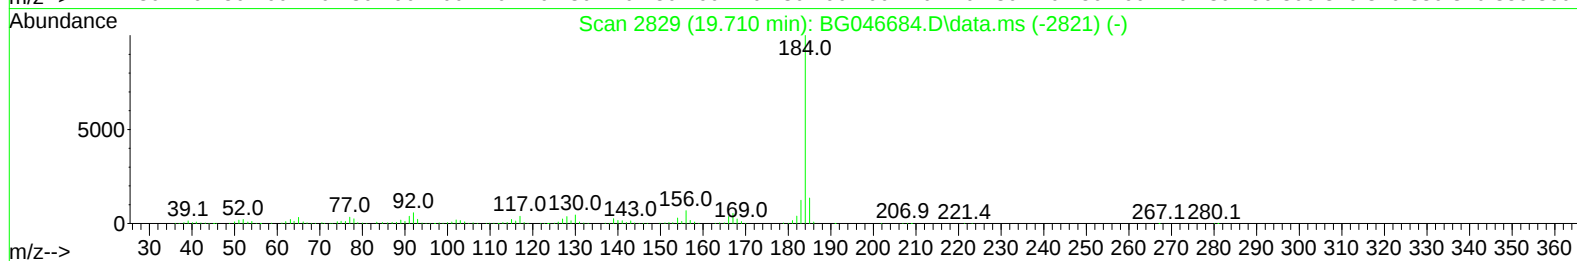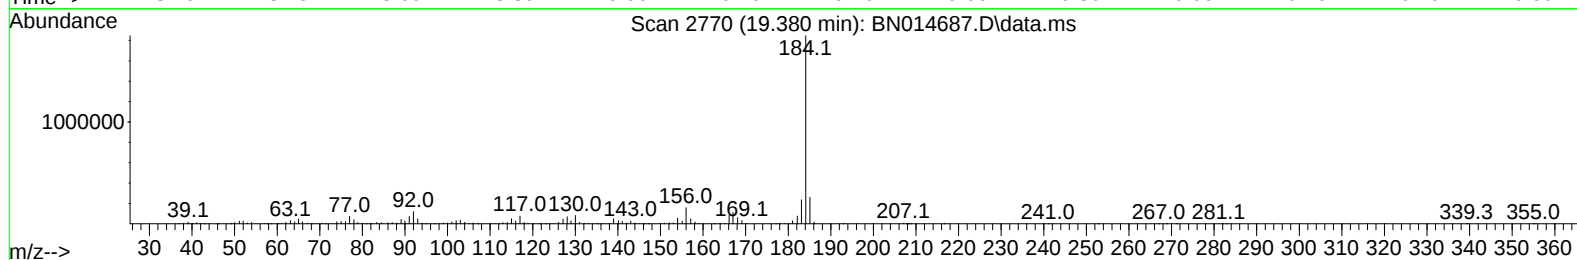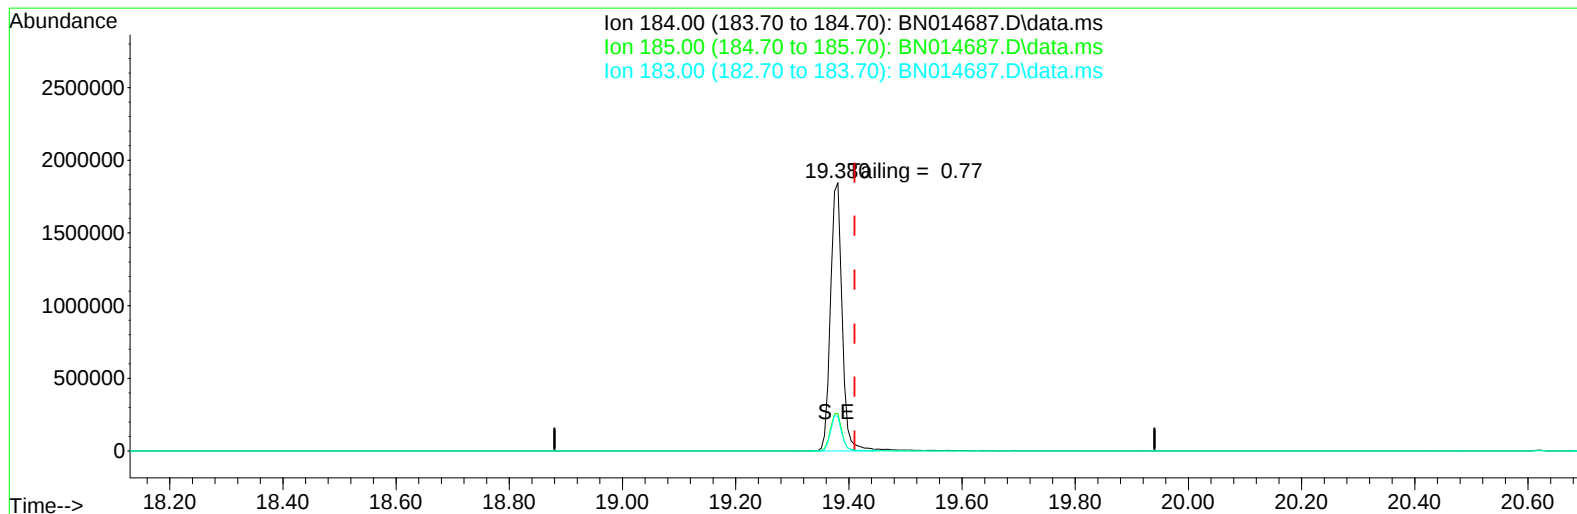

TIC: BN014687.D\data.ms

(77) Benzidine

19.380min (-0.029) 266897.91 ng




response 2640940

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014687.D
 Acq On : 21 May 2021 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 21 11:27:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 08 04:11:21 2021
 Response via : Initial Calibration

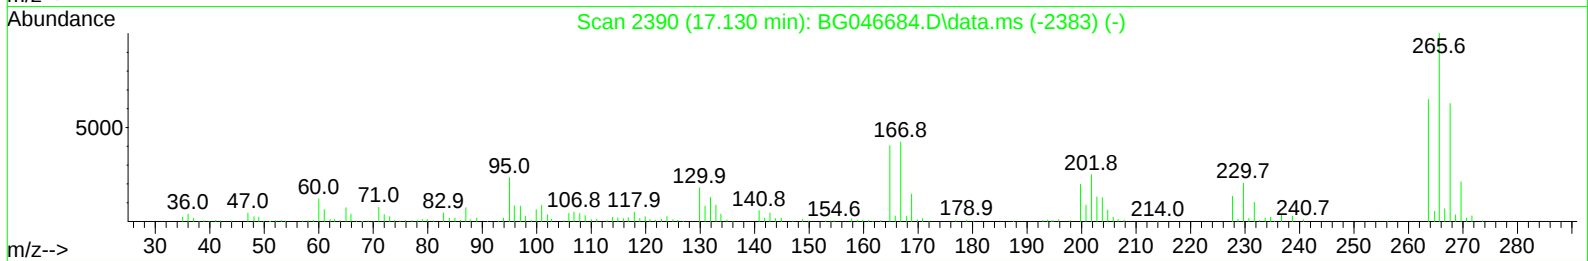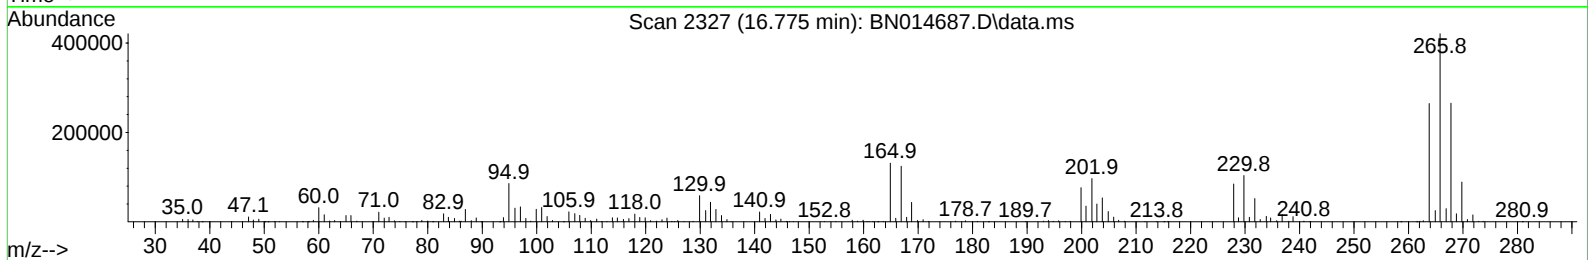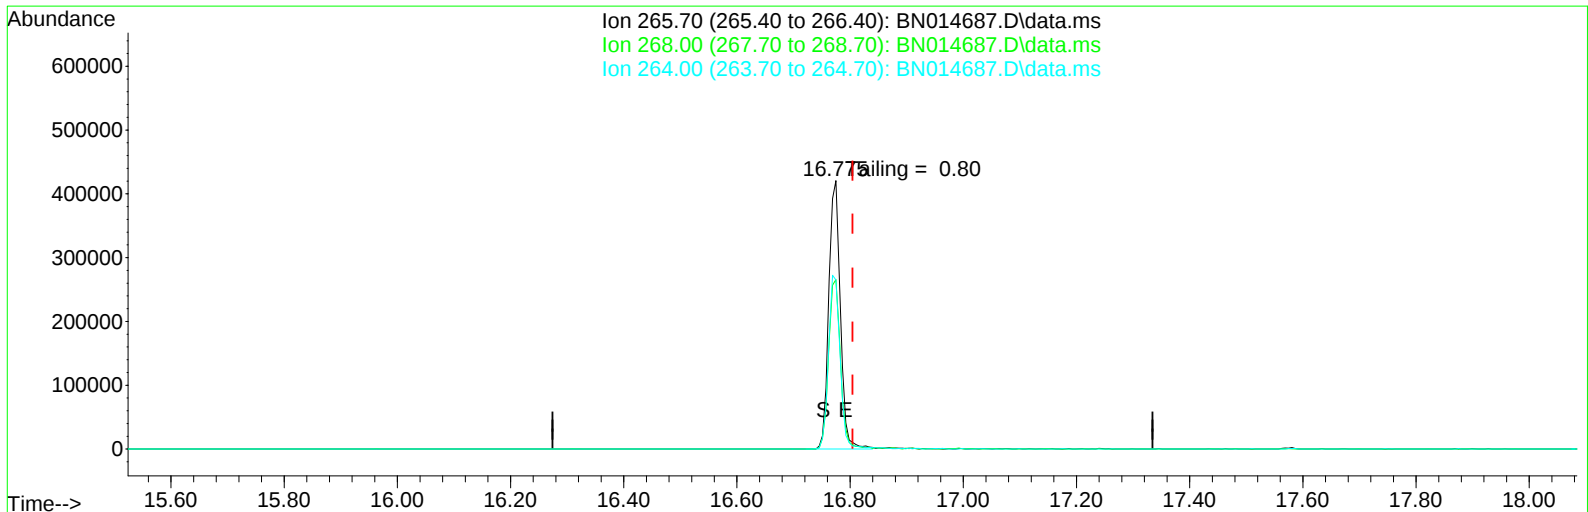

TIC: BN014687.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.029) 20452.84 ng

response 598858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.13
264.00	61.60	62.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/21/2021	BNA_N	<u>BN014687.D</u>
Compound Name	Response	Retention Time
DDT	1718264	20.62
DDD	10718	20.17
DDE	3421	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14139	1732403	0.82