


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
 Data File : BN014704.D
 Acq On : 21 May 2021 22:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 21 11:30:28 2021

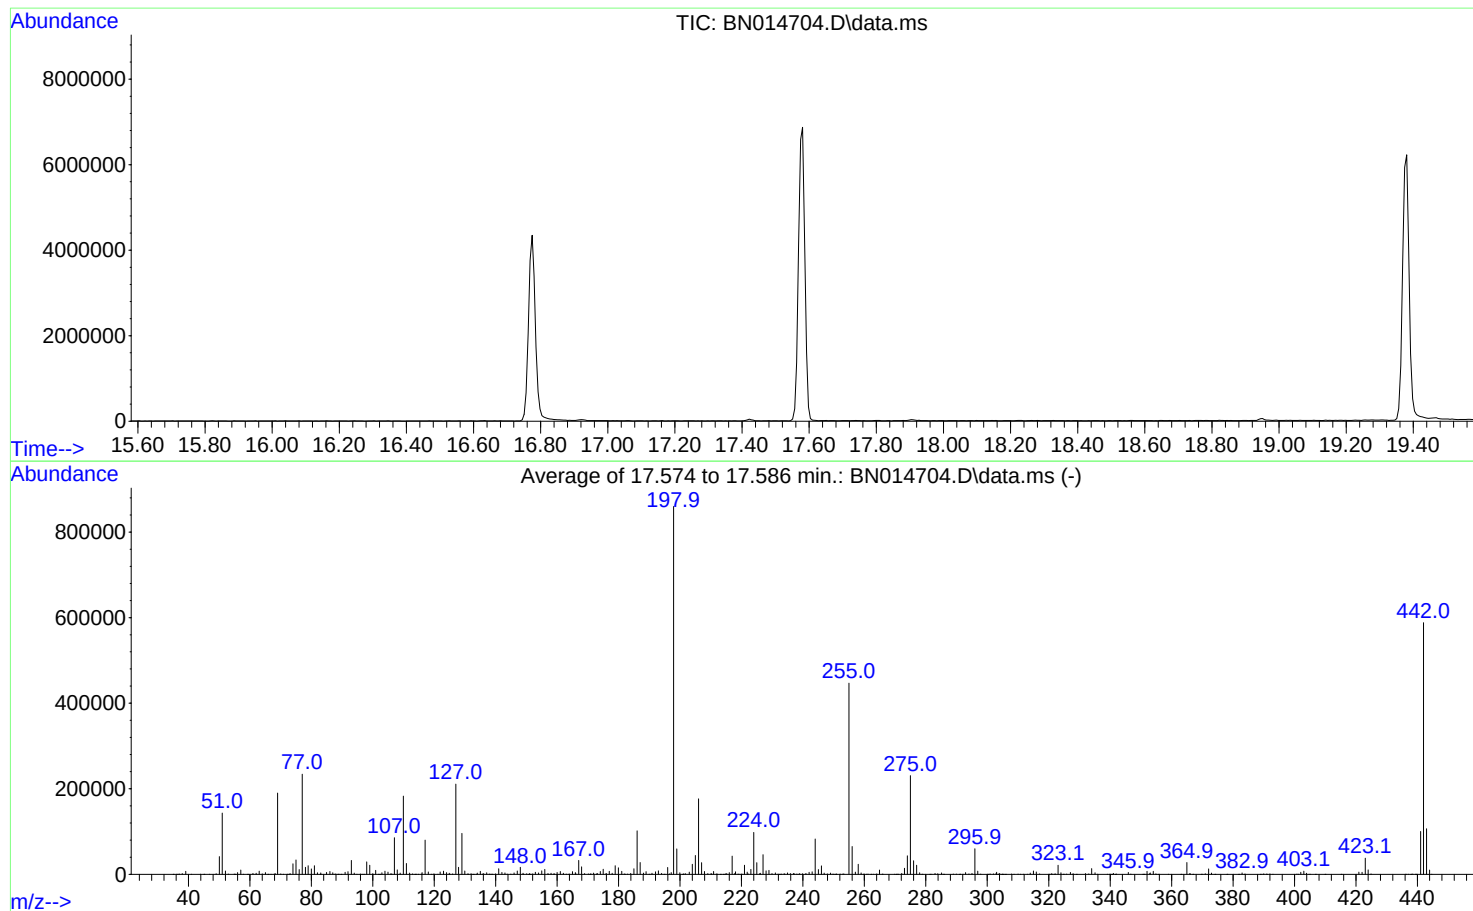




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	16.7	143203	PASS
68	69	0.00	2	0.9	1778	PASS
69	198	0.00	100	22.1	190136	PASS
70	69	0.00	2	0.6	1133	PASS
127	198	10	80	24.6	211072	PASS
197	198	0.00	2	0.5	4033	PASS
198	198	100	100	100.0	859733	PASS
199	198	5	9	6.9	59384	PASS
275	198	10	60	26.8	230827	PASS
365	198	1	100	3.2	27621	PASS
441	198	0.01	100	11.6	100112	PASS
442	442	50	100	100.0	588224	PASS
443	442	15	24	18.1	106453	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
Data File : BN014704.D
Acq On : 21 May 2021 22:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 22 07:55:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

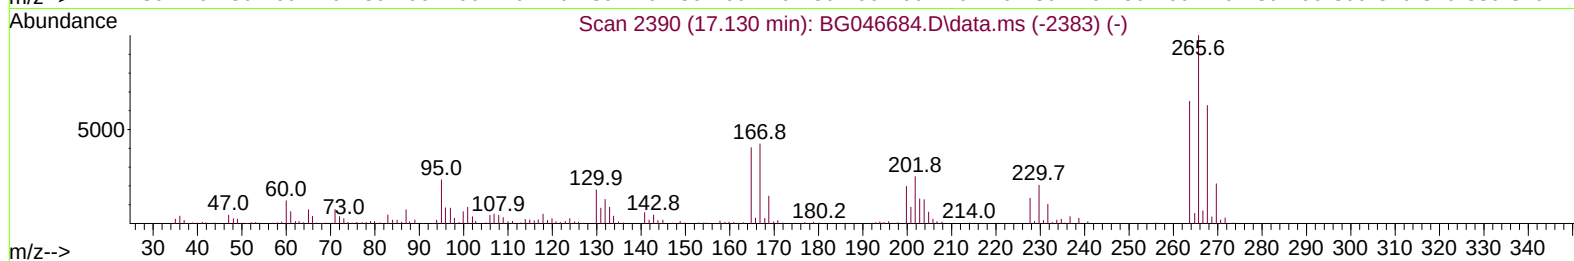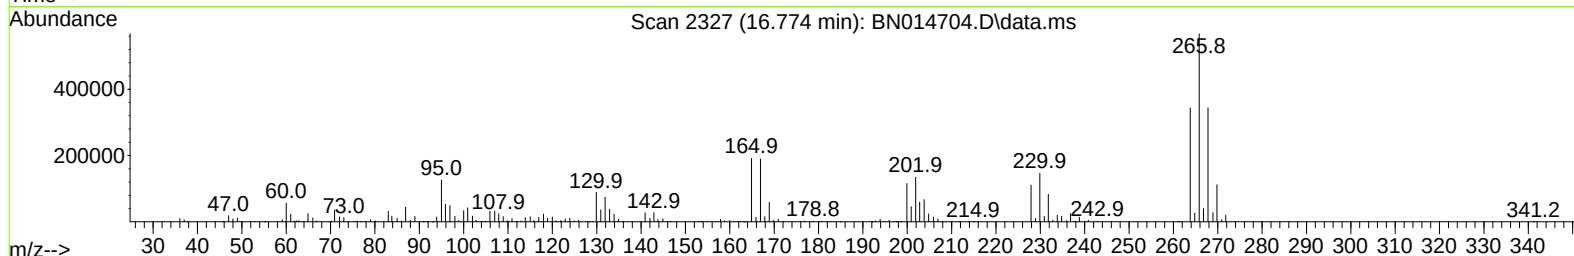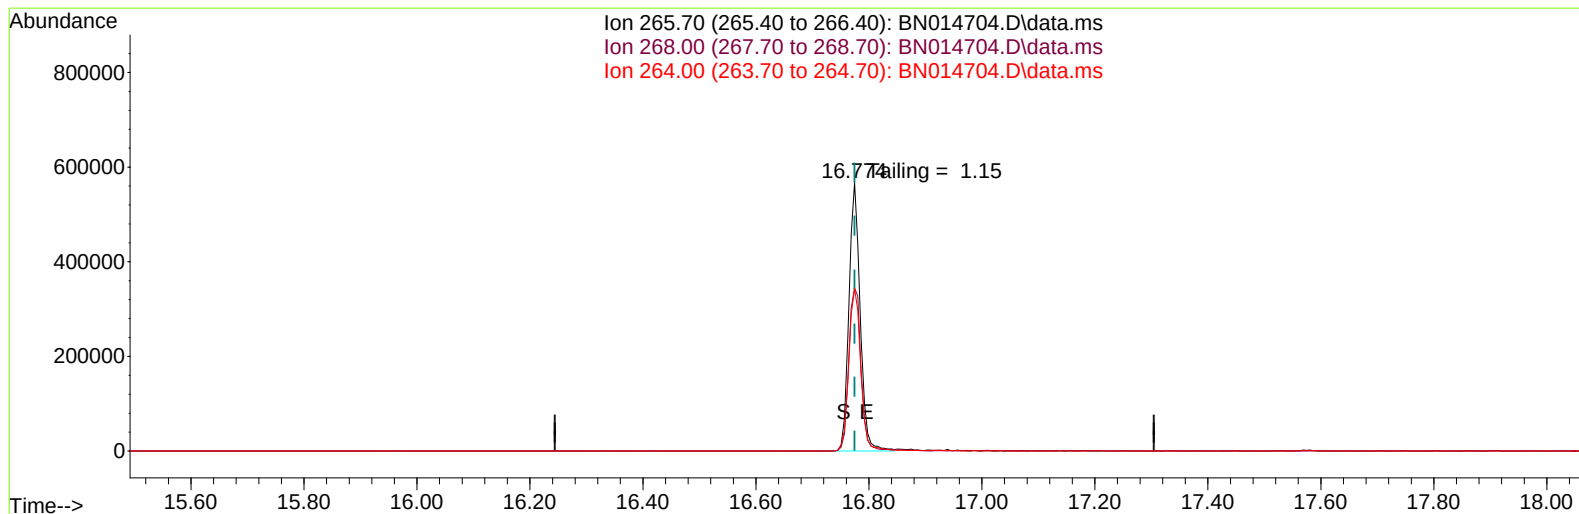

TIC: BN014704.D\data.ms

(70) Pentachlorophenol (C)

16.774min (0.000) 21212.87 ng




response 785088

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.66
264.00	61.60	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052121\
Data File : BN014704.D
Acq On : 21 May 2021 22:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 22 07:55:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

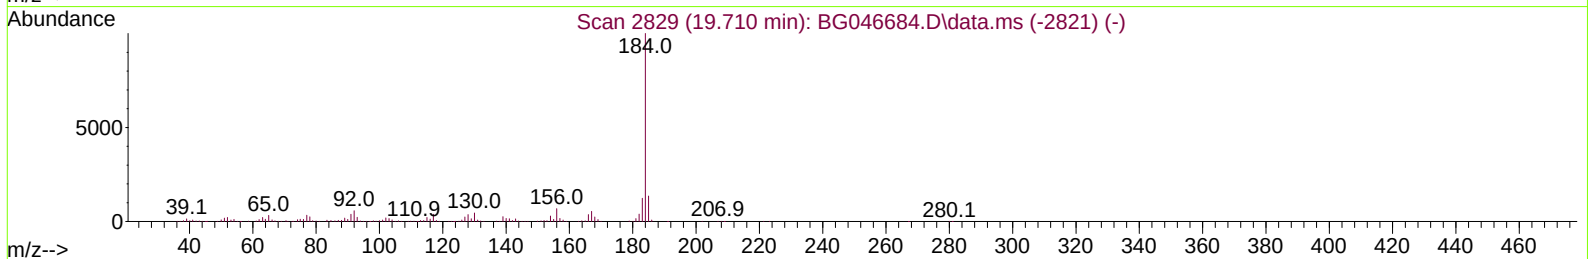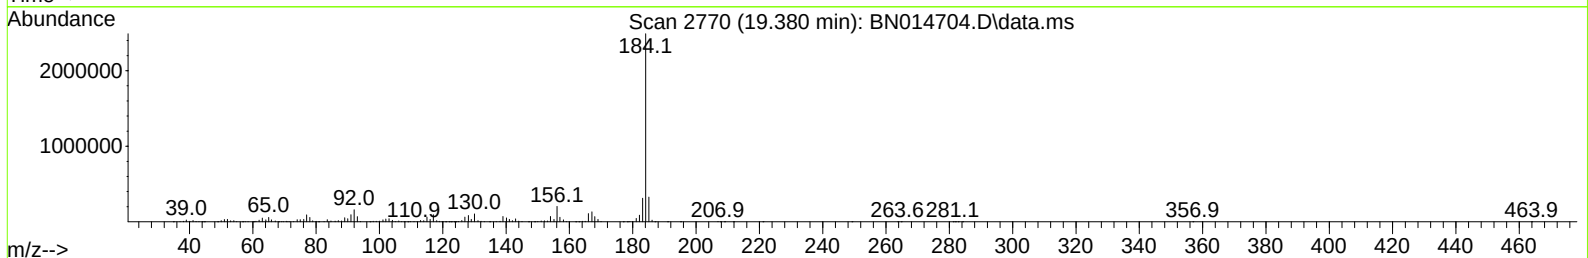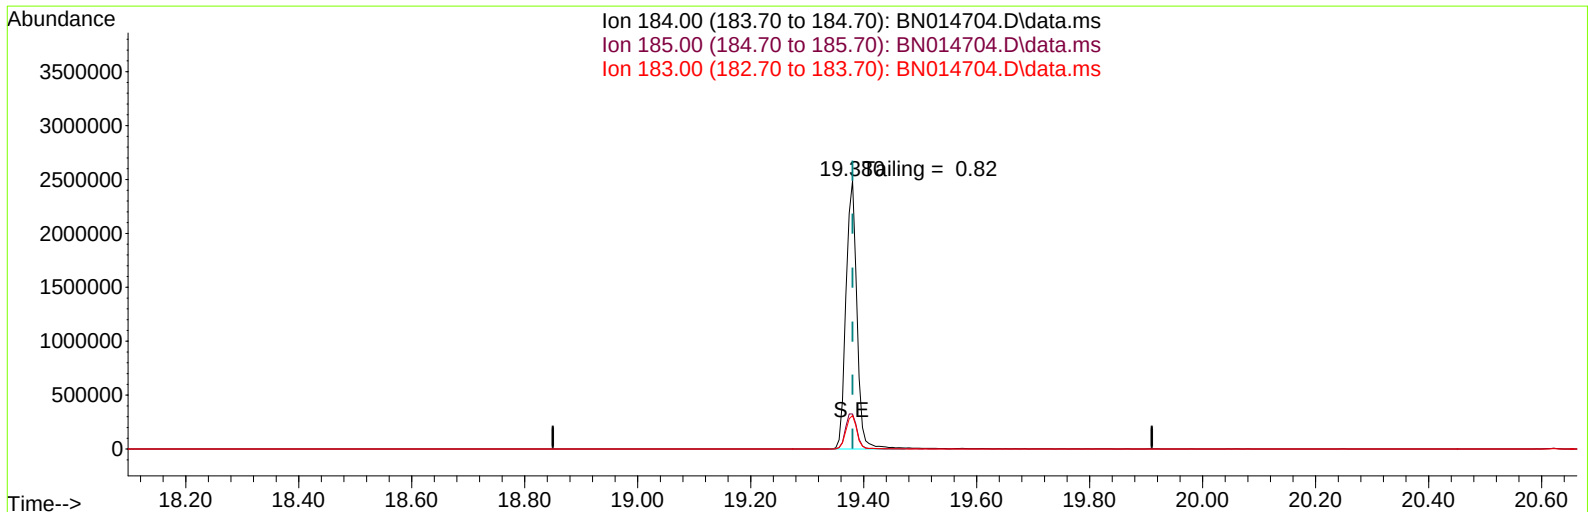

TIC: BN014704.D\data.ms

(77) Benzidine

19.380min (0.000) 0.00 ng

response 3372513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.09
183.00	13.20	12.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/21/2021	BNA_N	<u>BN014704.D</u>
Compound Name	Response	Retention Time
DDT	2150966	20.621
DDD	38347	20.18
DDE	8547	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46894	2197860	2.13

Instrument :
BNA_N
ClientSampleId :
DFTPP