
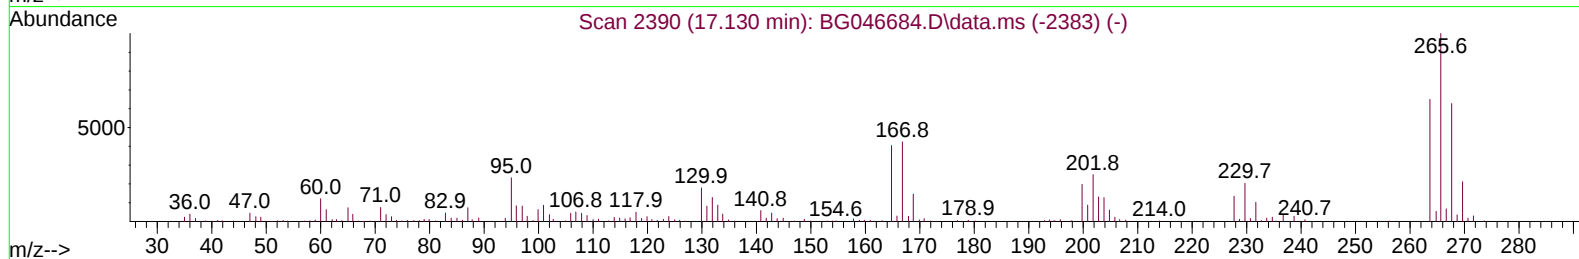
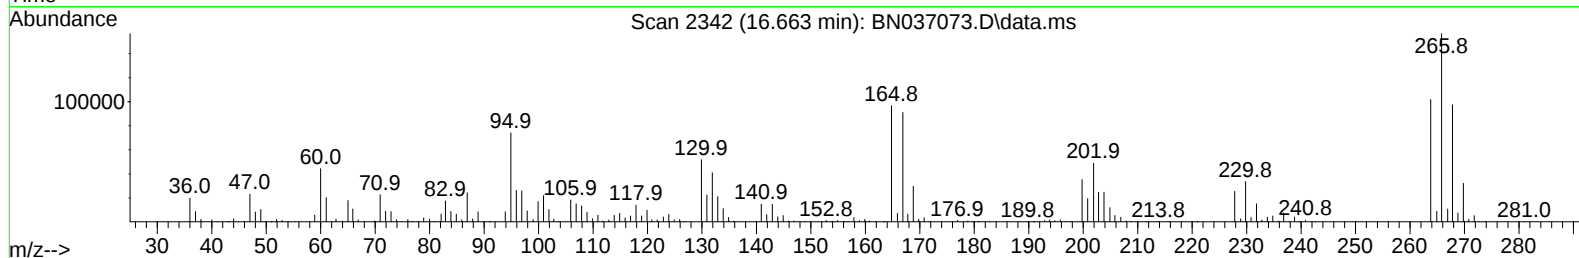


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052125\
Data File : BN037073.D
Acq On : 20 May 2025 14:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 01:54:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 21 01:54:36 2025
Response via : Initial Calibration

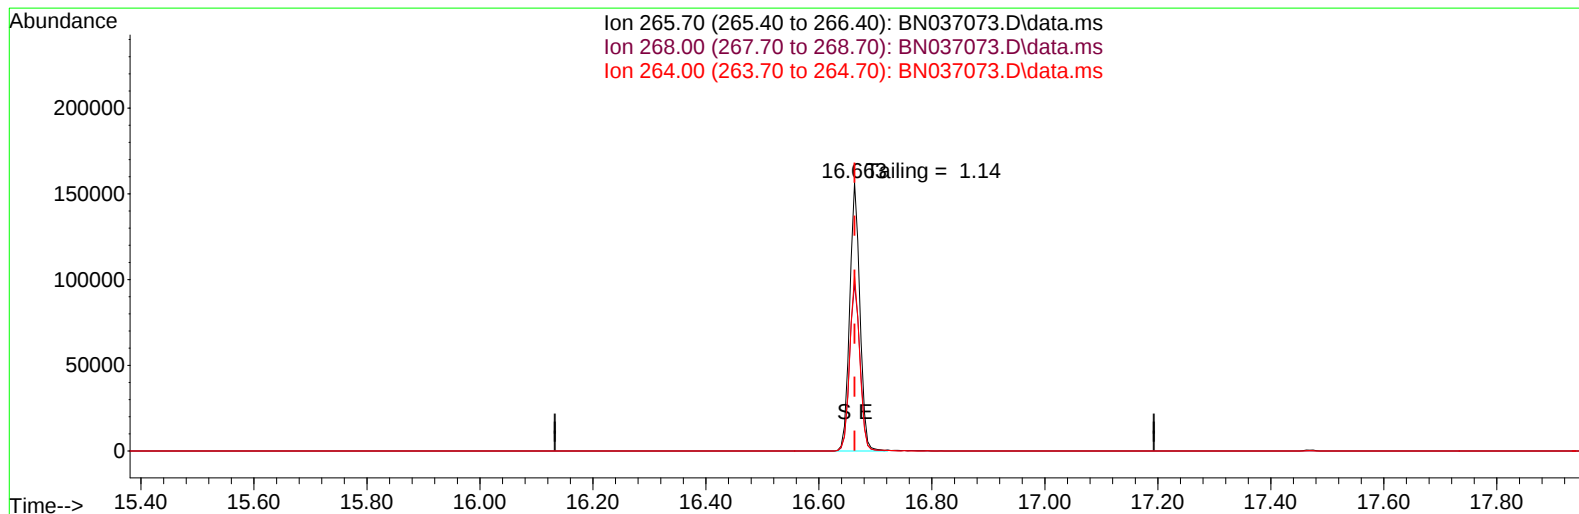

TIC: BN037073.D\data.ms

(70) Pentachlorophenol (C)




16.663min (0.000) 18354.59 ng

response 197914

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	65.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052125\
Data File : BN037073.D
Acq On : 20 May 2025 14:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 01:54:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 21 01:54:36 2025
Response via : Initial Calibration

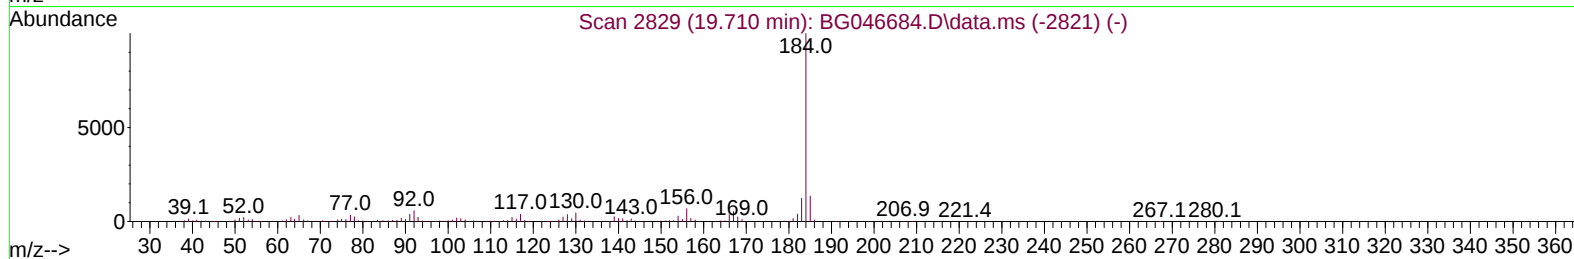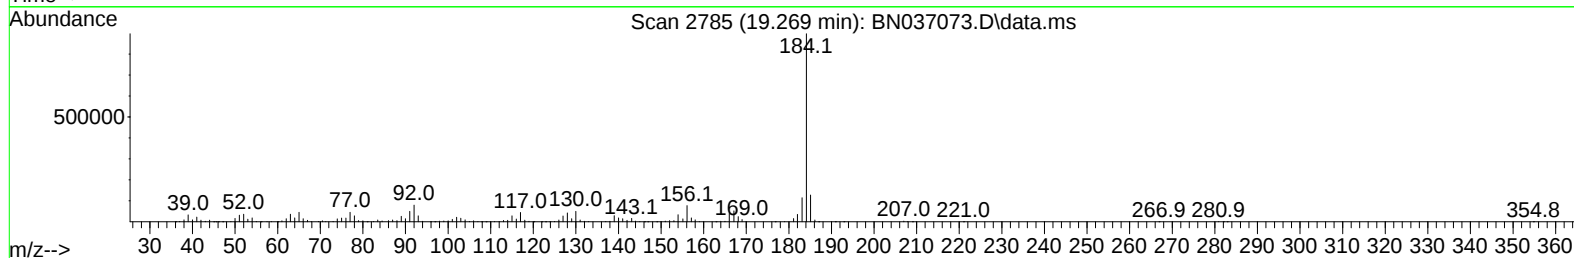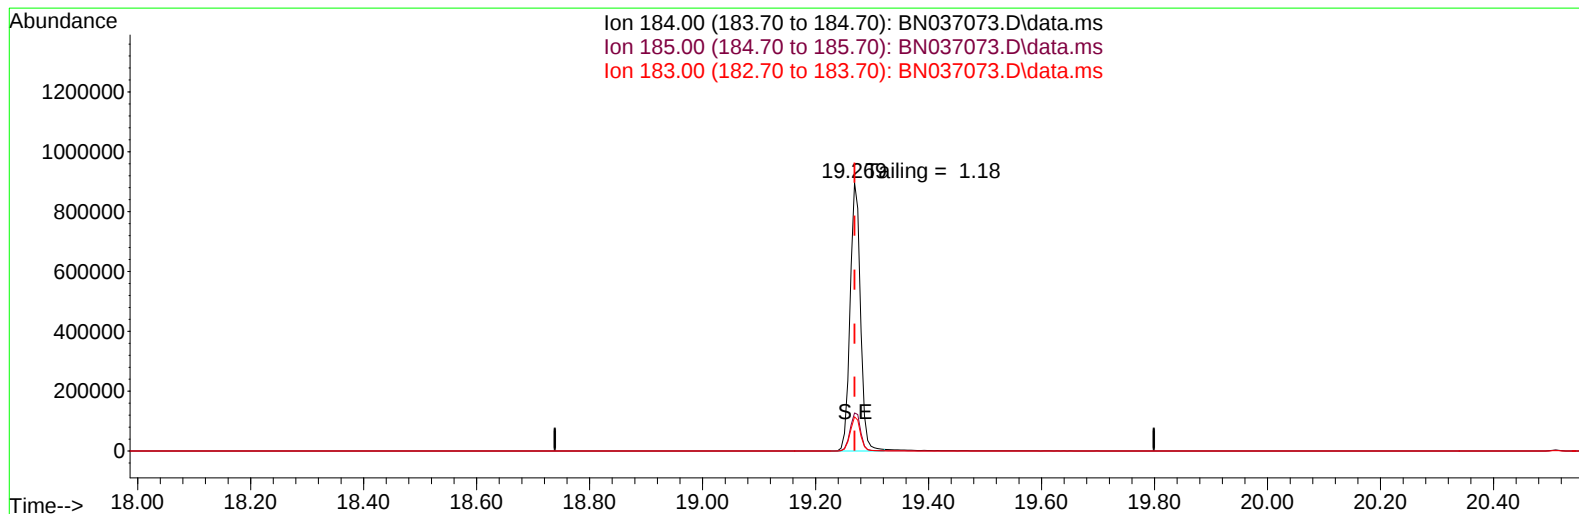

TIC: BN037073.D\data.ms

(77) Benzidine

19.269min (0.000) 0.00 ng

response 1157281

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	12.75
0.00	0.00	0.00