
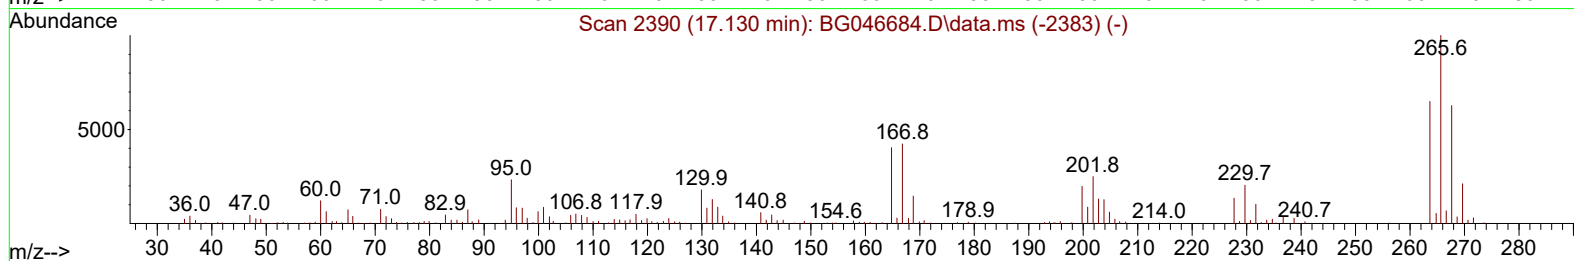
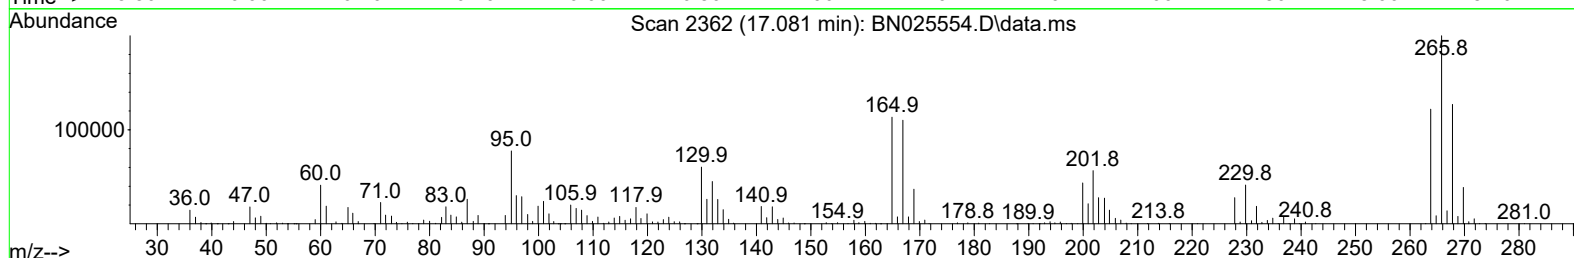


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
Data File : BN025554.D
Acq On : 23 May 2023 02:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 06:05:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 23 06:03:53 2023
Response via : Initial Calibration

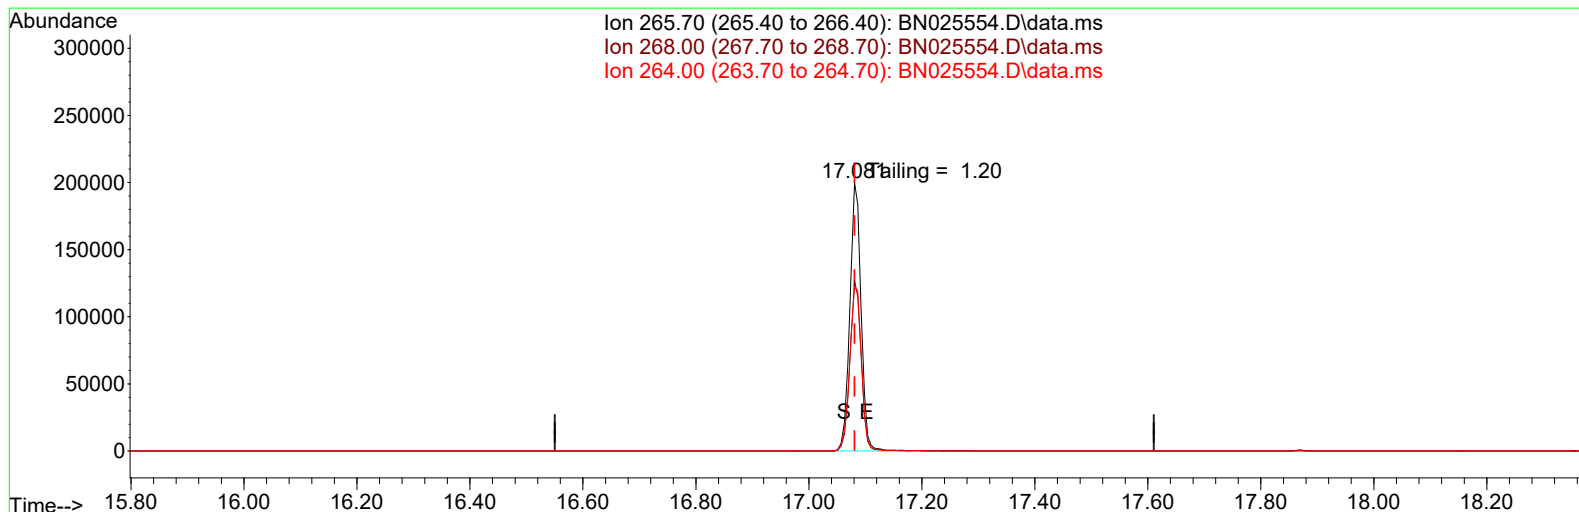

TIC: BN025554.D\data.ms

(70) Pentachlorophenol (C)




17.081min (+ 0.000) 14811.39 ng

response 276758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.50
264.00	61.60	60.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
Data File : BN025554.D
Acq On : 23 May 2023 02:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 06:05:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 23 06:03:53 2023
Response via : Initial Calibration

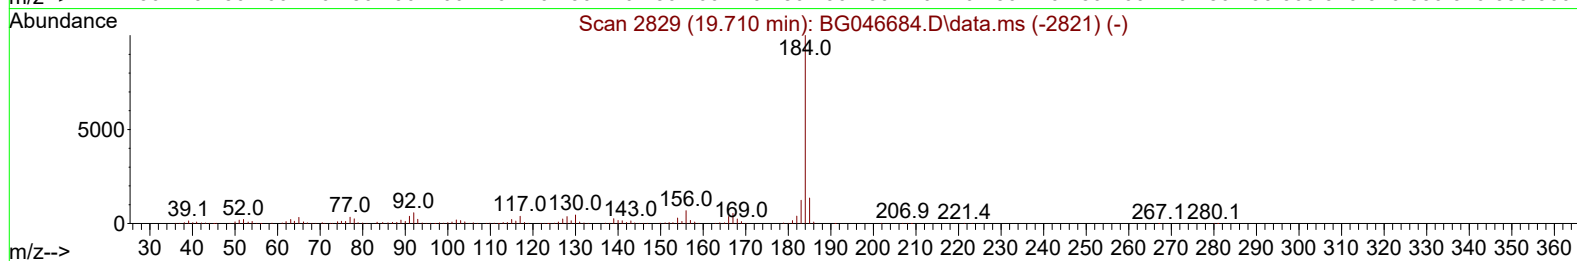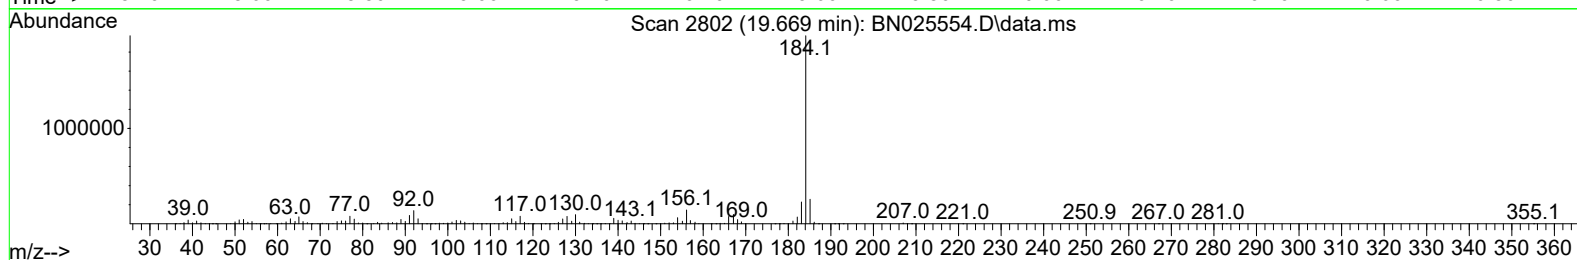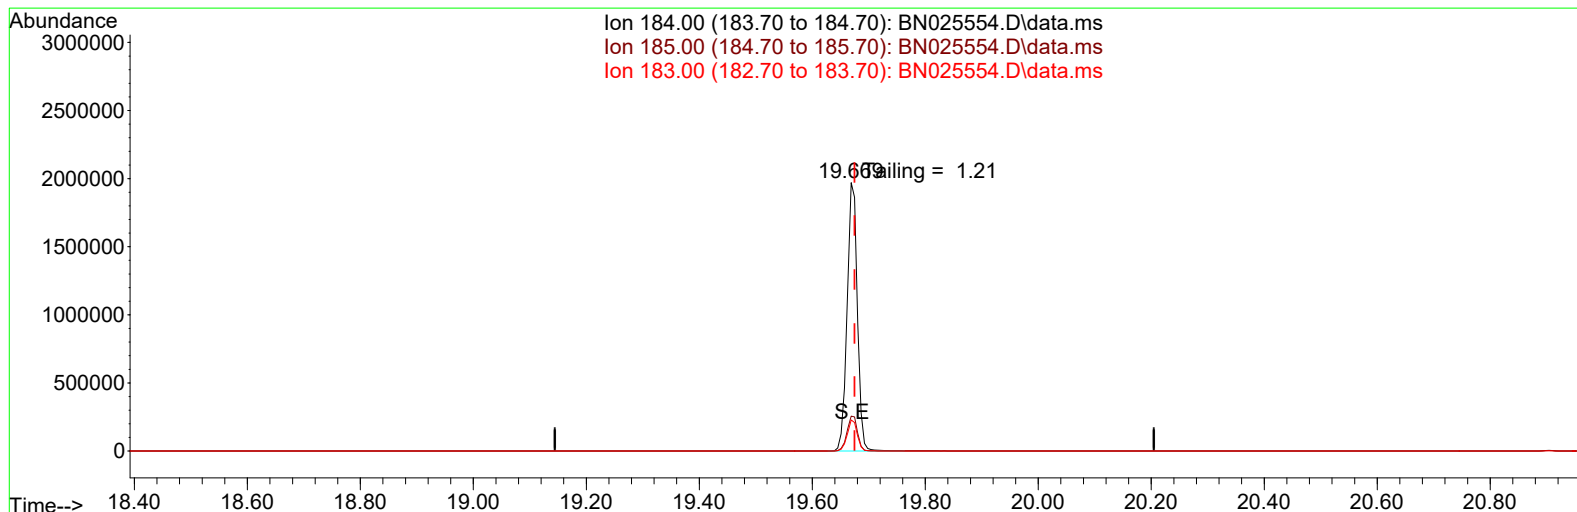

TIC: BN025554.D\data.ms

(77) Benzidine

19.669min (-0.006) 0.00 ng

response 2479245

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.56
0.00	0.00	0.00