
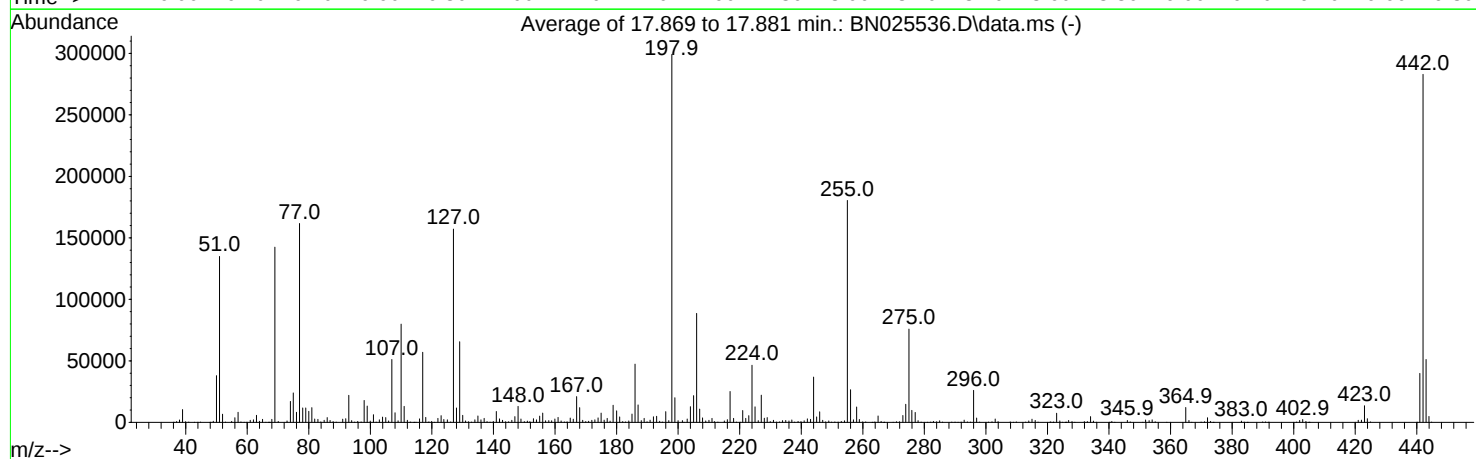


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
 Data File : BN025536.D
 Acq On : 22 May 2023 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 23 03:22:57 2023

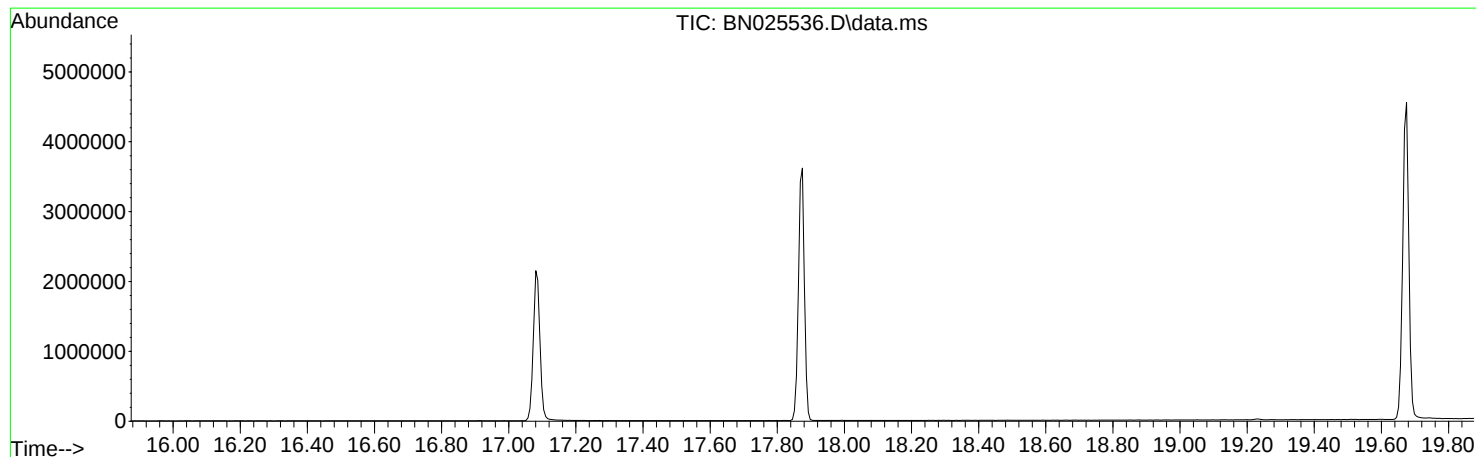

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	134949	PASS
68	69	0.00	2	1.7	2446	PASS
69	198	0.00	100	47.6	142459	PASS
70	69	0.00	2	0.5	733	PASS
127	198	10	80	52.6	157216	PASS
197	198	0.00	2	0.5	1385	PASS
198	198	100	100	100.0	299093	PASS
199	198	5	9	6.7	20066	PASS
275	198	10	60	25.4	75837	PASS
365	198	1	100	4.1	12169	PASS
441	198	0.01	100	13.3	39856	PASS
442	442	50	100	100.0	282944	PASS
443	442	15	24	18.1	51139	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/22/2023	BNA_N	<u>BN025536.D</u>
Compound Name	Response	Retention Time
DDT	1045575	20.904
DDD	10989	20.516
DDE	135	19.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11124	1056699	1.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
 Data File : BN025536.D
 Acq On : 22 May 2023 13:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 23 06:03:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 23 06:03:53 2023
 Response via : Initial Calibration

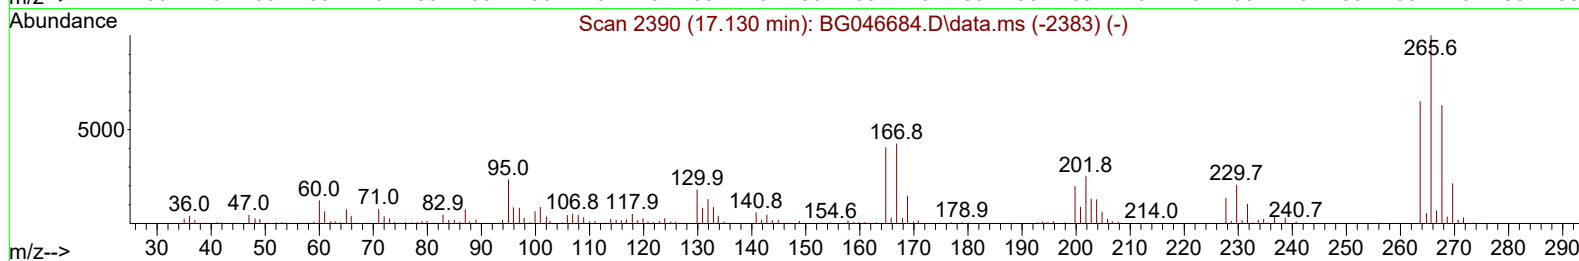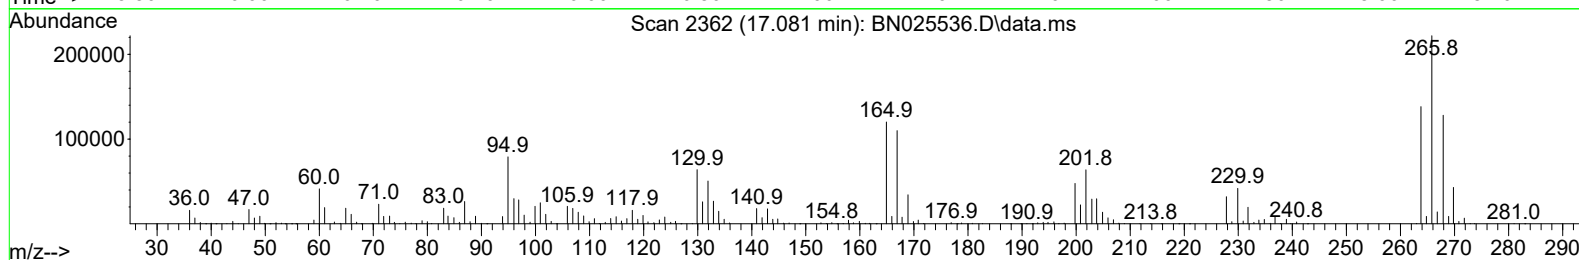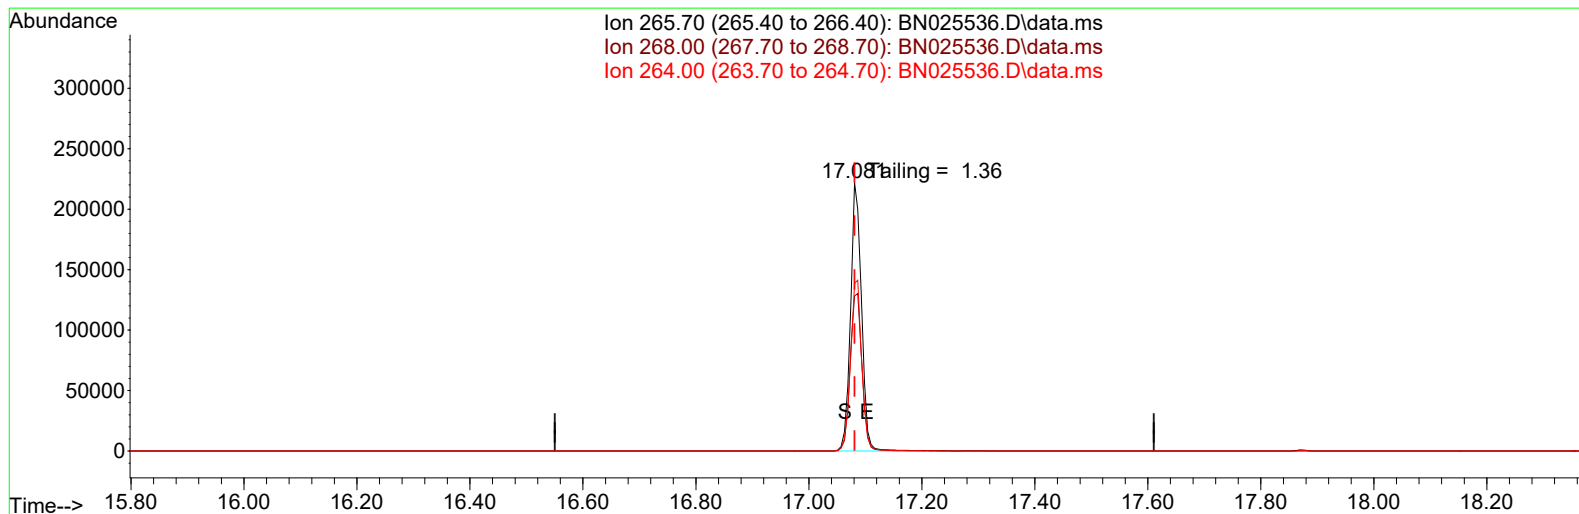

TIC: BN025536.D\data.ms

(70) Pentachlorophenol (C)

17.081min (0.000) 17053.11 ng




response 299642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.77
264.00	61.60	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
Data File : BN025536.D
Acq On : 22 May 2023 13:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 23 06:03:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 23 06:03:53 2023
Response via : Initial Calibration

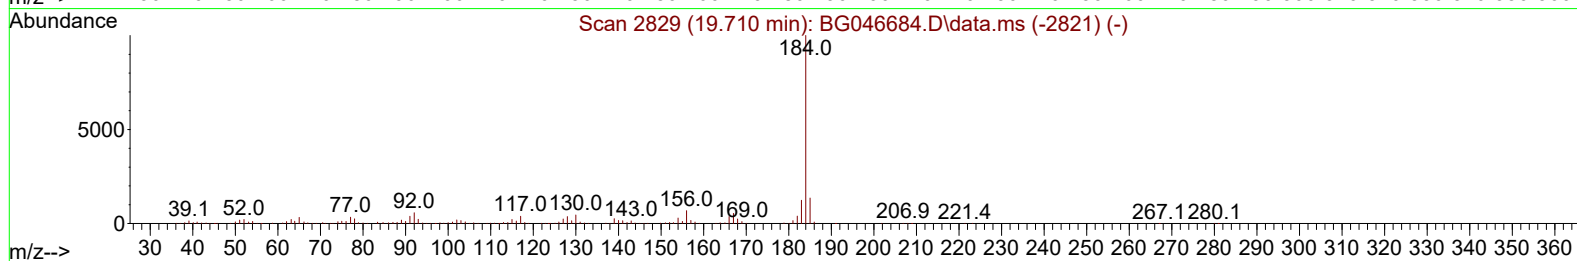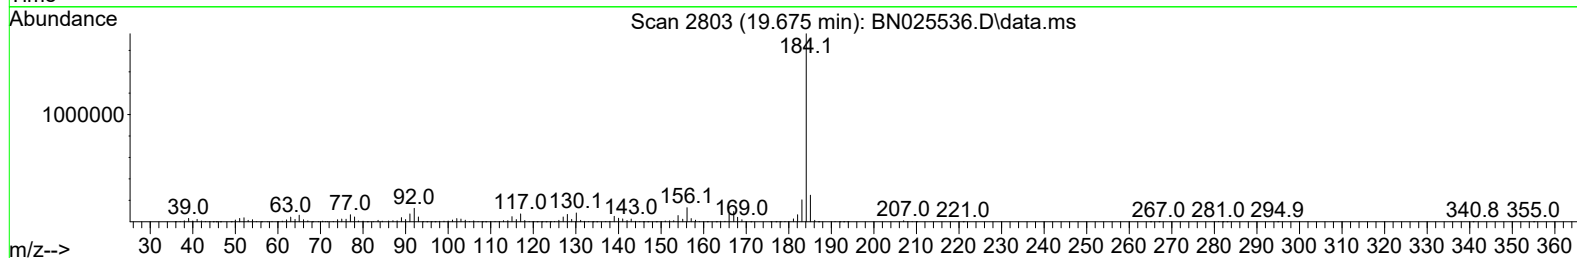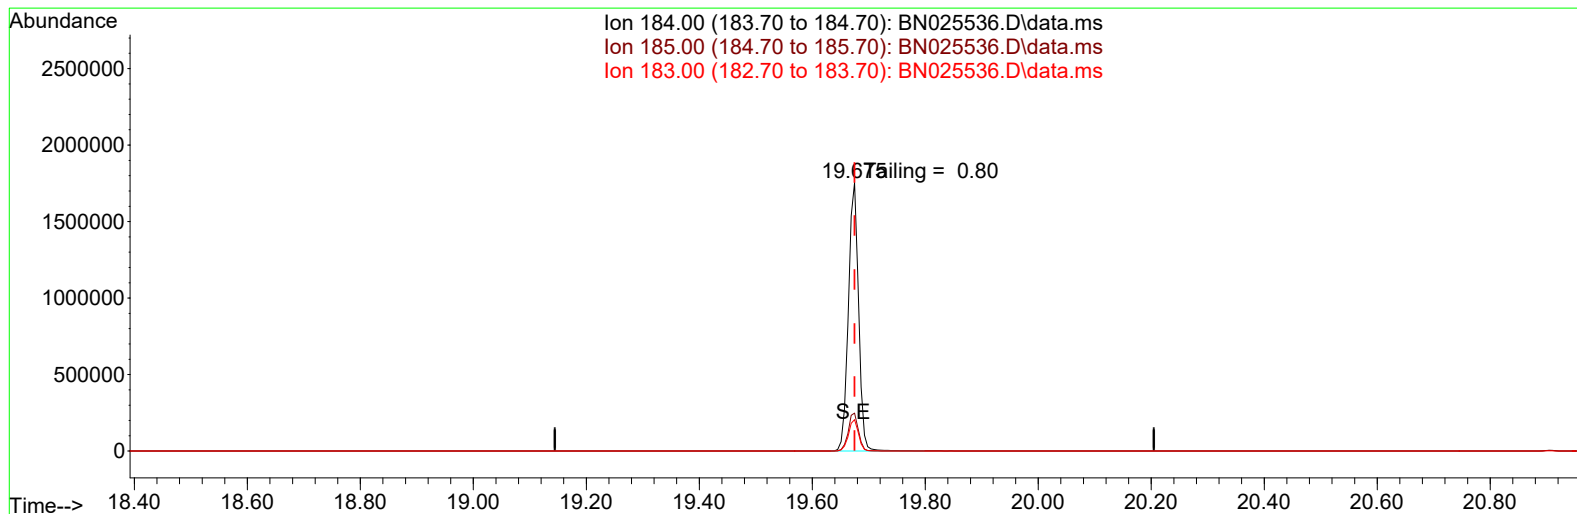

TIC: BN025536.D\data.ms

(77) Benzidine

19.675min (0.000) 0.00 ng

response 2200889

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	11.69
0.00	0.00	0.00