


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
Data File : BN025554.D
Acq On : 23 May 2023 02:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 23 03:22:57 2023

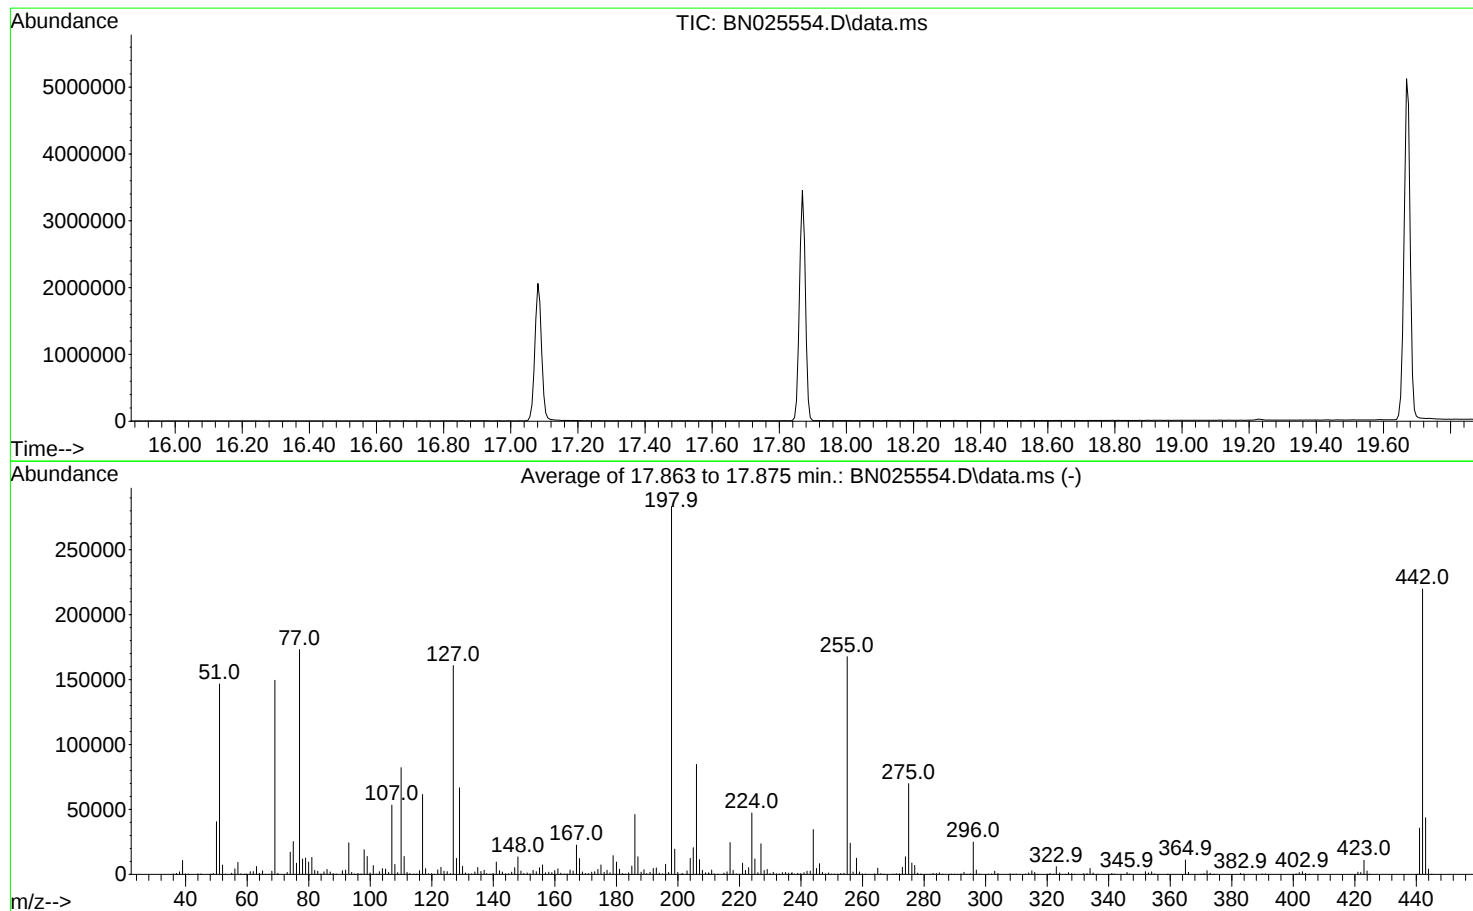

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.8	146619	PASS
68	69	0.00	2	1.7	2502	PASS
69	198	0.00	100	52.8	149445	PASS
70	69	0.00	2	0.6	857	PASS
127	198	10	80	56.8	160811	PASS
197	198	0.00	2	0.5	1443	PASS
198	198	100	100	100.0	283307	PASS
199	198	5	9	6.9	19528	PASS
275	198	10	60	24.7	69917	PASS
365	198	1	100	3.9	11089	PASS
441	198	0.01	100	12.6	35653	PASS
442	442	50	100	100.0	219691	PASS
443	442	15	24	19.9	43680	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/22/2023	BNA_N	<u>BN025554.D</u>
Compound Name	Response	Retention Time
DDT	1050382	20.904
DDD	10124	20.515
DDE	0	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10124	1060506	0.95

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
 Data File : BN025554.D
 Acq On : 23 May 2023 02:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 23 06:05:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 23 06:03:53 2023
 Response via : Initial Calibration

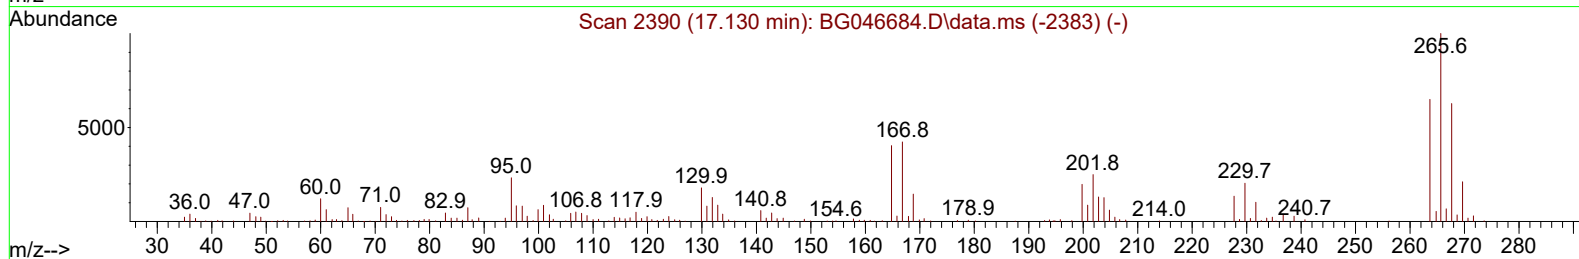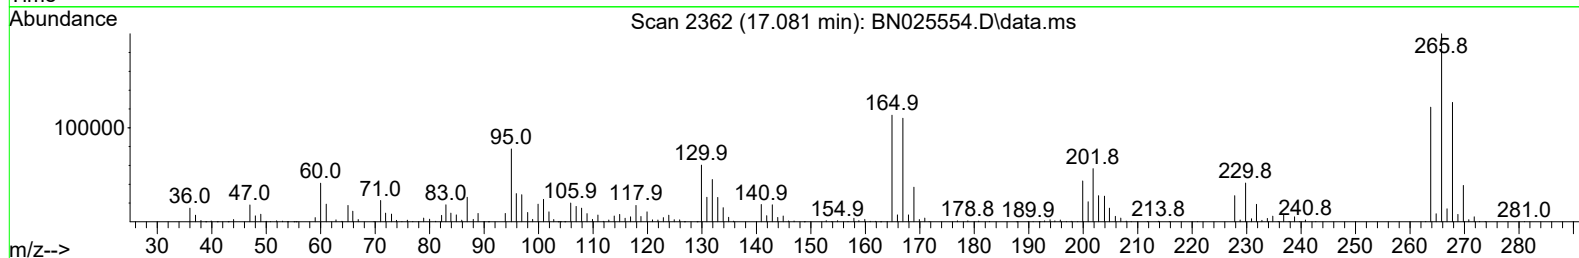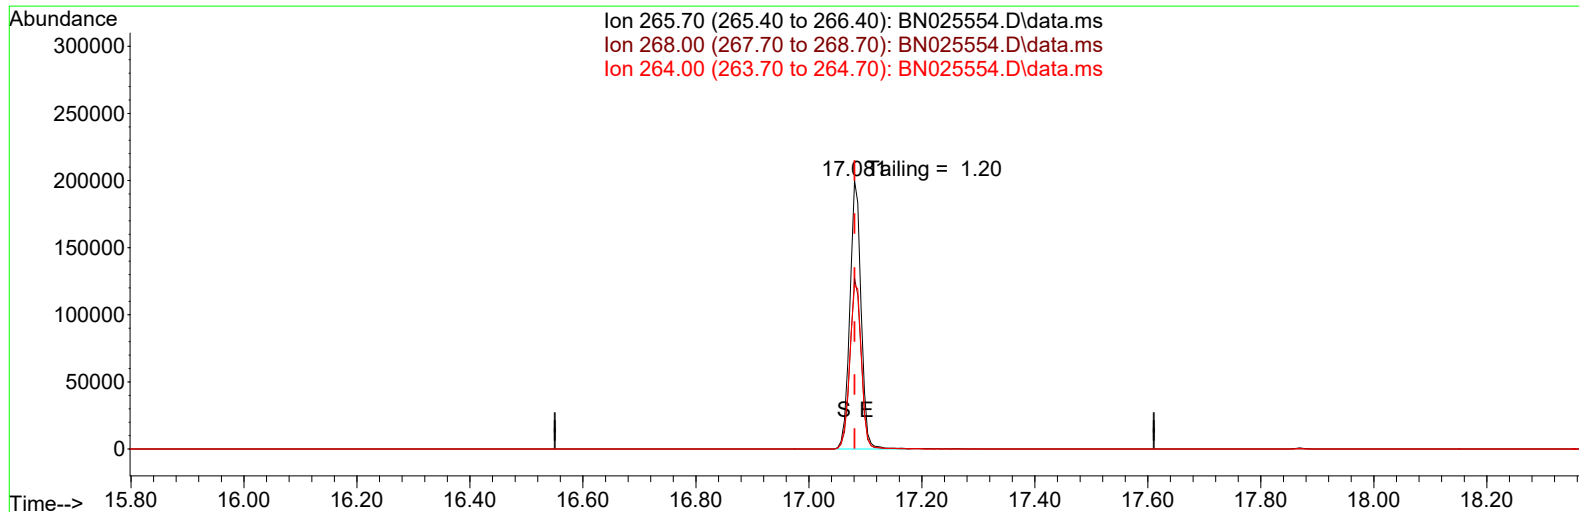

TIC: BN025554.D\data.ms

(70) Pentachlorophenol (C)

17.081min (+ 0.000) 14811.39 ng




response 276758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.50
264.00	61.60	60.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052223\
Data File : BN025554.D
Acq On : 23 May 2023 02:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 23 06:05:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 23 06:03:53 2023
Response via : Initial Calibration

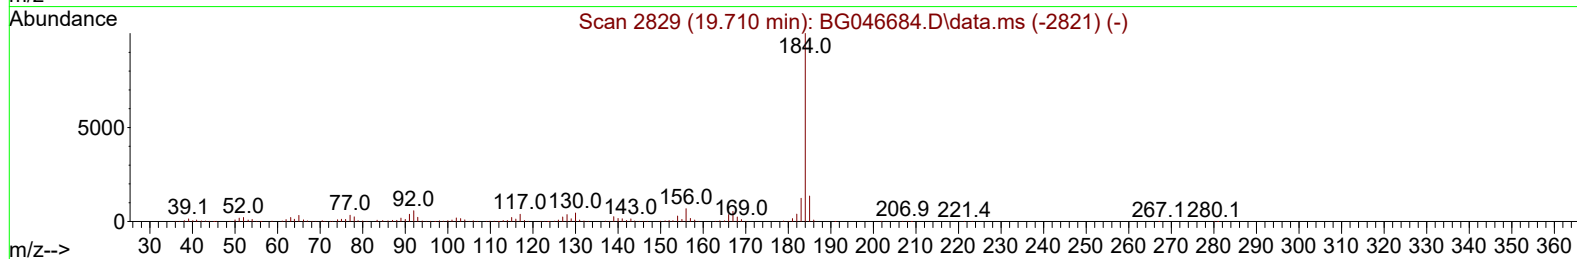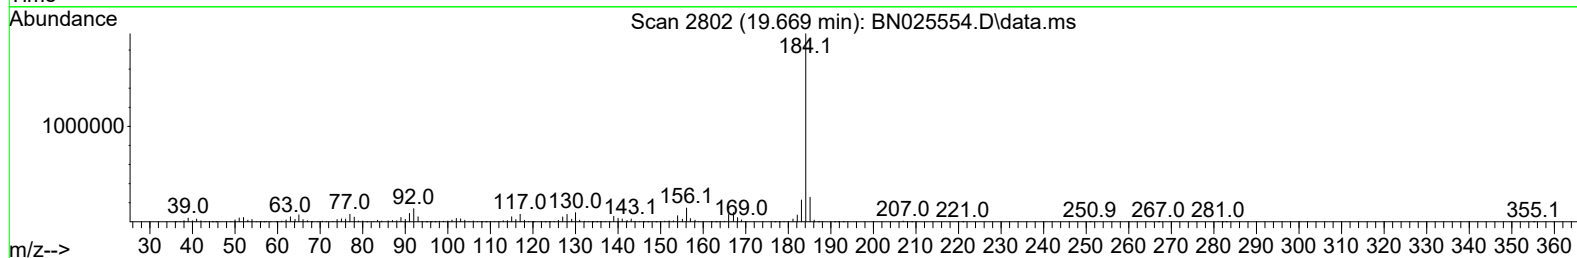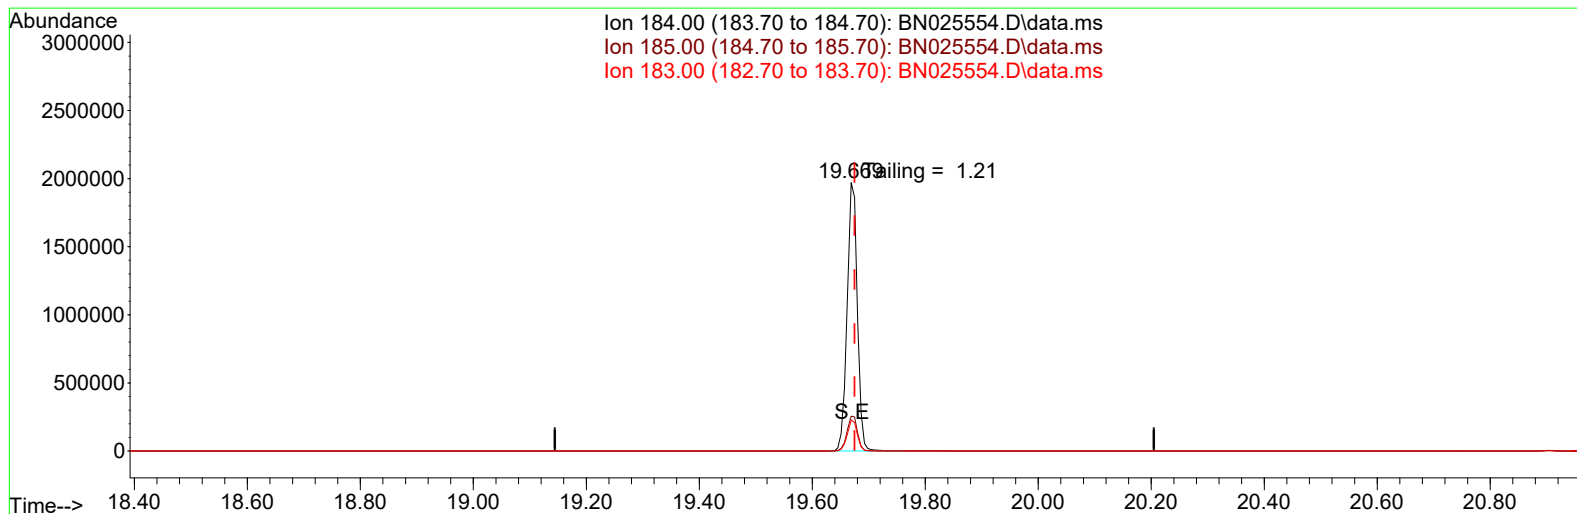

TIC: BN025554.D\data.ms

(77) Benzidine

19.669min (-0.006) 0.00 ng

response 2479245

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.56
0.00	0.00	0.00