

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031614.D
 Acq On : 22 May 2024 20:51
 Operator : MA/JU
 Sample : P2484-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9S5

Quant Time: May 22 23:09:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 23:42:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	508376	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	1994384	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.328	164	1082910	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.075	188	1987768	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1670867	20.000	ng/ul	0.00
88) Perylene-d12	24.239	264	1860660	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	71874	5.604	ng/uL	0.00
4) Pyridine-d5	3.605	84	955591	26.698	ng/ul	0.00
7) Phenol-d5	6.858	99	1265556	30.241	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	784936	31.273	ng/ul	0.00
11) 2-Chlorophenol-d4	7.222	132	991724	30.754	ng/ul	0.00
15) 4-Methylphenol-d8	8.387	113	966575	29.835	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	472056	31.274	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	430941	29.898	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	827531	29.364	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	1294941	31.876	ng/ul	0.00
46) Dimethylphthalate-d6	13.745	166	2310198	33.851	ng/ul	0.00
49) Acenaphthylene-d8	14.022	160	2932059	34.279	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	367712	28.477	ng/ul	0.00
60) Fluorene-d10	15.322	176	2054947	34.746	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	182017	21.180	ng/ul	0.00
73) Anthracene-d10	17.169	188	2799355	33.268	ng/ul	0.00
81) Pyrene-d10	19.469	212	3180803	30.350	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.039	264	3037854	34.685	ng/ul	0.00
Target Compounds						
55) 4-Nitrophenol	14.557	109	18216	1.872	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031614.D
Acq On : 22 May 2024 20:51
Operator : MA/JU
Sample : P2484-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S5


Quant Time: May 22 23:09:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 23:42:49 2024
Response via : Initial Calibration

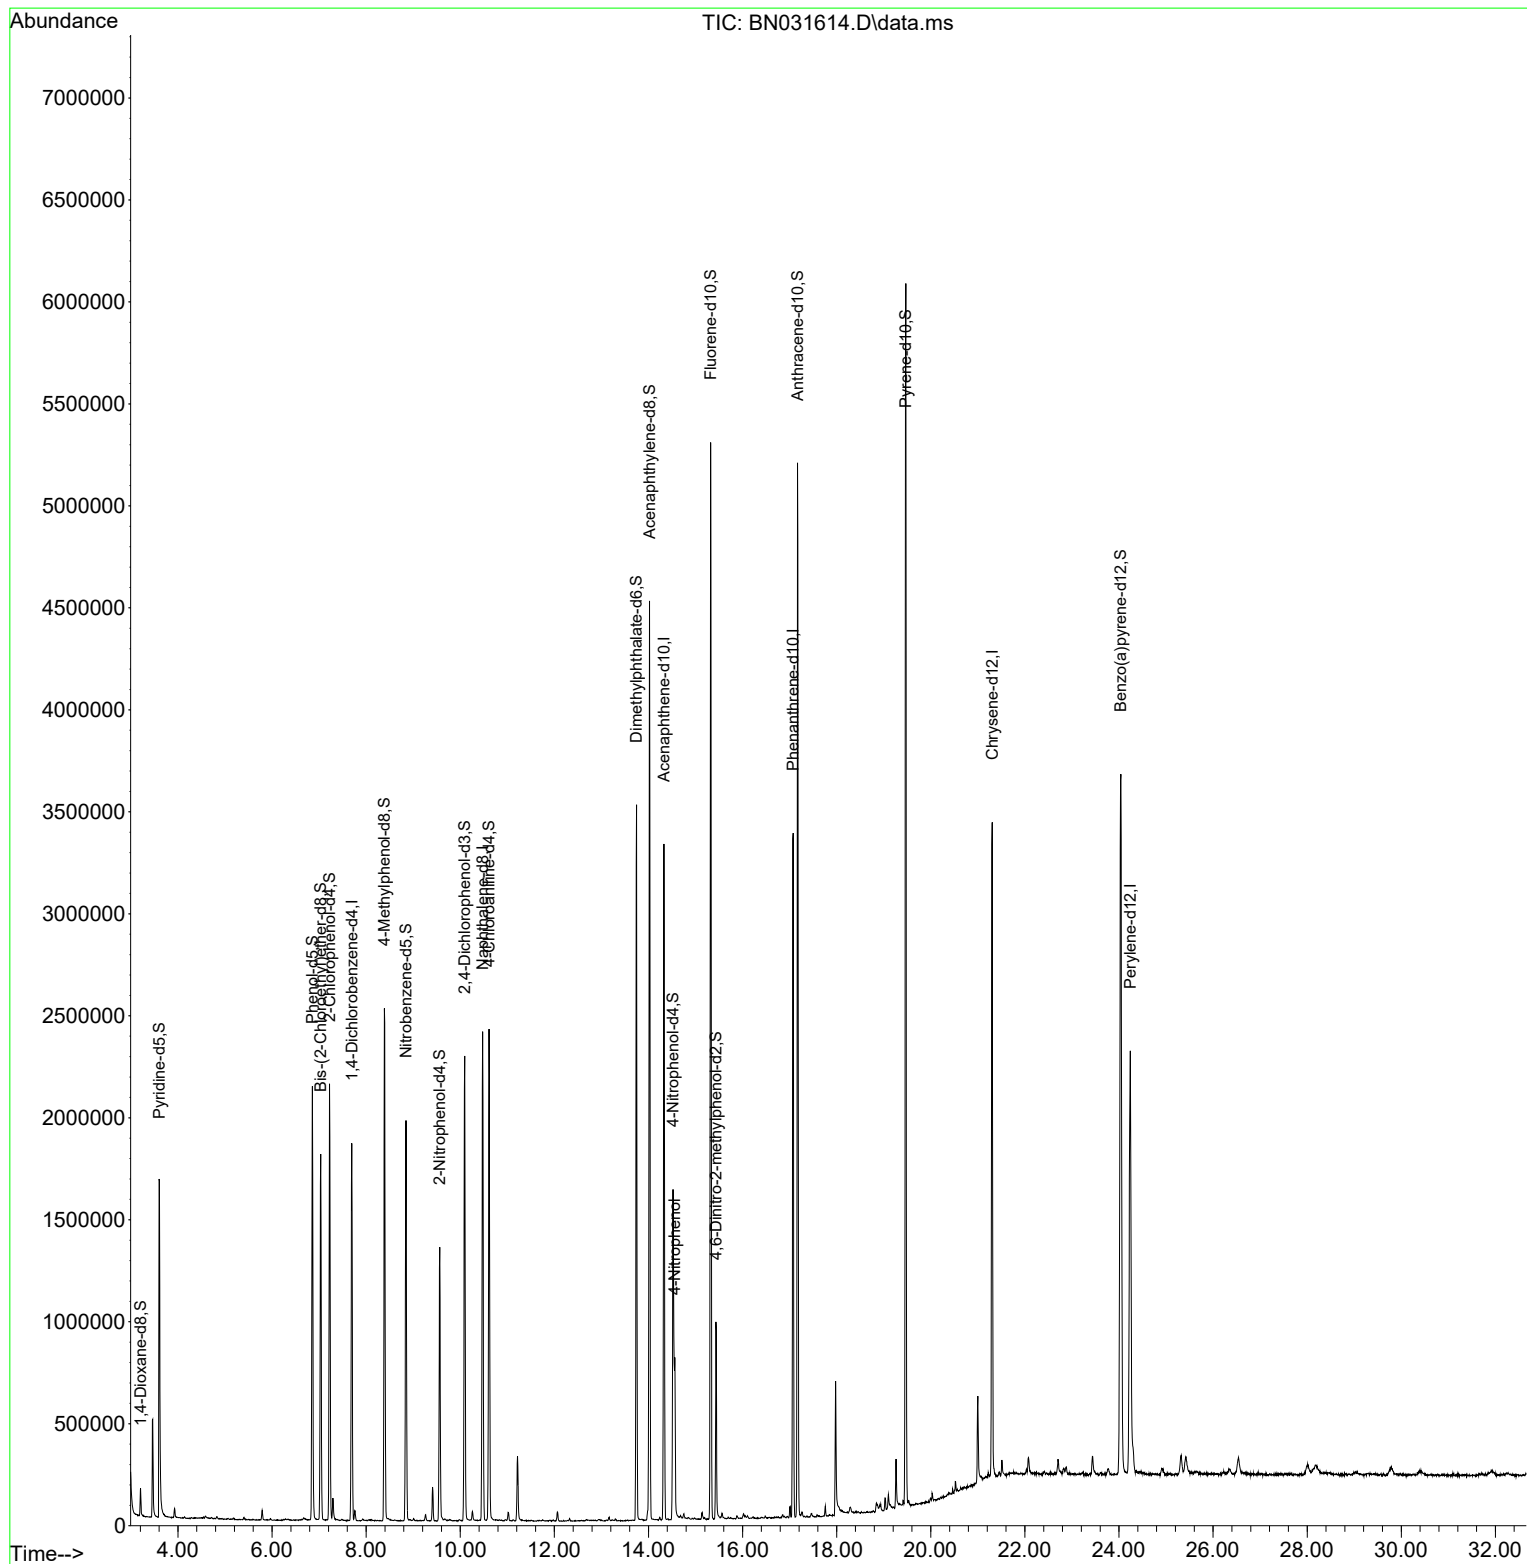

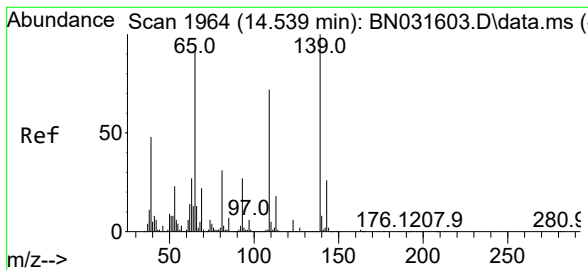

#55
 4-Nitrophenol
 Concen: 1.872 ng/ul
 RT: 14.557 min Scan# 1967
 Delta R.T. 0.018 min
 Lab File: BN031614.D
 Acq: 22 May 2024 20:51

Instrument :
 BNA_N
 ClientSampleId :
 BH9S5

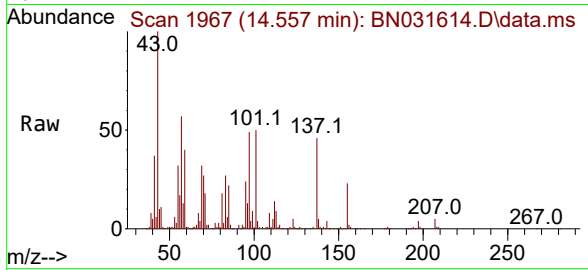

Tgt Ion	Ratio	Lower	Upper
109	100		
139	8.6	113.8	170.6#
65	17.5	101.1	151.7#

