

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031617.D
 Acq On : 22 May 2024 22:49
 Operator : MA/JU
 Sample : P2484-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q0

Quant Time: May 22 23:27:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 23:42:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	469088	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	1863447	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.328	164	1026400	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.075	188	1854228	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1512801	20.000	ng/ul	0.00
88) Perylene-d12	24.233	264	1760798	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	50852	4.297	ng/uL	0.00
4) Pyridine-d5	3.605	84	408932	12.382	ng/ul	0.00
7) Phenol-d5	6.857	99	948847	24.572	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	588780	25.422	ng/ul	0.00
11) 2-Chlorophenol-d4	7.222	132	743083	24.974	ng/ul	0.00
15) 4-Methylphenol-d8	8.387	113	503423	16.841	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	344479	24.426	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	309612	22.990	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	593743	22.549	ng/ul	0.00
31) 4-Chloroaniline-d4	10.610	131	782217	20.608	ng/ul	0.00
46) Dimethylphthalate-d6	13.745	166	1683246	26.023	ng/ul	0.00
49) Acenaphthylene-d8	14.022	160	2072993	25.570	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	237125	19.375	ng/ul	0.00
60) Fluorene-d10	15.322	176	1507953	26.901	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	120731	15.060	ng/ul	0.00
73) Anthracene-d10	17.169	188	1970161	25.100	ng/ul	0.00
81) Pyrene-d10	19.463	212	2454536	25.867	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.033	264	2323898	28.038	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.510	105	52102	1.117	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031617.D
Acq On : 22 May 2024 22:49
Operator : MA/JU
Sample : P2484-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9Q0

Quant Time: May 22 23:27:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 23:42:49 2024
Response via : Initial Calibration

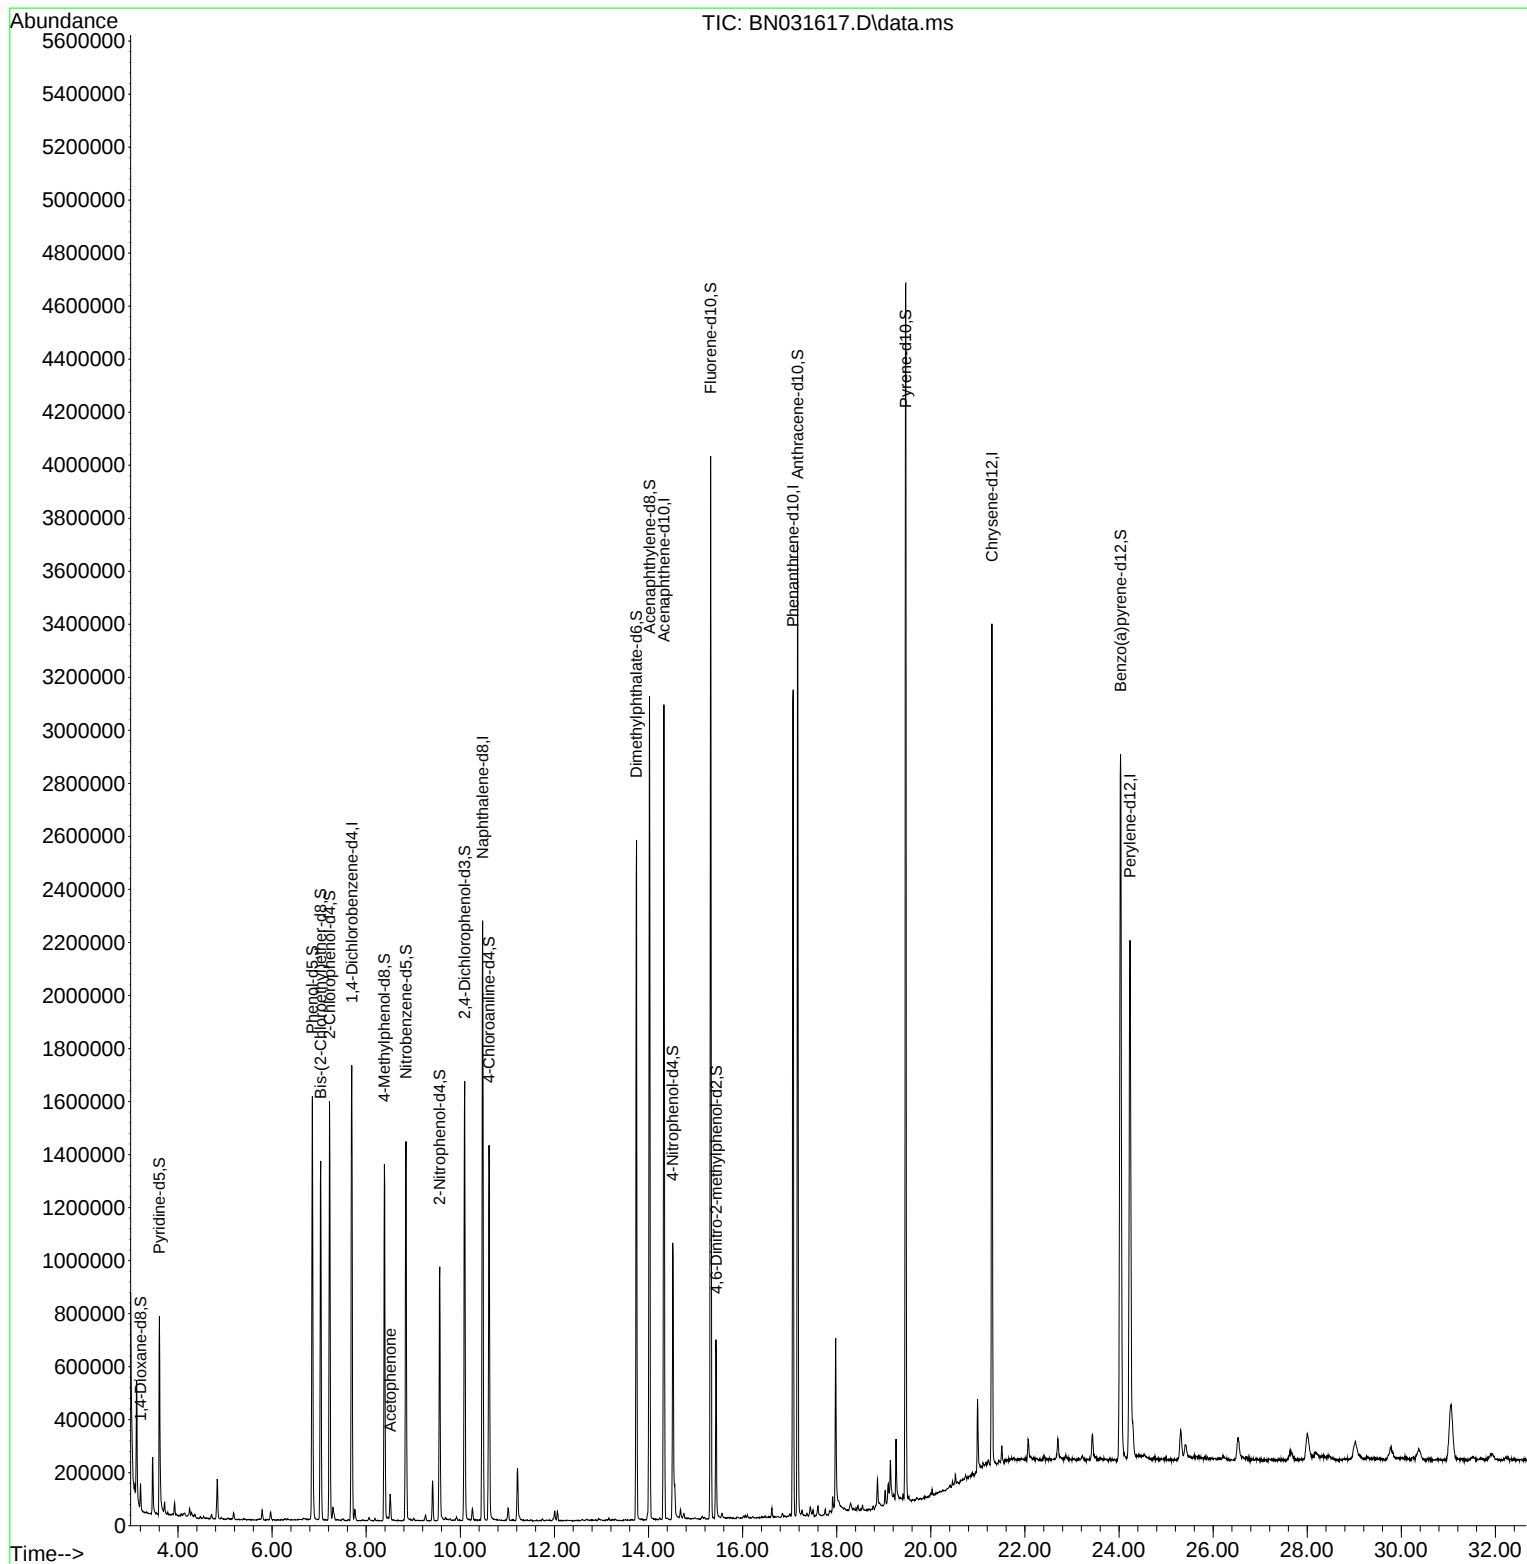

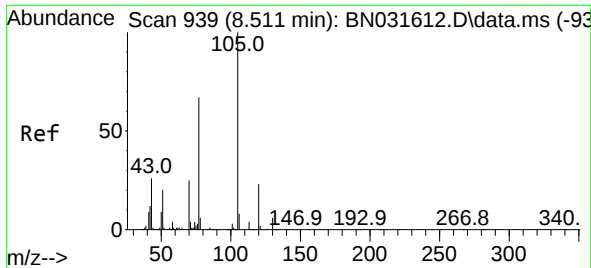

#16
 Acetophenone
 Concen: 1.117 ng/ul
 RT: 8.510 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN031617.D
 Acq: 22 May 2024 22:49

Instrument :
 BNA_N
 ClientSampleId :
 BH9Q0

Tgt Ion:105 Resp: 52102
 Ion Ratio Lower Upper
 105 100
 77 75.4 60.7 91.1
 51 24.9 18.6 28.0

