

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031604.D
 Acq On : 22 May 2024 09:47
 Operator : MA/JU
 Sample : PB160908BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK908

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rBV	130661	163281	1.86%	0.163%
2	3.599	101	104	130	rBV	1686119	2434763	27.70%	2.427%
3	3.922	155	159	166	rVB	31895	47929	0.55%	0.048%
4	4.140	191	196	202	rBV5	12325	18345	0.21%	0.018%
5	4.381	233	237	241	rBV5	5078	10130	0.12%	0.010%
6	4.540	260	264	269	rVB4	8314	11682	0.13%	0.012%
7	6.852	650	657	666	rBV	1806831	2839770	32.31%	2.830%
8	7.028	678	687	699	rVB	1539921	2463391	28.02%	2.455%
9	7.222	712	720	734	rBV	1783532	2868641	32.63%	2.859%
10	7.693	792	800	808	rBV	1507360	2481936	28.24%	2.474%
11	8.387	910	918	929	rBV	2314049	3598537	40.94%	3.586%
12	8.846	988	996	1007	rBV	1686011	2827746	32.17%	2.818%
13	9.557	1109	1117	1131	rBV	1234802	2049827	23.32%	2.043%
14	10.087	1197	1207	1217	rBV	2004389	3417605	38.88%	3.406%
15	10.475	1264	1273	1282	rVB	2194304	3726301	42.39%	3.714%
16	10.610	1288	1296	1309	rBV	2356225	3921052	44.61%	3.908%
17	12.063	1536	1543	1549	rBV	42560	69708	0.79%	0.069%
18	13.292	1747	1752	1759	rBV4	6639	14192	0.16%	0.014%
19	13.745	1821	1829	1839	rBV	3958632	5522980	62.83%	5.504%
20	14.022	1867	1876	1883	rBV	4489281	6750133	76.79%	6.727%
21	14.328	1921	1928	1935	rBV	3534246	5060824	57.57%	5.044%
22	14.516	1951	1960	1984	rBV	1743939	2659700	30.26%	2.651%
23	14.751	1995	2000	2003	rVB7	7465	12874	0.15%	0.013%
24	15.322	2090	2097	2105	rBV	5839270	8073868	91.85%	8.047%
25	15.434	2110	2116	2132	rVV	1192694	1686181	19.18%	1.680%
26	15.557	2134	2137	2145	rVB3	28085	46040	0.52%	0.046%
27	15.886	2190	2193	2199	rVB4	6212	8935	0.10%	0.009%
28	16.110	2226	2231	2234	rVB7	8291	12250	0.14%	0.012%
29	16.751	2337	2340	2347	rVB8	8405	9055	0.10%	0.009%
30	16.857	2354	2358	2366	rBV3	10616	15796	0.18%	0.016%
31	17.075	2388	2395	2403	rBV	3898597	5699609	64.84%	5.680%
32	17.169	2404	2411	2425	rVV	5933799	8428012	95.88%	8.400%
33	17.975	2544	2548	2558	rBV4	33160	61214	0.70%	0.061%
34	18.298	2600	2603	2608	rVB6	11146	15670	0.18%	0.016%
35	19.027	2723	2727	2733	rBV2	67845	92874	1.06%	0.093%
36	19.098	2735	2739	2744	rVB2	63420	87255	0.99%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031604.D
Acq On : 22 May 2024 09:47
Operator : MA/JU
Sample : PB160908BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK908

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

37	19.263	2764	2767	2772	rBV5	12312	21374	0.24%	0.021%
38	19.416	2790	2793	2795	rBV3	16927	17125	0.19%	0.017%
39	19.469	2795	2802	2812	rVV	6353260	8790125	100.00%	8.760%
40	21.304	3108	3114	3127	rBV	3038362	4492730	51.11%	4.478%
41	24.033	3570	3578	3596	rVB	2392735	5984824	68.09%	5.965%
42	24.233	3604	3612	3623	rBV2	1545842	3825111	43.52%	3.812%




Sum of corrected areas: 100339395

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031604.D
Acq On : 22 May 2024 09:47
Operator : MA/JU
Sample : PB160908BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK908

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

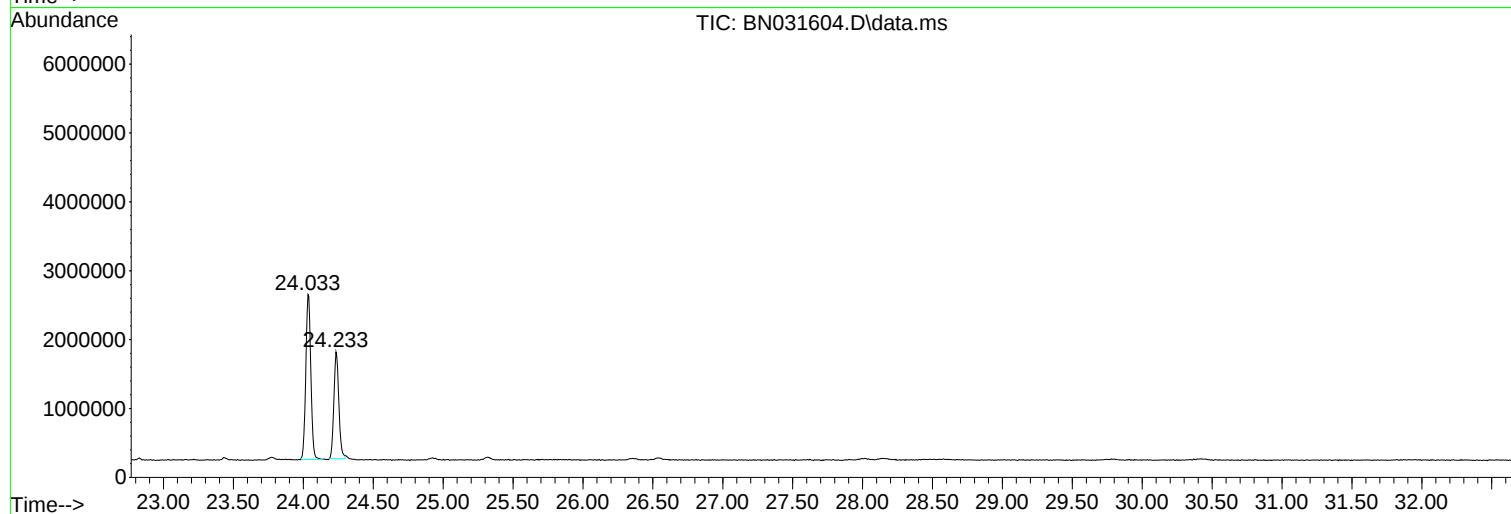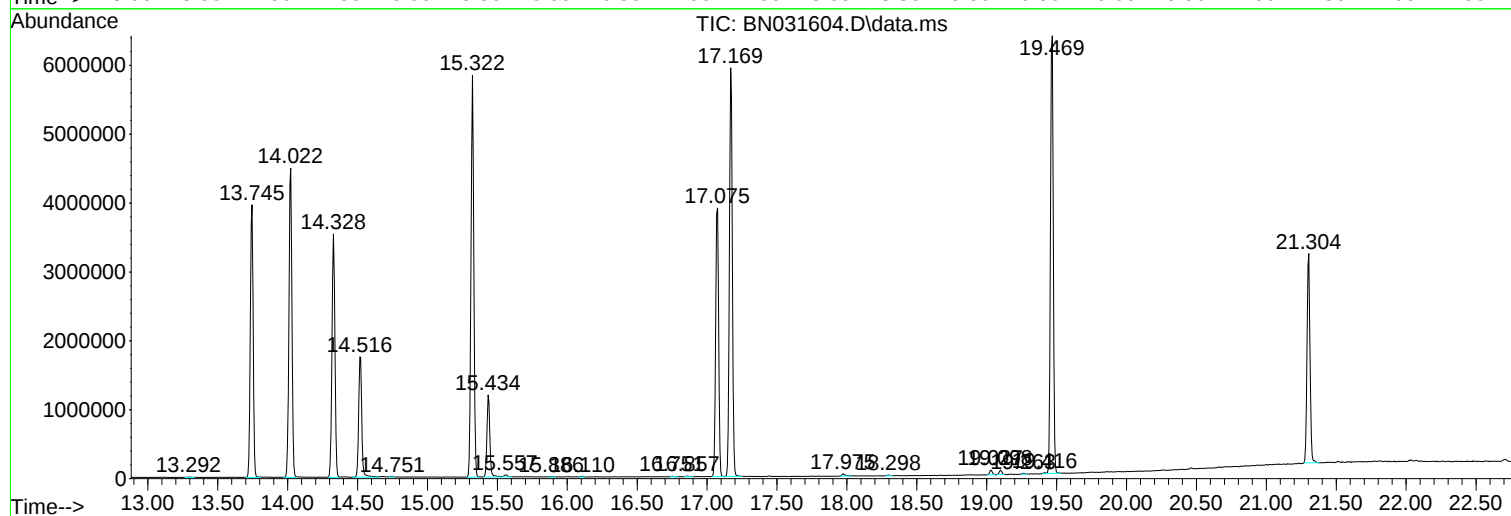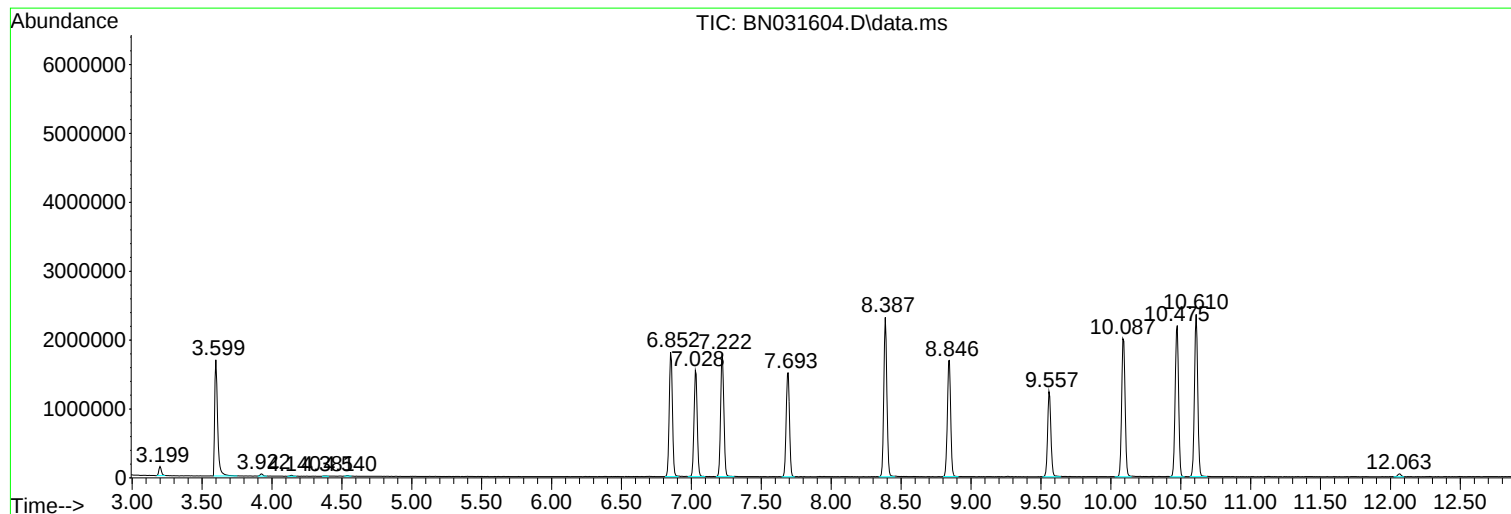

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031604.D
Acq On : 22 May 2024 09:47
Operator : MA/JU
Sample : PB160908BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK908

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031604.D
Acq On : 22 May 2024 09:47
Operator : MA/JU
Sample : PB160908BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK908

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------