

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031609.D
 Acq On : 22 May 2024 16:52
 Operator : MA/JU
 Sample : PB160913BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK913

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	46	rVB	128868	172118	2.05%	0.178%
2	3.599	101	104	121	rBV	1687574	2463473	29.30%	2.548%
3	3.922	154	159	166	rVB	37679	57102	0.68%	0.059%
4	4.140	191	196	203	rBV3	24456	36164	0.43%	0.037%
5	4.540	260	264	271	rVB3	18738	26728	0.32%	0.028%
6	6.852	650	657	672	rBV	1800932	2829764	33.66%	2.927%
7	7.028	681	687	699	rVB	1547496	2464594	29.31%	2.549%
8	7.222	712	720	735	rBV	1819480	2858541	34.00%	2.957%
9	7.693	791	800	807	rBV	1518434	2459902	29.26%	2.544%
10	8.387	907	918	933	rBV	2199063	3544739	42.16%	3.667%
11	8.846	988	996	1008	rBV	1691674	2767129	32.91%	2.862%
12	9.563	1110	1118	1127	rBV	1170875	1947499	23.16%	2.014%
13	10.093	1200	1208	1224	rBV	2016986	3350180	39.85%	3.465%
14	10.475	1265	1273	1282	rVB	2179292	3617396	43.03%	3.742%
15	10.610	1288	1296	1311	rBV	2288994	3822651	45.47%	3.954%
16	12.063	1538	1543	1550	rVB	38373	65435	0.78%	0.068%
17	13.293	1748	1752	1758	rVB5	6886	9831	0.12%	0.010%
18	13.745	1821	1829	1839	rBV	3712065	5289704	62.92%	5.471%
19	14.022	1868	1876	1884	rBV	4351846	6441833	76.62%	6.663%
20	14.328	1921	1928	1937	rBV	3338431	4874584	57.98%	5.042%
21	14.416	1939	1943	1947	rVB7	5520	9047	0.11%	0.009%
22	14.522	1954	1961	1974	rBV	1699265	2472921	29.41%	2.558%
23	14.745	1996	1999	2003	rVB6	5989	8724	0.10%	0.009%
24	15.322	2090	2097	2106	rBV	5457635	7720146	91.82%	7.985%
25	15.434	2110	2116	2127	rBV	1060588	1555833	18.51%	1.609%
26	15.563	2134	2138	2143	rVB2	25302	38368	0.46%	0.040%
27	16.857	2354	2358	2363	rBV4	7895	12013	0.14%	0.012%
28	17.075	2388	2395	2404	rBV	3793378	5433701	64.63%	5.620%
29	17.169	2405	2411	2425	rVV	5634280	7955083	94.62%	8.228%
30	17.451	2454	2459	2462	rBV4	6593	10652	0.13%	0.011%
31	17.975	2544	2548	2554	rBV4	27884	52545	0.62%	0.054%
32	18.298	2601	2603	2607	rVB5	8403	10266	0.12%	0.011%
33	18.869	2696	2700	2705	rBV7	13810	20418	0.24%	0.021%
34	19.033	2723	2728	2733	rBV	61487	89602	1.07%	0.093%
35	19.098	2735	2739	2744	rVB	63581	86842	1.03%	0.090%
36	19.263	2764	2767	2770	rBV4	11507	14938	0.18%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031609.D
Acq On : 22 May 2024 16:52
Operator : MA/JU
Sample : PB160913BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK913

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

37	19.416	2790	2793	2795	rBV2	22383	22857	0.27%	0.024%
38	19.469	2795	2802	2811	rVV	6417536	8407601	100.00%	8.696%
39	21.304	3108	3114	3127	rVB	3008912	4314808	51.32%	4.463%
40	24.039	3570	3579	3593	rBV2	2447063	5623377	66.88%	5.817%
41	24.239	3605	3613	3632	rVB	1485442	3719226	44.24%	3.847%




Sum of corrected areas: 96678335

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031609.D
Acq On : 22 May 2024 16:52
Operator : MA/JU
Sample : PB160913BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK913

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

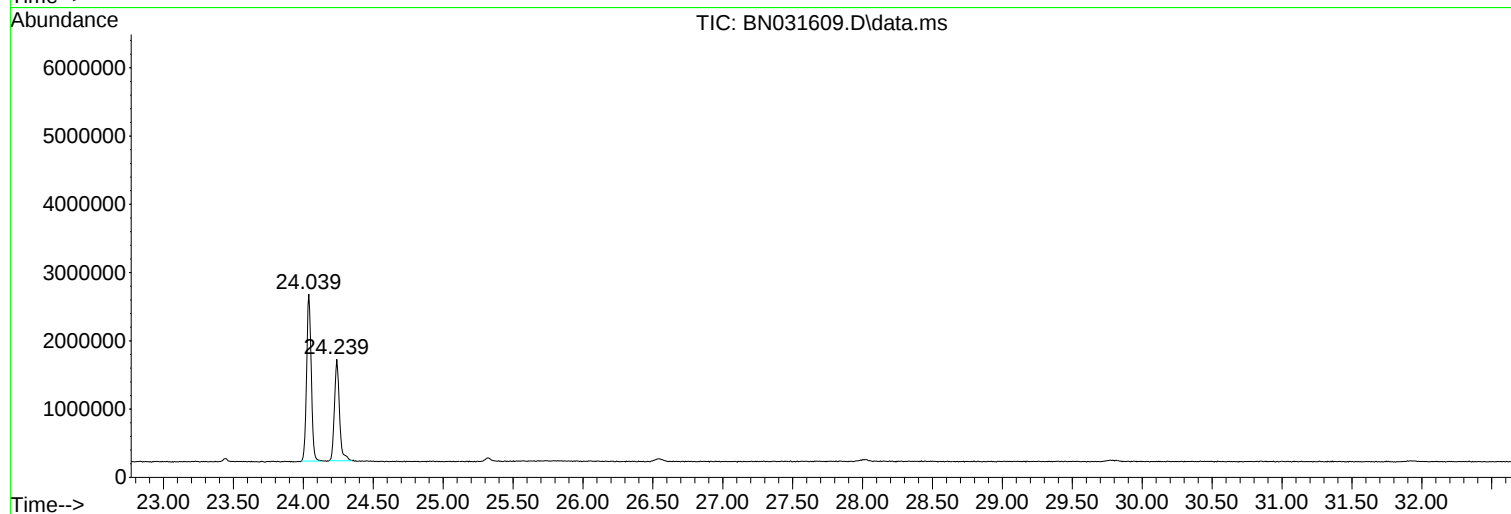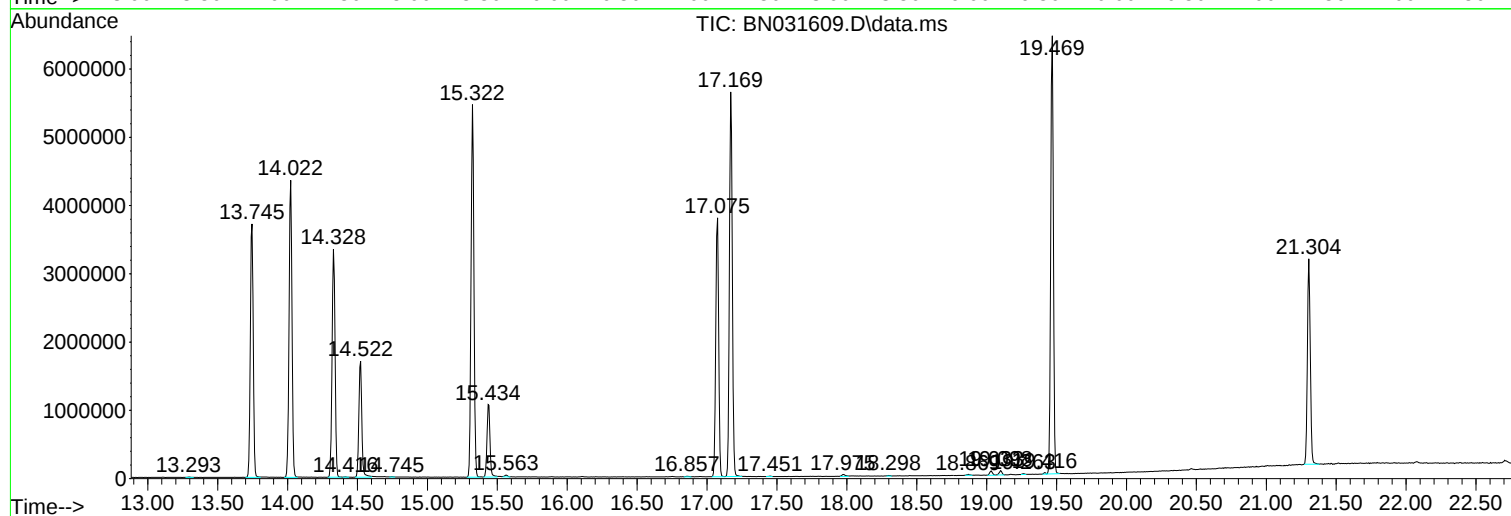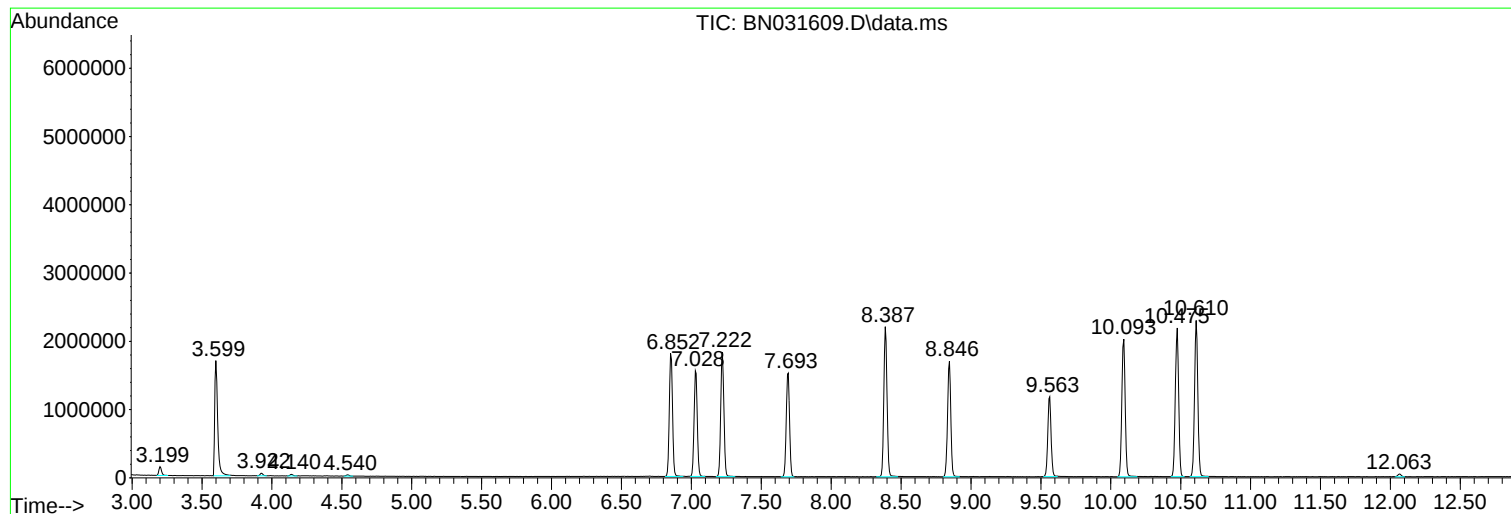

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031609.D
Acq On : 22 May 2024 16:52
Operator : MA/JU
Sample : PB160913BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK913

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031609.D
Acq On : 22 May 2024 16:52
Operator : MA/JU
Sample : PB160913BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK913

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc