

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031613.D
 Acq On : 22 May 2024 20:11
 Operator : MA/JU
 Sample : PB160987BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK987

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	29	rVB	51668	82363	0.66%	0.057%
2	3.199	32	36	50	rVB	154975	212674	1.69%	0.148%
3	3.599	101	104	122	rBV	2189284	3174808	25.26%	2.210%
4	3.928	155	160	169	rVB	71616	103131	0.82%	0.072%
5	4.140	192	196	202	rVB2	24147	33693	0.27%	0.023%
6	4.546	260	265	271	rVB3	17881	25261	0.20%	0.018%
7	6.858	650	658	669	rBV	2434289	3801298	30.24%	2.646%
8	7.034	681	688	698	rVB	2120861	3293271	26.20%	2.293%
9	7.222	712	720	731	rBV	2452708	3813988	30.34%	2.655%
10	7.693	792	800	810	rVB	2463543	3834069	30.50%	2.669%
11	8.387	910	918	932	rBV	2932066	4772484	37.97%	3.322%
12	8.846	987	996	1006	rBV	2308704	3738614	29.74%	2.603%
13	9.563	1110	1118	1129	rBV	1666234	2702735	21.50%	1.882%
14	10.093	1200	1208	1219	rBV	2718200	4561110	36.28%	3.175%
15	10.475	1265	1273	1283	rVB	3521021	5787773	46.04%	4.029%
16	10.610	1287	1296	1308	rBV	3142947	5212402	41.47%	3.629%
17	12.063	1537	1543	1549	rBV	53497	91006	0.72%	0.063%
18	13.745	1822	1829	1841	rBV	5343748	7494047	59.62%	5.217%
19	14.022	1869	1876	1886	rBV	6057438	8834676	70.28%	6.150%
20	14.328	1921	1928	1940	rBV	5226165	7781338	61.90%	5.417%
21	14.522	1953	1961	1977	rBV	2633209	3760391	29.91%	2.618%
22	14.739	1996	1998	2004	rVB6	9830	14702	0.12%	0.010%
23	15.322	2090	2097	2110	rBV	7463388	10773713	85.71%	7.500%
24	15.439	2110	2117	2130	rVV	1756830	2559245	20.36%	1.782%
25	15.563	2133	2138	2146	rVB2	35922	63861	0.51%	0.044%
26	16.857	2353	2358	2363	rBV	13710	24283	0.19%	0.017%
27	17.075	2388	2395	2402	rBV	6242438	8934961	71.08%	6.220%
28	17.169	2404	2411	2425	rBV2	7935256	11448016	91.07%	7.970%
29	17.451	2454	2459	2462	rBV3	10187	15046	0.12%	0.010%
30	17.975	2544	2548	2556	rBV6	27168	55034	0.44%	0.038%
31	18.298	2599	2603	2610	rBV6	11052	20263	0.16%	0.014%
32	18.863	2694	2699	2704	rBV3	29690	54577	0.43%	0.038%
33	19.027	2723	2727	2732	rBV	94675	129677	1.03%	0.090%
34	19.098	2734	2739	2746	rVB	94738	133192	1.06%	0.093%
35	19.263	2764	2767	2770	rBV5	15260	19179	0.15%	0.013%
36	19.416	2789	2793	2795	rBV2	30893	36609	0.29%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031613.D
Acq On : 22 May 2024 20:11
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

37	19.469	2795	2802	2810	rVV	8796780	12570374	100.00%	8.751%
38	20.463	2968	2971	2975	rVB4	31307	33664	0.27%	0.023%
39	21.304	3107	3114	3123	rBV	5225719	7798381	62.04%	5.429%
40	24.033	3569	3578	3595	rBV	3821435	9064886	72.11%	6.311%
41	24.239	3604	3613	3633	rVB	2718040	6785240	53.98%	4.724%




Sum of corrected areas: 143646035

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031613.D
Acq On : 22 May 2024 20:11
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

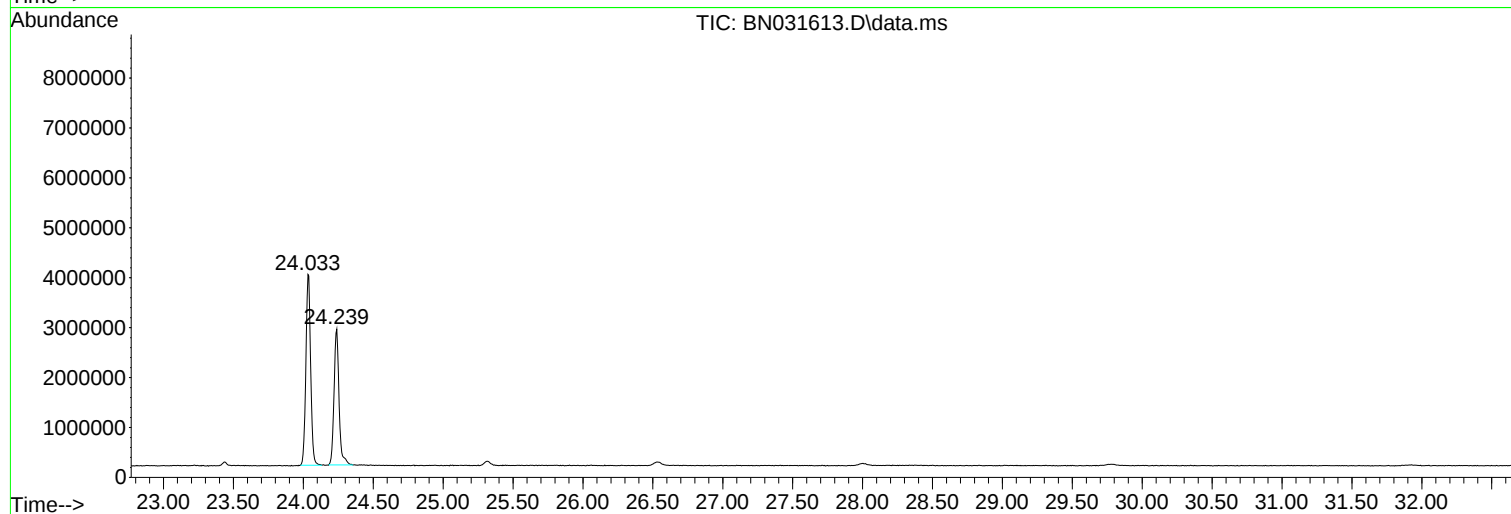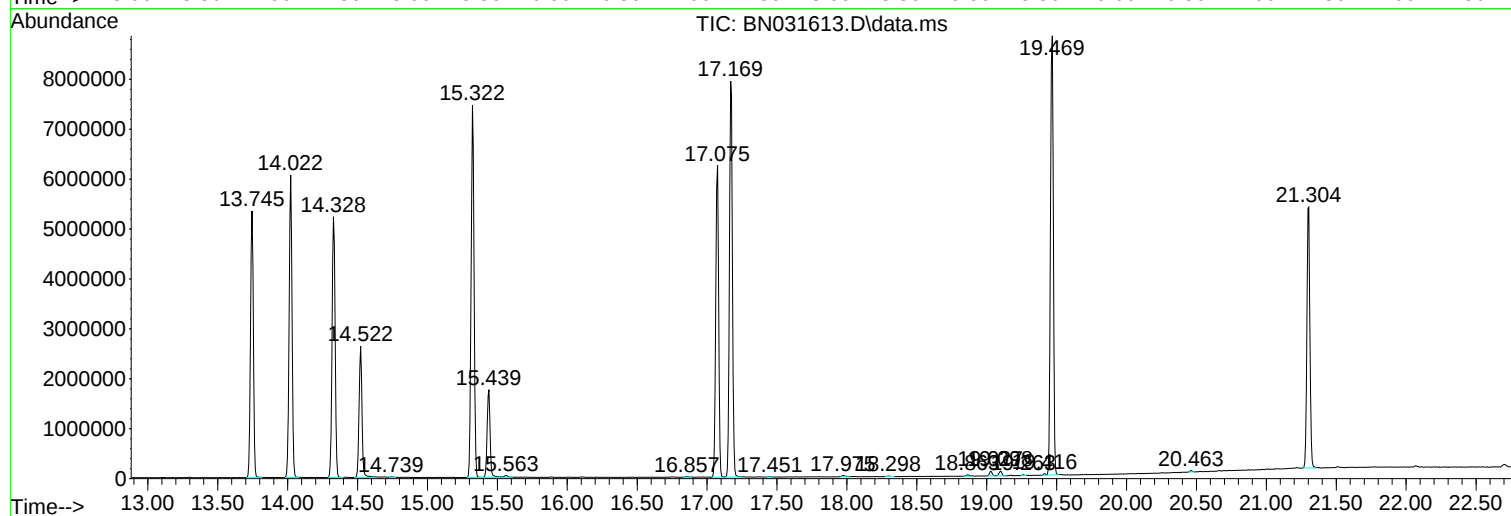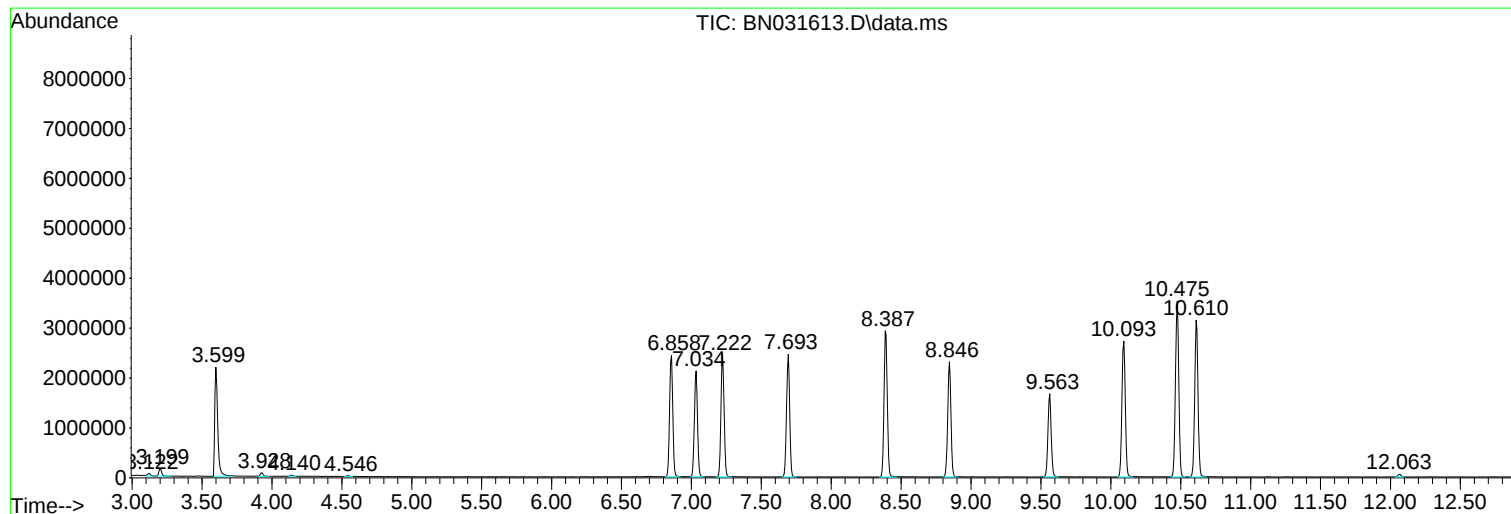

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031613.D
Acq On : 22 May 2024 20:11
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031613.D
Acq On : 22 May 2024 20:11
Operator : MA/JU
Sample : PB160987BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK987

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc