

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031615.D
 Acq On : 22 May 2024 21:30
 Operator : MA/JU
 Sample : P2484-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	48	rVB	108040	158625	1.71%	0.150%
2	3.464	77	81	92	rVB	56482	85422	0.92%	0.081%
3	3.599	101	104	120	rBV	1163936	1734953	18.70%	1.639%
4	3.928	155	160	164	rVB	42914	57354	0.62%	0.054%
5	4.146	193	197	202	rVB2	16555	23010	0.25%	0.022%
6	4.546	261	265	268	rVB2	10746	13269	0.14%	0.013%
7	5.787	471	476	483	rBV	32767	51840	0.56%	0.049%
8	5.963	501	506	511	rVB9	8698	14852	0.16%	0.014%
9	6.857	650	658	668	rBV	1596508	2575403	27.76%	2.433%
10	7.034	678	688	697	rBV	1626335	2549671	27.48%	2.409%
11	7.222	713	720	729	rBV	1417890	2207624	23.79%	2.086%
12	7.299	729	733	745	rVB5	15048	35180	0.38%	0.033%
13	7.693	793	800	807	rBV	2161471	3494936	37.67%	3.302%
14	7.757	807	811	818	rVB2	46602	78845	0.85%	0.074%
15	8.063	857	863	867	rBV7	4819	9616	0.10%	0.009%
16	8.387	909	918	928	rBV	2132925	3445143	37.13%	3.255%
17	8.846	988	996	1007	rBV	1821072	2925266	31.53%	2.764%
18	9.010	1018	1024	1030	rVB8	10812	20208	0.22%	0.019%
19	9.263	1060	1067	1072	rVB2	21924	36214	0.39%	0.034%
20	9.410	1086	1092	1099	rVB	134347	200025	2.16%	0.189%
21	9.563	1110	1118	1129	rBV	306070	546046	5.88%	0.516%
22	9.975	1183	1188	1194	rBV10	6180	13119	0.14%	0.012%
23	10.093	1200	1208	1216	rBV	1250797	2059468	22.20%	1.946%
24	10.257	1229	1236	1243	rBV2	30088	53697	0.58%	0.051%
25	10.475	1265	1273	1281	rBV	3102741	5178524	55.81%	4.893%
26	10.610	1286	1296	1307	rBV	2389504	4072884	43.89%	3.848%
27	11.016	1359	1365	1373	rVB	44842	68581	0.74%	0.065%
28	11.122	1377	1383	1388	rBV6	5319	9282	0.10%	0.009%
29	11.216	1392	1399	1412	rBV	231978	415028	4.47%	0.392%
30	11.651	1468	1473	1477	rBV6	5018	10105	0.11%	0.010%
31	11.975	1522	1528	1534	rVB4	6482	13874	0.15%	0.013%
32	12.063	1534	1543	1549	rBV2	44326	80110	0.86%	0.076%
33	12.140	1549	1556	1560	rBV3	8787	14685	0.16%	0.014%
34	12.357	1590	1593	1601	rVB4	6813	10767	0.12%	0.010%
35	13.163	1725	1730	1736	rVV4	15738	24621	0.27%	0.023%
36	13.298	1747	1753	1758	rBV6	10413	18657	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031615.D
 Acq On : 22 May 2024 21:30
 Operator : MA/JU
 Sample : P2484-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9T0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

37	13.651	1808	1813	1816	rBV6	5067	9983	0.11%	0.009%
38	13.745	1822	1829	1838	rBV	4196892	5655328	60.95%	5.343%
39	14.022	1863	1876	1892	rBV	4719643	7219569	77.81%	6.821%
40	14.239	1909	1913	1917	rVB5	15388	20407	0.22%	0.019%

41	14.328	1920	1928	1937	rBV	4565620	6869414	74.03%	6.490%
42	14.522	1953	1961	1965	rBV3	138370	324154	3.49%	0.306%
43	14.557	1965	1967	1978	rVB	133737	175444	1.89%	0.166%
44	14.751	1995	2000	2005	rBV6	16256	28595	0.31%	0.027%
45	15.139	2061	2066	2072	rBV2	26464	47679	0.51%	0.045%

46	15.192	2072	2075	2080	rVB5	11675	16768	0.18%	0.016%
47	15.322	2090	2097	2106	rBV	5936091	8697184	93.73%	8.217%
48	15.433	2112	2116	2120	rVB4	16363	23180	0.25%	0.022%
49	15.563	2134	2138	2142	rBV2	25131	40423	0.44%	0.038%
50	15.881	2188	2192	2200	rBV9	8526	17737	0.19%	0.017%

51	16.022	2211	2216	2219	rBV	30731	46400	0.50%	0.044%
52	16.051	2219	2221	2224	rVV4	16053	19645	0.21%	0.019%
53	16.104	2228	2230	2234	rVB4	10397	13165	0.14%	0.012%
54	16.216	2246	2249	2259	rVB9	8332	19000	0.20%	0.018%
55	16.751	2337	2340	2344	rVB5	8605	11974	0.13%	0.011%

56	16.845	2353	2356	2361	rBV4	18174	28773	0.31%	0.027%
57	16.886	2361	2363	2368	rVB6	8430	12262	0.13%	0.012%
58	16.951	2368	2374	2379	rBV3	15325	26189	0.28%	0.025%
59	17.004	2379	2383	2387	rVB6	13191	17813	0.19%	0.017%
60	17.075	2387	2395	2404	rBV	5430560	7650588	82.45%	7.228%

61	17.169	2405	2411	2424	rVV	6061228	8682970	93.58%	8.204%
62	17.269	2424	2428	2432	rVB7	14571	21863	0.24%	0.021%
63	17.369	2443	2445	2451	rVB4	9401	13474	0.15%	0.013%
64	17.445	2455	2458	2464	rVV5	7935	13973	0.15%	0.013%
65	17.751	2507	2510	2515	rVB4	13174	17579	0.19%	0.017%

66	17.975	2543	2548	2556	rBV3	51218	94497	1.02%	0.089%
67	18.286	2597	2601	2608	rVB8	13410	29245	0.32%	0.028%
68	18.863	2696	2699	2705	rVB2	24868	32570	0.35%	0.031%
69	18.910	2705	2707	2711	rBV3	9206	10815	0.12%	0.010%
70	19.027	2723	2727	2732	rVB2	73293	101746	1.10%	0.096%

71	19.098	2735	2739	2744	rVB	74876	100565	1.08%	0.095%
72	19.257	2764	2766	2772	rBV6	15915	22440	0.24%	0.021%
73	19.416	2789	2793	2796	rBV3	28174	40330	0.43%	0.038%
74	19.463	2796	2801	2809	rVV2	6772324	9278772	100.00%	8.767%
75	19.527	2810	2812	2819	rVB3	31279	40550	0.44%	0.038%

76	20.027	2894	2897	2902	rBV2	44743	56810	0.61%	0.054%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031615.D
Acq On : 22 May 2024 21:30
Operator : MA/JU
Sample : P2484-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

77	20.527	2979	2982	2985	rVB	65553	65844	0.71%	0.062%
78	20.998	3057	3062	3072	rBV3	251607	450370	4.85%	0.426%
79	21.298	3107	3113	3123	rVB2	3859185	5867801	63.24%	5.544%
80	21.510	3146	3149	3158	rVB2	81545	110033	1.19%	0.104%
81	24.039	3569	3579	3594	rVB2	2533271	6252033	67.38%	5.907%
82	24.233	3604	3612	3630	rVB2	1990483	5236847	56.44%	4.948%




Sum of corrected areas: 105839705

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031615.D
Acq On : 22 May 2024 21:30
Operator : MA/JU
Sample : P2484-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

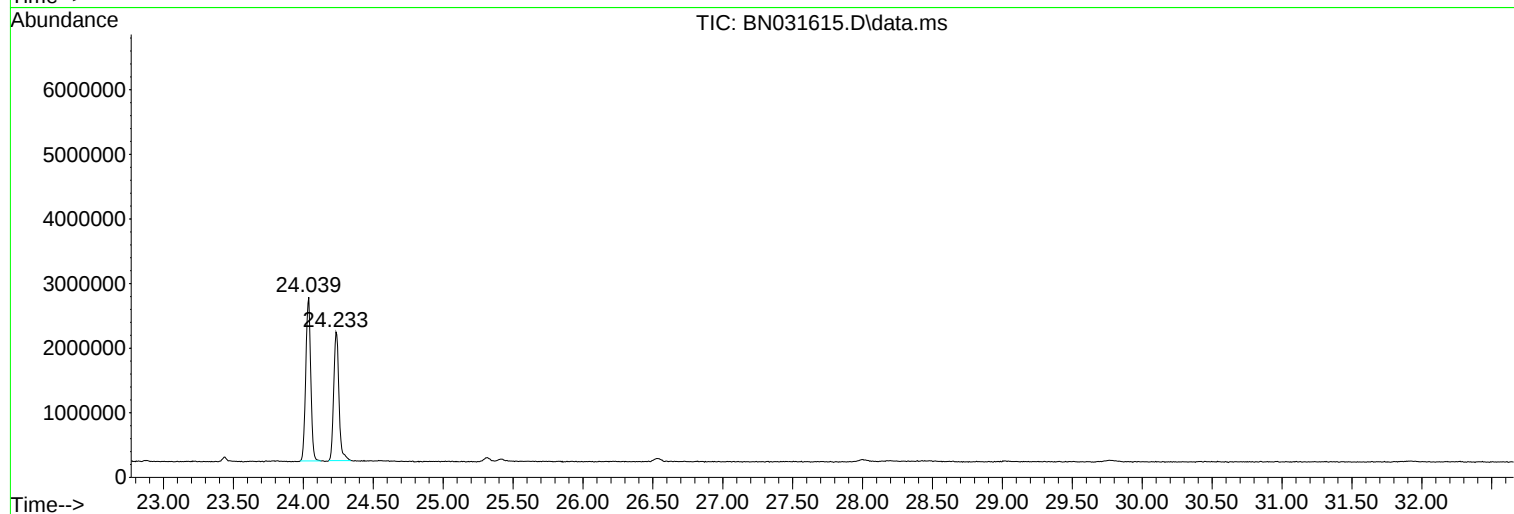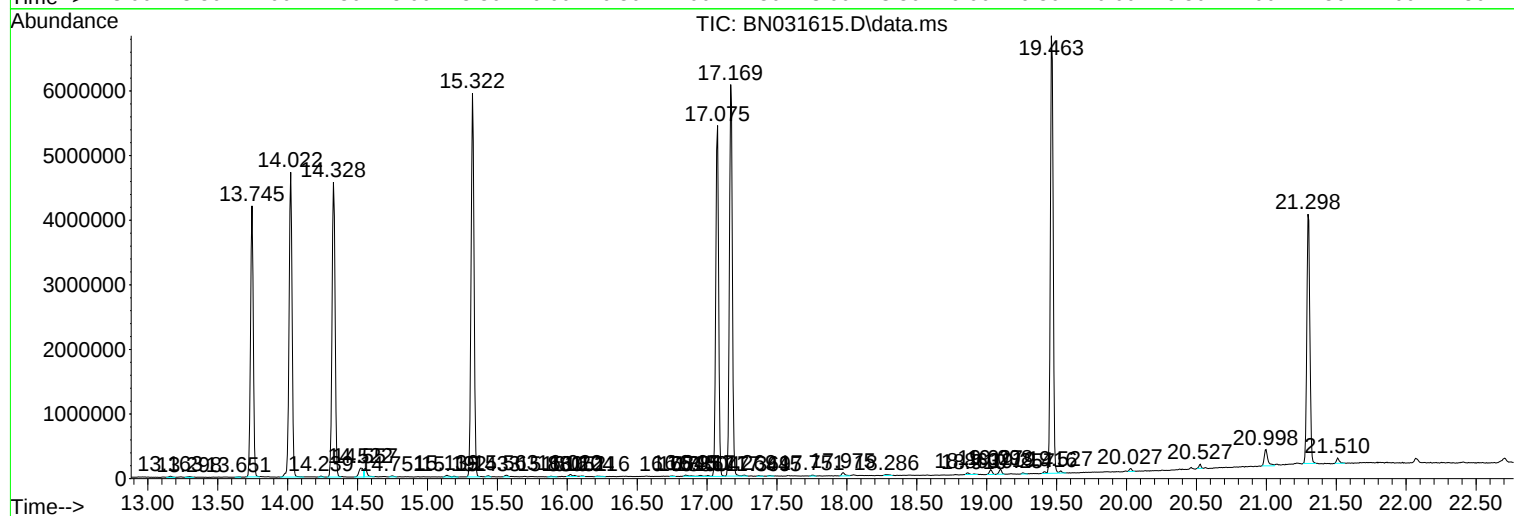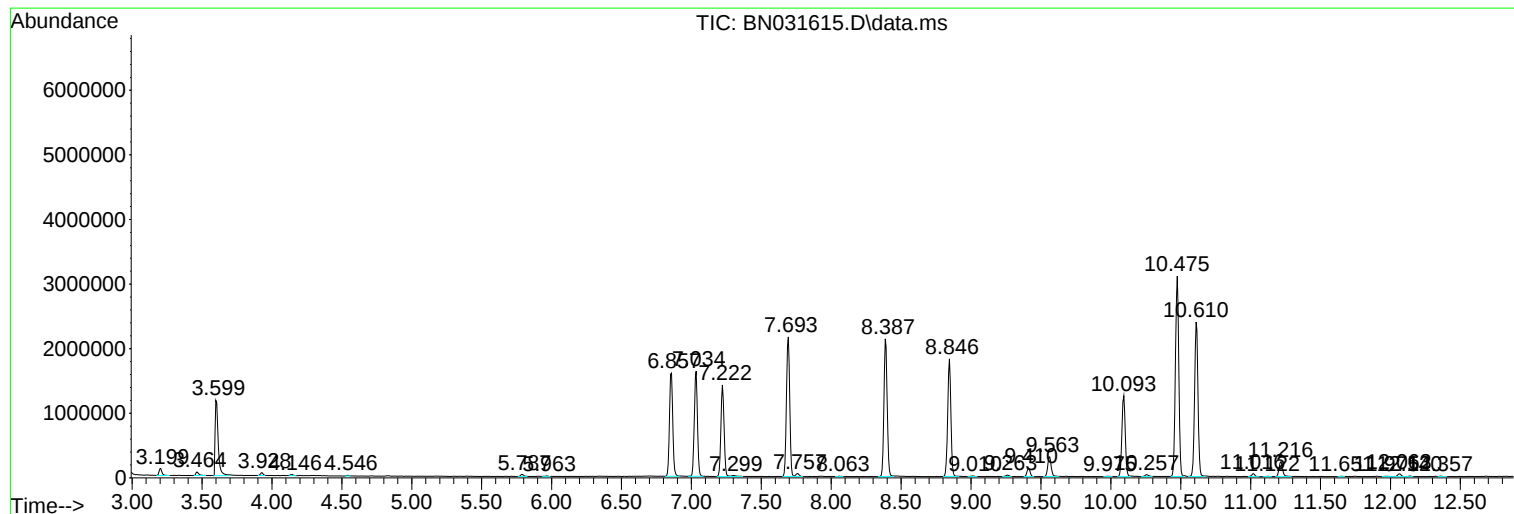

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031615.D
Acq On : 22 May 2024 21:30
Operator : MA/JU
Sample : P2484-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031615.D
Acq On : 22 May 2024 21:30
Operator : MA/JU
Sample : P2484-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9T0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc