

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031620.D
 Acq On : 23 May 2024 00:48
 Operator : MA/JU
 Sample : P2484-24
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9S7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	32	37	44	rVB	93517	132241	1.92%	0.145%
2	3.464	76	81	92	rBV	173167	254489	3.69%	0.280%
3	3.605	102	105	120	rBV	884529	1336008	19.39%	1.467%
4	3.922	156	159	164	rBV	33968	50007	0.73%	0.055%
5	4.246	210	214	220	rVB	29521	40498	0.59%	0.044%
6	4.834	309	314	324	rVB	107894	155766	2.26%	0.171%
7	5.058	349	352	359	rBV7	5102	7827	0.11%	0.009%
8	5.187	370	374	377	rVB5	5305	8818	0.13%	0.010%
9	5.787	471	476	486	rBV	37070	58061	0.84%	0.064%
10	5.969	504	507	510	rVB4	6474	7432	0.11%	0.008%
11	6.675	622	627	631	rBV7	4243	8842	0.13%	0.010%
12	6.858	650	658	669	rBV	1495042	2442233	35.45%	2.682%
13	7.034	679	688	699	rVB	1276884	2042208	29.64%	2.243%
14	7.222	712	720	728	rBV	1525688	2394783	34.76%	2.630%
15	7.293	728	732	743	rVV	45276	87045	1.26%	0.096%
16	7.693	791	800	807	rBV	2049867	3282154	47.64%	3.605%
17	7.763	807	812	820	rVB2	41586	69769	1.01%	0.077%
18	8.387	907	918	928	rBV	1877558	3004966	43.62%	3.300%
19	8.846	988	996	1007	rBV	1410920	2322848	33.72%	2.551%
20	9.004	1020	1023	1028	rVB7	8356	13984	0.20%	0.015%
21	9.263	1062	1067	1071	rVB	16429	28453	0.41%	0.031%
22	9.410	1085	1092	1100	rBV	160115	246940	3.58%	0.271%
23	9.563	1110	1118	1133	rBV	948957	1599581	23.22%	1.757%
24	9.781	1149	1155	1162	rVB9	5064	11146	0.16%	0.012%
25	10.093	1200	1208	1223	rBV	1697718	2871506	41.68%	3.154%
26	10.257	1229	1236	1242	rBV2	49052	83008	1.20%	0.091%
27	10.475	1263	1273	1282	rBV	2940278	4903035	71.17%	5.385%
28	10.610	1287	1296	1305	rBV	1873967	3099805	44.99%	3.405%
29	11.016	1360	1365	1372	rVB	46371	71412	1.04%	0.078%
30	11.122	1379	1383	1390	rVB7	5730	11016	0.16%	0.012%
31	11.216	1392	1399	1411	rBV	224869	401925	5.83%	0.441%
32	12.063	1538	1543	1549	rVB	32046	55375	0.80%	0.061%
33	12.687	1642	1649	1653	rBV8	5527	13003	0.19%	0.014%
34	12.957	1688	1695	1698	rBV9	5846	13815	0.20%	0.015%
35	13.157	1725	1729	1733	rBV4	10572	15350	0.22%	0.017%
36	13.298	1748	1753	1758	rVB7	8548	15691	0.23%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
 Data File : BN031620.D
 Acq On : 23 May 2024 00:48
 Operator : MA/JU
 Sample : P2484-24
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9S7

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

37	13.745	1822	1829	1837	rBV	2877356	4121660	59.82%	4.527%
38	14.022	1864	1876	1887	rBV	3597449	5407718	78.49%	5.940%
39	14.239	1908	1913	1916	rVB7	7620	11366	0.16%	0.012%
40	14.328	1921	1928	1935	rBV	4276310	6401039	92.91%	7.031%
41	14.522	1953	1961	1978	rBV	1119847	1953401	28.35%	2.146%
42	14.687	1986	1989	1993	rVB6	7038	10233	0.15%	0.011%
43	14.745	1994	1999	2006	rVV10	15834	31366	0.46%	0.034%
44	15.134	2061	2065	2071	rBV2	11226	20326	0.30%	0.022%
45	15.192	2071	2075	2080	rVB5	9122	11836	0.17%	0.013%
46	15.322	2090	2097	2108	rBV	4385229	6283040	91.20%	6.901%
47	15.434	2110	2116	2131	rBV	672098	978842	14.21%	1.075%
48	15.563	2131	2138	2143	rVV3	19764	31315	0.45%	0.034%
49	15.686	2153	2159	2160	rBV6	4466	7202	0.10%	0.008%
50	15.886	2189	2193	2198	rVB8	8848	12230	0.18%	0.013%
51	16.057	2218	2222	2223	rBV3	6816	8634	0.13%	0.009%
52	16.104	2228	2230	2236	rVB6	8100	11692	0.17%	0.013%
53	16.563	2305	2308	2314	rBV7	5460	9711	0.14%	0.011%
54	16.851	2351	2357	2361	rBV4	16721	32314	0.47%	0.035%
55	17.010	2379	2384	2387	rBV4	11551	14693	0.21%	0.016%
56	17.069	2387	2394	2404	rVV	4779432	6889653	100.00%	7.567%
57	17.169	2405	2411	2423	rVV2	4318320	6107449	88.65%	6.708%
58	17.263	2424	2427	2431	rVB5	19863	28510	0.41%	0.031%
59	17.463	2458	2461	2466	rVB6	8175	12197	0.18%	0.013%
60	17.757	2507	2511	2516	rVB2	22532	29503	0.43%	0.032%
61	17.839	2523	2525	2530	rBV4	6394	9694	0.14%	0.011%
62	17.922	2535	2539	2541	rBV5	6230	8916	0.13%	0.010%
63	17.975	2543	2548	2557	rBV	297590	435077	6.31%	0.478%
64	18.298	2597	2603	2608	rBV7	19618	40033	0.58%	0.044%
65	18.410	2619	2622	2626	rBV5	9361	10728	0.16%	0.012%
66	18.863	2692	2699	2705	rBV7	30521	73838	1.07%	0.081%
67	19.027	2723	2727	2733	rBV3	53994	74057	1.07%	0.081%
68	19.098	2735	2739	2743	rBV	53275	75646	1.10%	0.083%
69	19.257	2762	2766	2773	rBV3	95263	143214	2.08%	0.157%
70	19.416	2789	2793	2795	rBV4	33038	39922	0.58%	0.044%
71	19.463	2795	2801	2809	rVV	4383027	6192004	89.87%	6.801%
72	20.022	2894	2896	2901	rBV4	18804	25875	0.38%	0.028%
73	20.522	2979	2981	2984	rVB3	41373	39966	0.58%	0.044%
74	20.992	3057	3061	3068	rBV3	178546	298431	4.33%	0.328%
75	21.298	3107	3113	3122	rVB2	3439886	4926486	71.51%	5.411%
76	24.033	3569	3578	3590	rVB2	1803780	4310486	62.56%	4.734%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031620.D
Acq On : 23 May 2024 00:48
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

77	24.233	3603	3612	3626	rBV	1816823	4754547	69.01%	5.222%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 91045890

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031620.D
Acq On : 23 May 2024 00:48
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

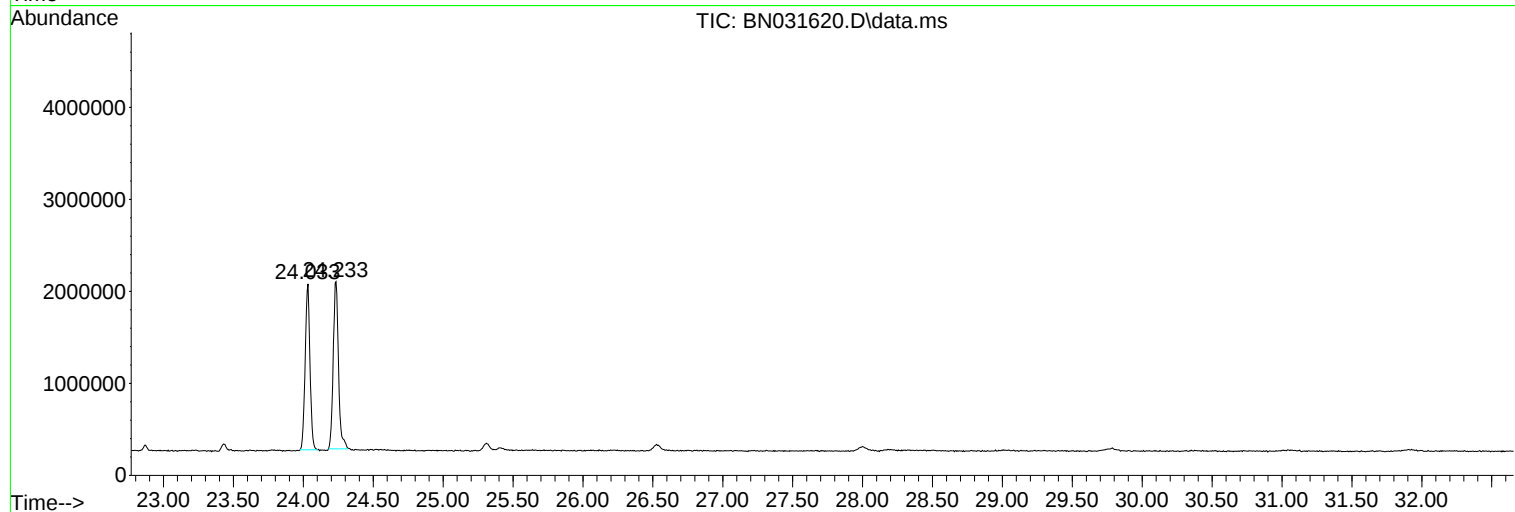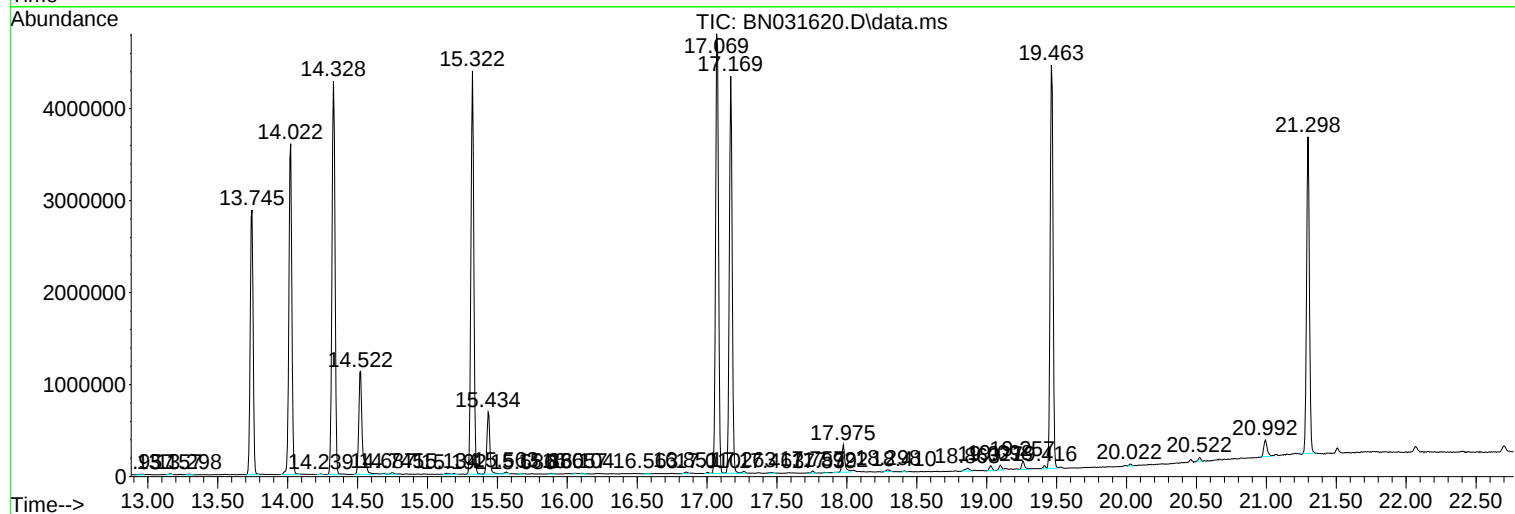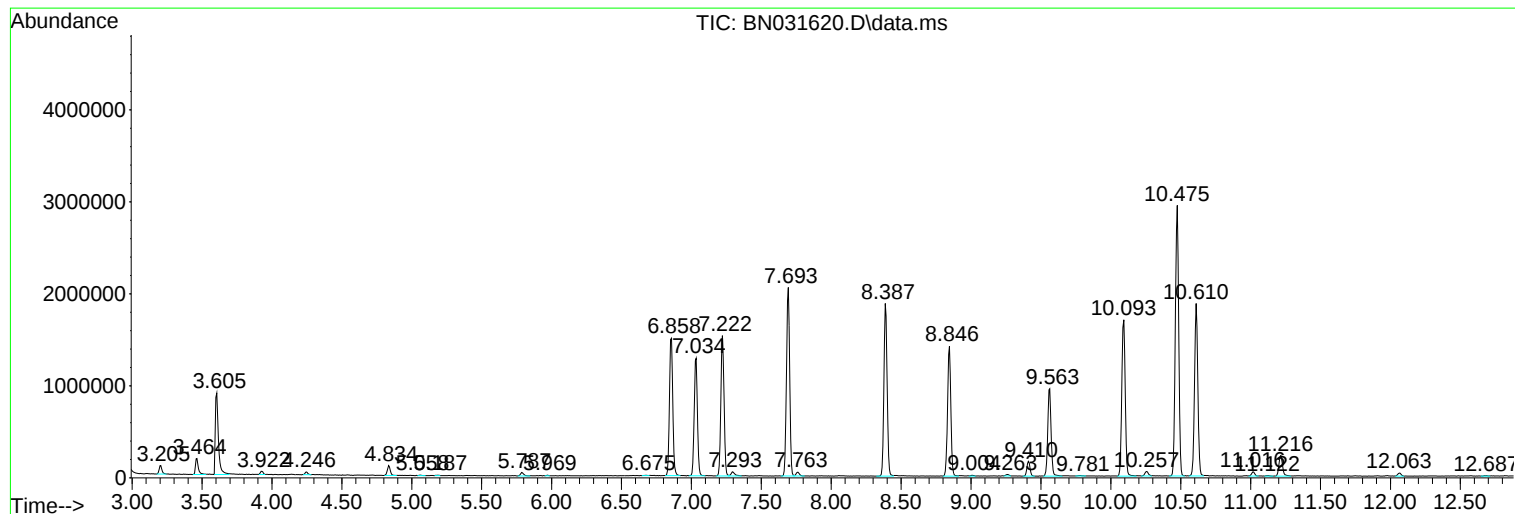

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031620.D
Acq On : 23 May 2024 00:48
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052224\
Data File : BN031620.D
Acq On : 23 May 2024 00:48
Operator : MA/JU
Sample : P2484-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9S7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------