
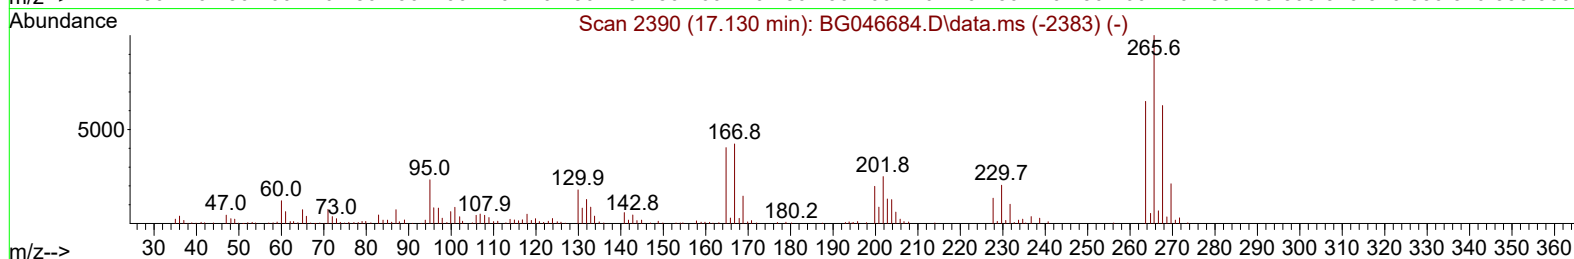
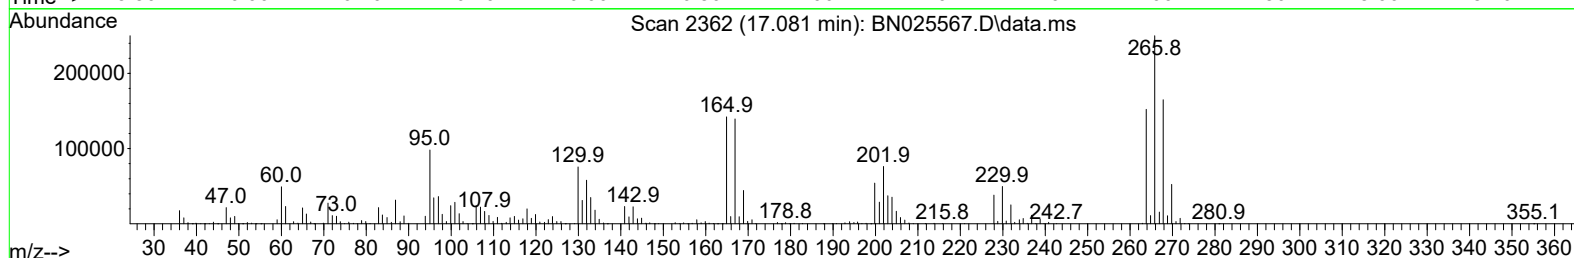


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052323\
 Data File : BN025567.D
 Acq On : 23 May 2023 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 07:02:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 07:02:20 2023
 Response via : Initial Calibration

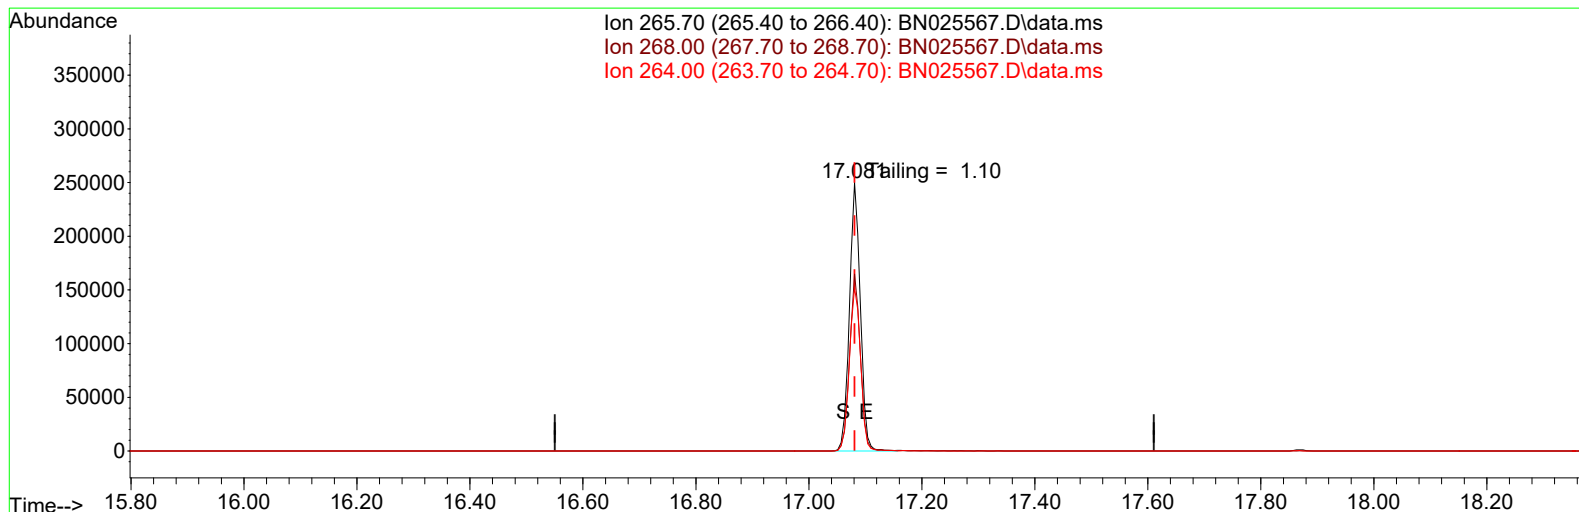

TIC: BN025567.D\data.ms

(70) Pentachlorophenol (C)




17.081min (0.000) 17650.24 ng

response 335898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.94
264.00	61.60	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052323\
Data File : BN025567.D
Acq On : 23 May 2023 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 07:02:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 07:02:20 2023
Response via : Initial Calibration

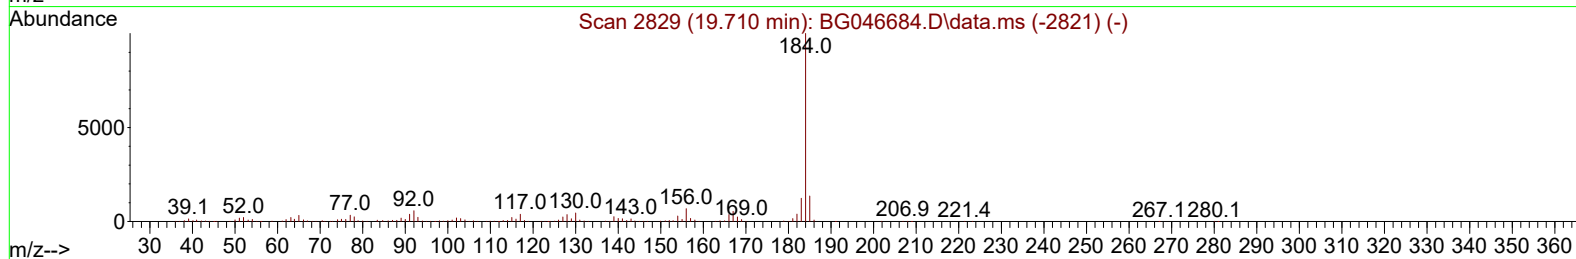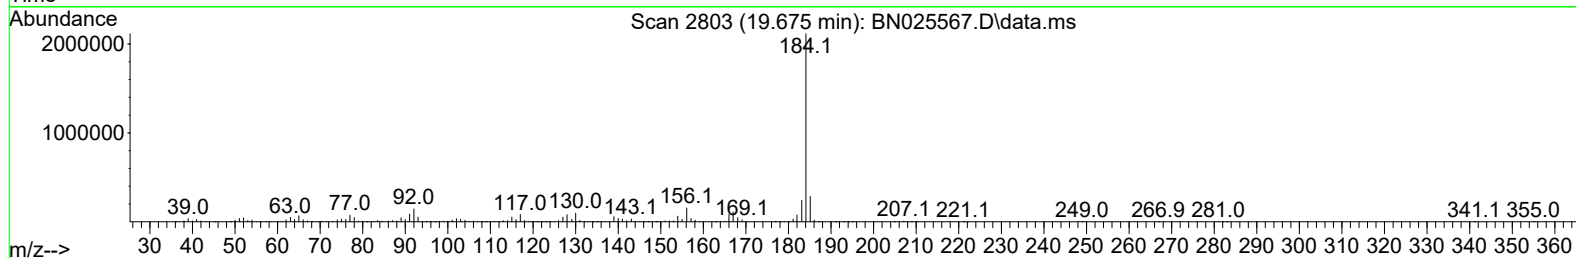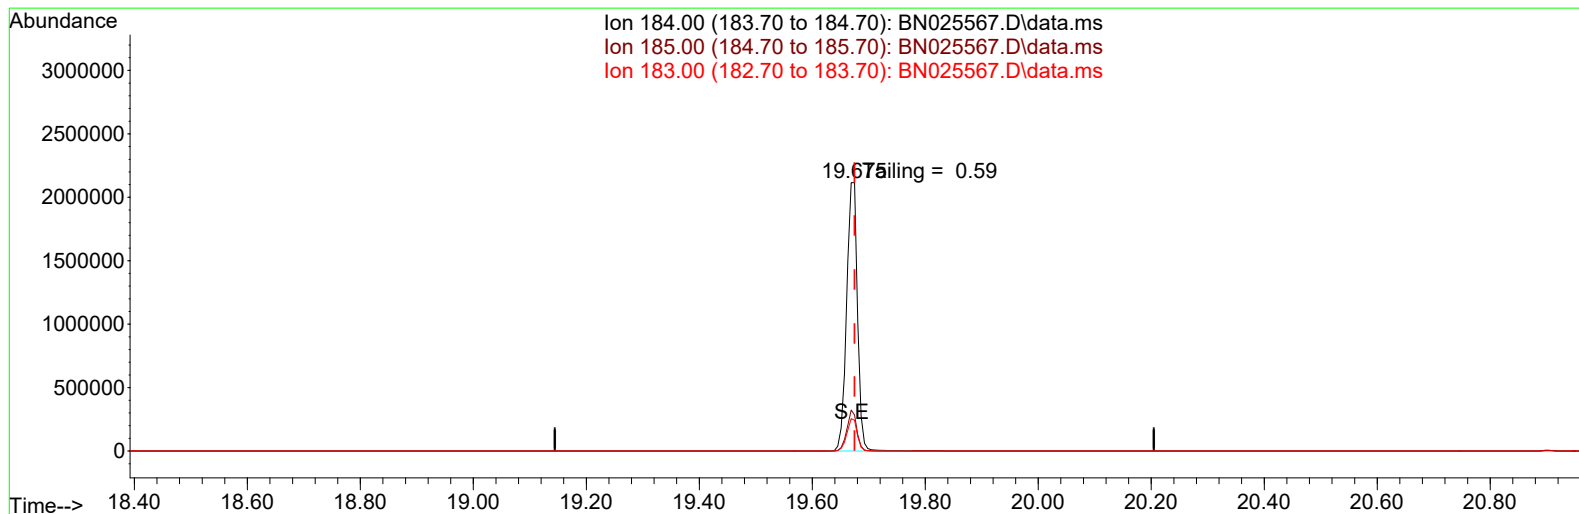

TIC: BN025567.D\data.ms

(77) Benzidine

19.675min (0.000) 0.00 ng

response 2830466

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.43
183.00	13.20	11.46
0.00	0.00	0.00