
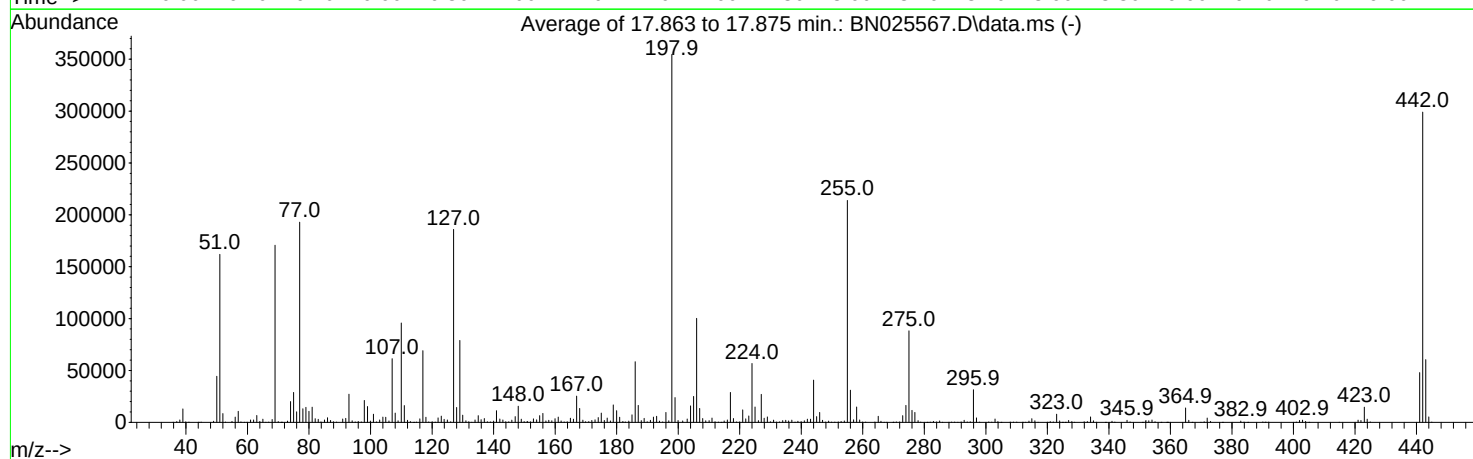


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052323\
Data File : BN025567.D
Acq On : 23 May 2023 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 23 03:22:57 2023

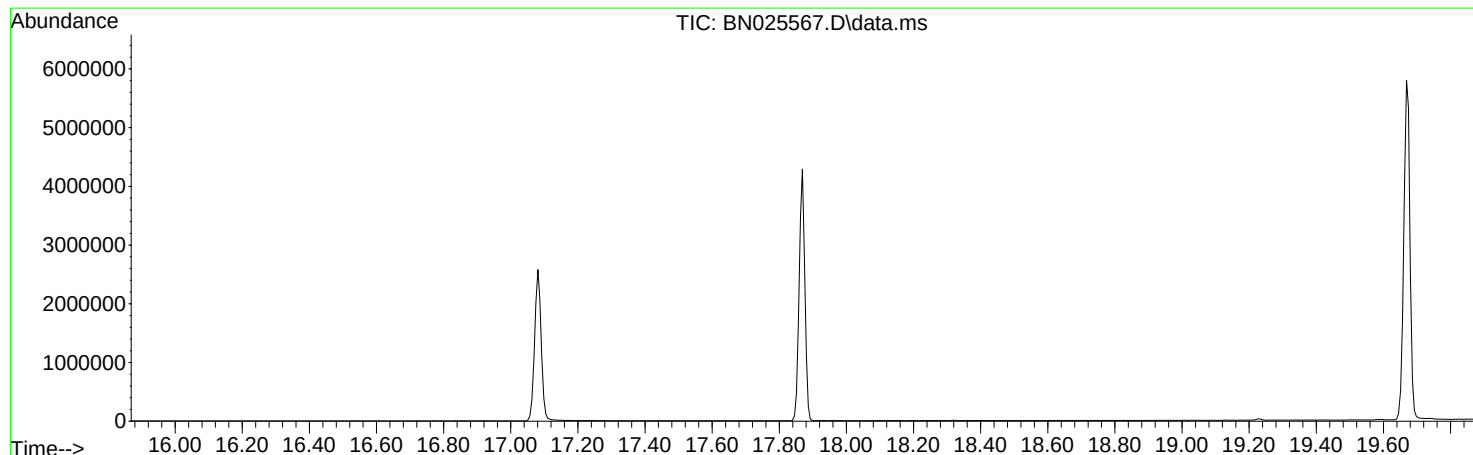

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	161933	PASS
68	69	0.00	2	1.6	2751	PASS
69	198	0.00	100	48.2	170760	PASS
70	69	0.00	2	0.5	857	PASS
127	198	10	80	52.4	185920	PASS
197	198	0.00	2	0.4	1568	PASS
198	198	100	100	100.0	354517	PASS
199	198	5	9	6.8	23968	PASS
275	198	10	60	24.9	88208	PASS
365	198	1	100	3.9	13888	PASS
441	198	0.01	100	13.5	47976	PASS
442	442	50	100	100.0	298987	PASS
443	442	15	24	20.2	60480	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/23/2023	BNA_N	<u>BN025567.D</u>
Compound Name	Response	Retention Time
DDT	1249497	20.904
DDD	16371	20.51
DDE	0	19.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16371	1265868	1.29

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052323\
 Data File : BN025567.D
 Acq On : 23 May 2023 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 24 07:02:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 07:02:20 2023
 Response via : Initial Calibration

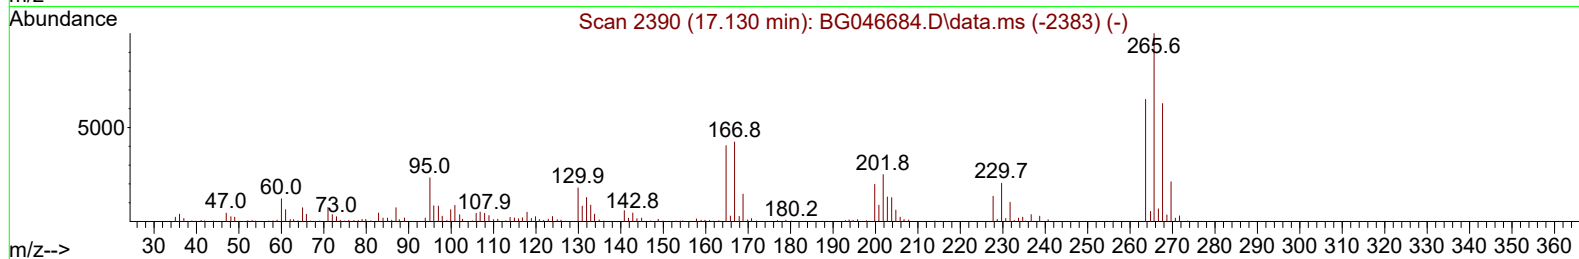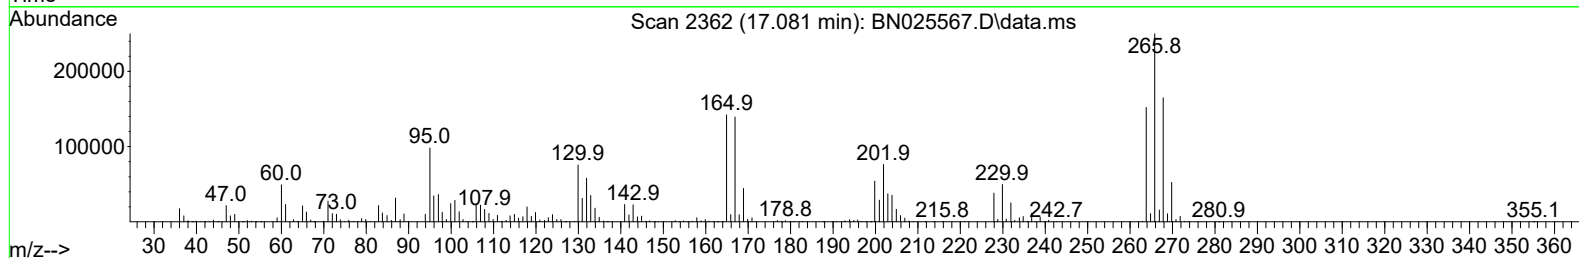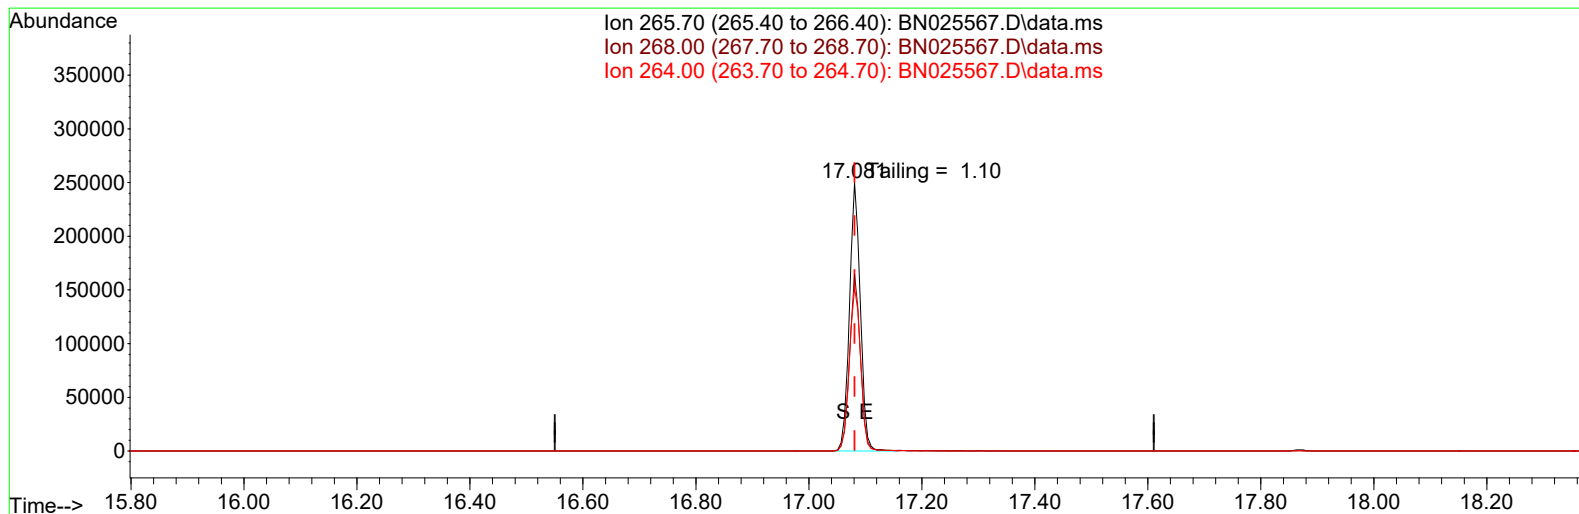

TIC: BN025567.D\data.ms

(70) Pentachlorophenol (C)

17.081min (0.000) 17650.24 ng




response 335898

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.94
264.00	61.60	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052323\
Data File : BN025567.D
Acq On : 23 May 2023 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 24 07:02:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 07:02:20 2023
Response via : Initial Calibration

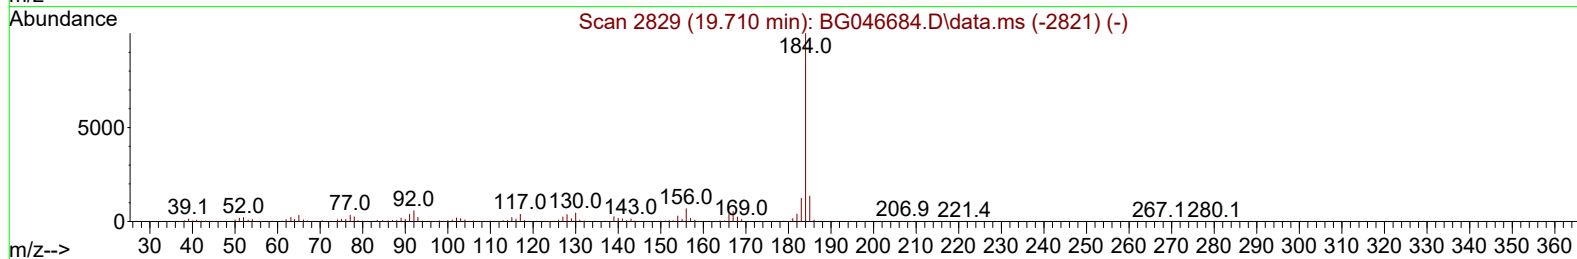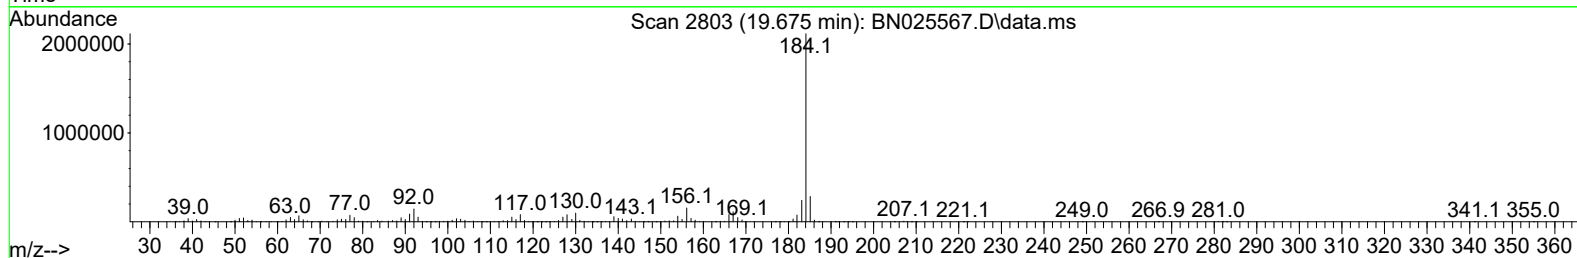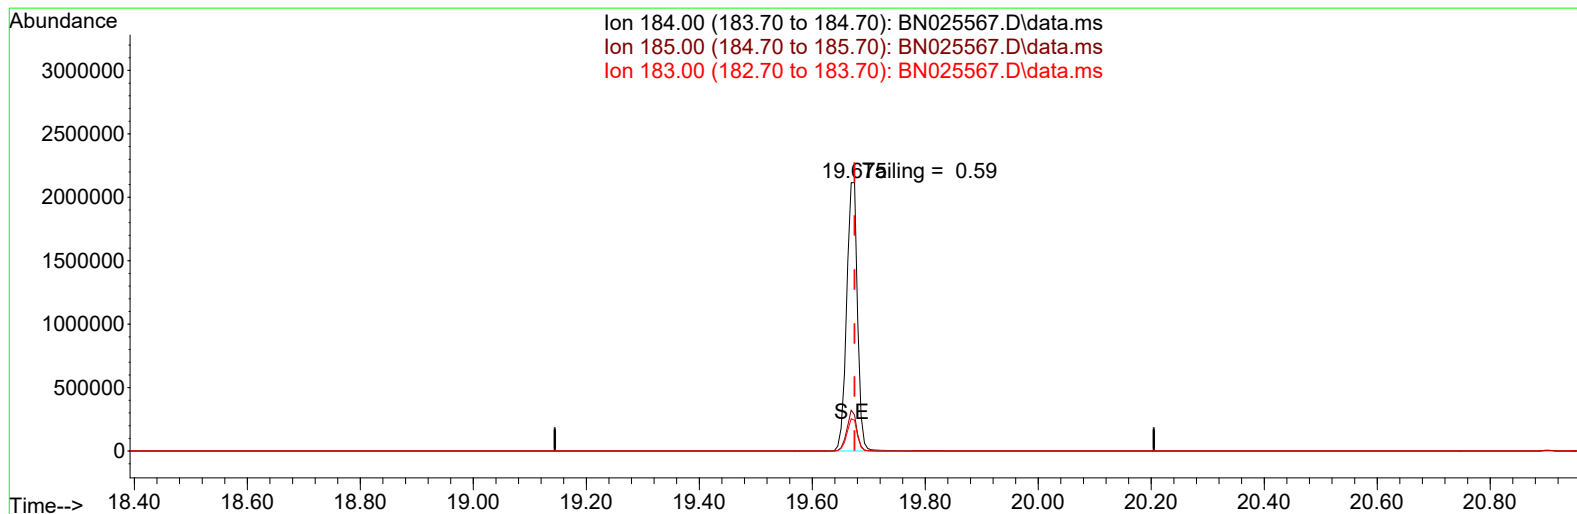

TIC: BN025567.D\data.ms

(77) Benzidine

19.675min (0.000) 0.00 ng

response 2830466

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.43
183.00	13.20	11.46
0.00	0.00	0.00