

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031631.D
 Acq On : 23 May 2024 14:12
 Operator : MA/JU
 Sample : P2547-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5P3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/24/2024
 Supervised By :mohammad ahmed 05/25/2024

Quant Time: May 23 23:08:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 21 23:42:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	455257	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	1979448	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.328	164	1232989	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.069	188	2329968	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1392204	20.000	ng/u1	0.00
88) Perylene-d12	24.233	264	1283595	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	40437	3.521	ng/uL	0.00
4) Pyridine-d5	3.599	84	537623	16.773	ng/u1	0.00
7) Phenol-d5	6.852	99	767388	20.477	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	475855	21.171	ng/u1	0.00
11) 2-Chlorophenol-d4	7.222	132	578375	20.029	ng/u1	0.00
15) 4-Methylphenol-d8	8.387	113	608837	20.986	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	284678	19.003	ng/u1	0.00
24) 2-Nitrophenol-d4	9.558	143	257932	18.030	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	540212	19.313	ng/u1	0.00
31) 4-Chloroaniline-d4	10.610	131	828333	20.544	ng/u1	0.00
46) Dimethylphthalate-d6	13.740	166	1753146	22.562	ng/u1	0.00
49) Acenaphthylene-d8	14.022	160	2039577	20.942	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	240312	16.345	ng/u1	0.00
60) Fluorene-d10	15.322	176	1501956	22.304	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	126144	12.522	ng/u1	0.00
73) Anthracene-d10	17.169	188	2180595	22.108	ng/u1	0.00
81) Pyrene-d10	19.463	212	2203738	25.236	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.039	264	1428812	23.648	ng/u1	0.00
Target Compounds					Qvalue	
72) Phenanthrene	17.110	178	264185	2.234	ng/u1	99
80) Fluoranthene	19.128	202	524976	4.864	ng/u1	97
82) Pyrene	19.492	202	484409	4.376	ng/u1	97
85) Benzo(a)anthracene	21.281	228	233041	2.489	ng/u1	98
87) Chrysene	21.345	228	205312	2.374	ng/u1	97
90) Benzo(b)fluoranthene	23.304	252	254694m	3.400	ng/u1	
91) Benzo(k)fluoranthene	23.363	252	105618	1.383	ng/u1	96
93) Benzo(a)pyrene	24.098	252	215421	2.994	ng/u1	97
94) Indeno(1,2,3-cd)pyrene	27.527	276	154704	1.791	ng/u1	98
96) Benzo(g,h,i)perylene	28.545	276	159165	2.231	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031631.D
Acq On : 23 May 2024 14:12
Operator : MA/JU
Sample : P2547-05
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH5P3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2024
Supervised By :mohammad ahmed 05/25/2024

Quant Time: May 23 23:08:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 21 23:42:49 2024
Response via : Initial Calibration

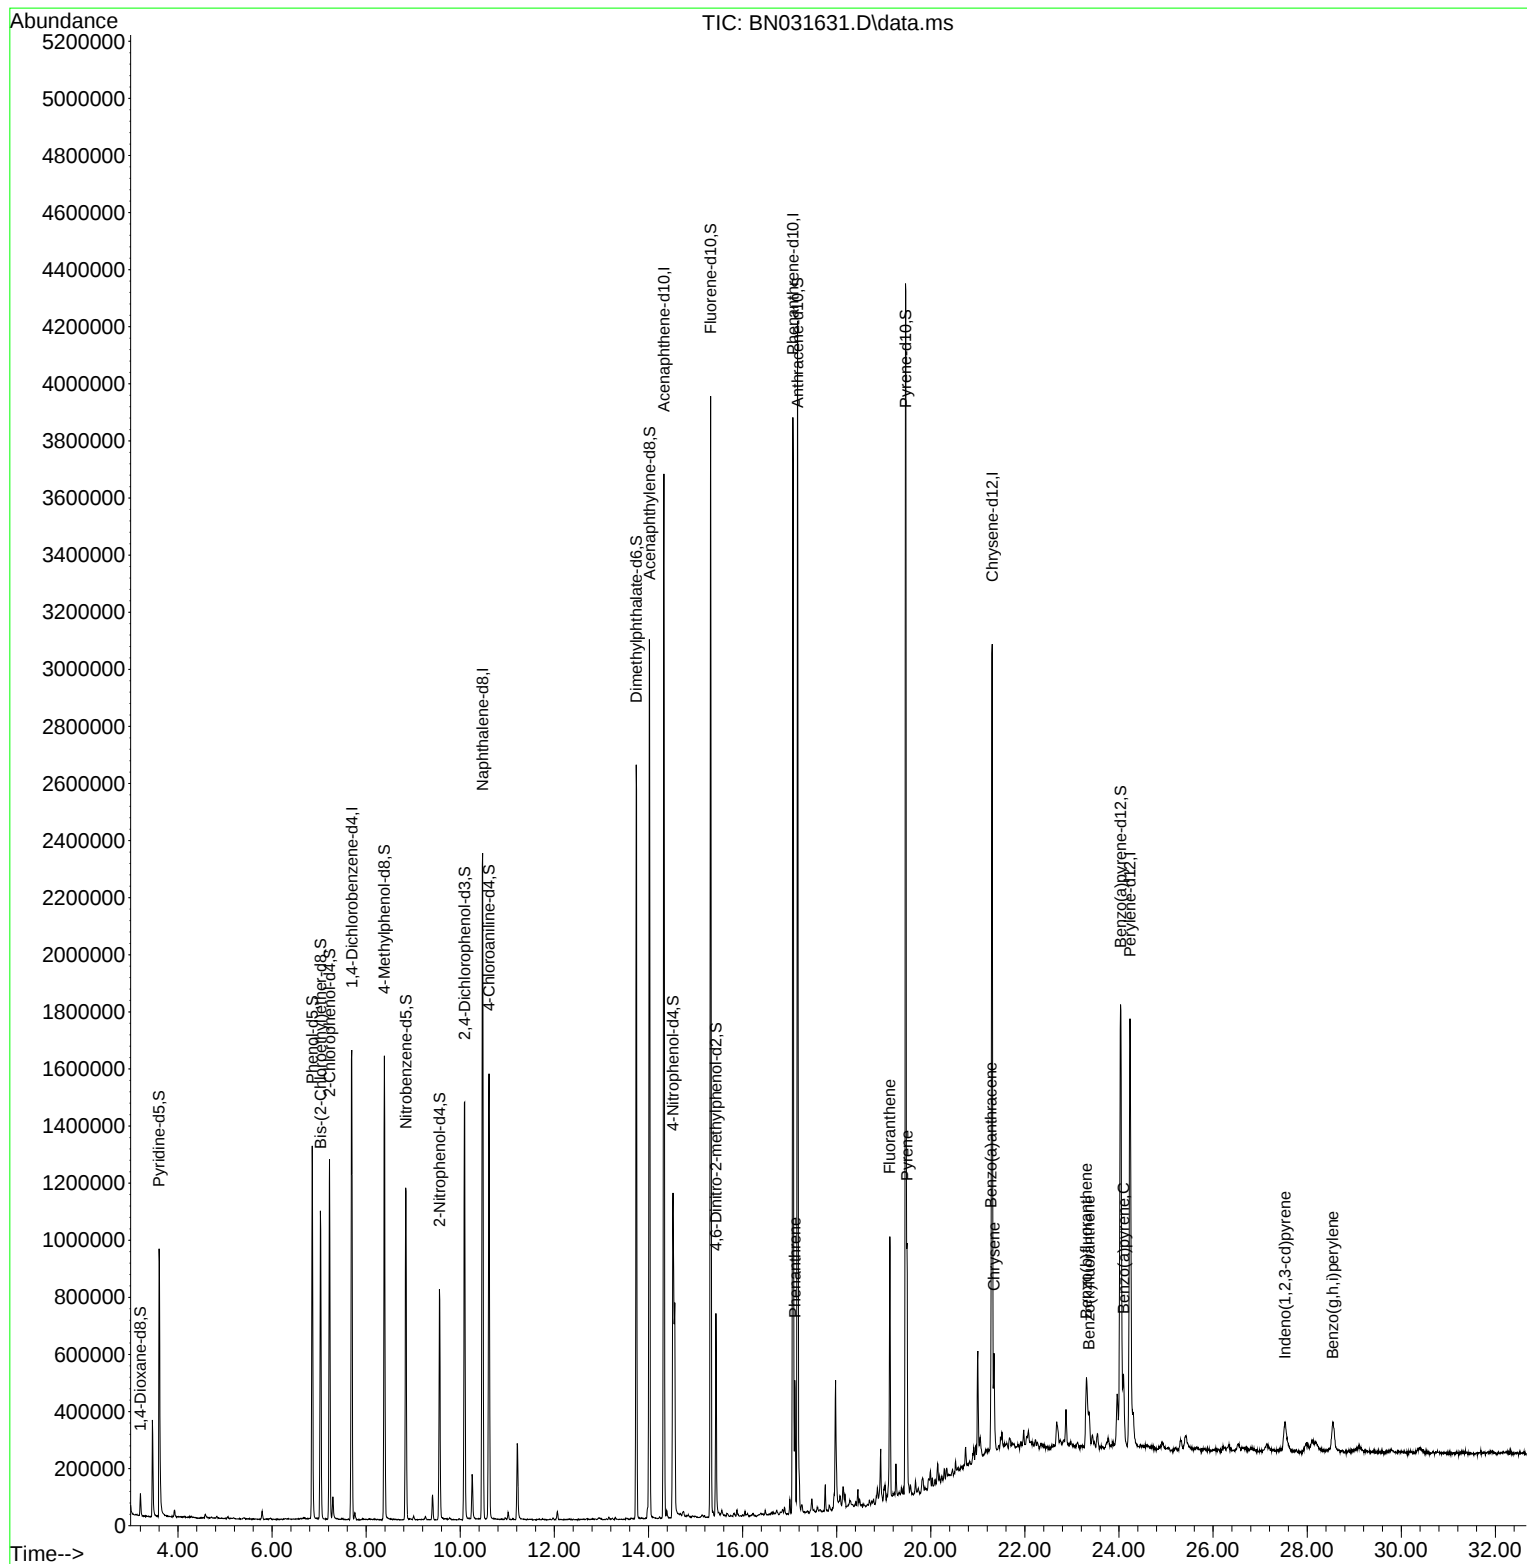

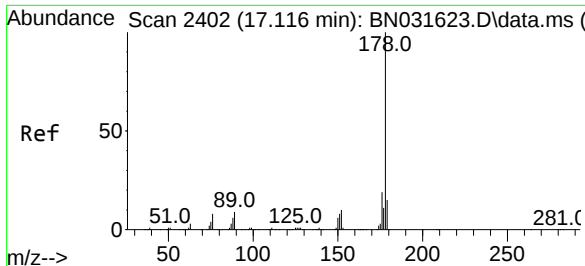





#72
Phenanthrene
Concen: 2.234 ng/ul
RT: 17.110 min Scan# 2402
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12

Instrument :
BNA_N
ClientSampleId :
BH5P3

Tgt Ion:178 Resp: 264185
Ion Ratio Lower Upper
178 100
179 15.6 12.6 18.8
176 19.9 15.2 22.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 05/24/2024
Supervised By :mohammad ahmed 05/25/2024

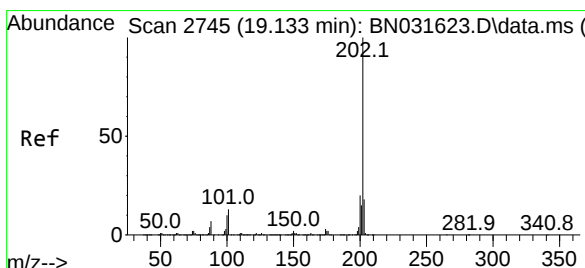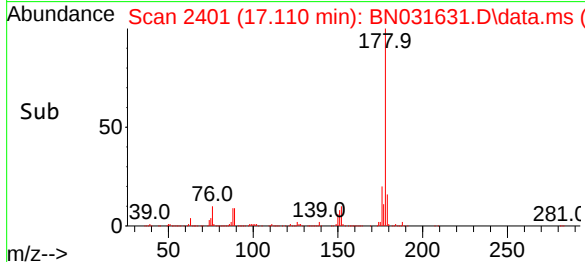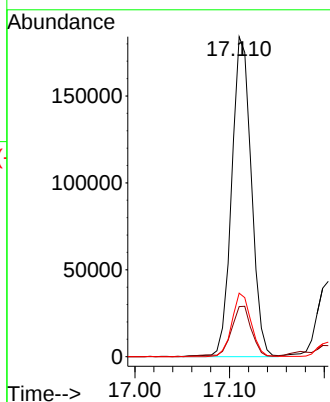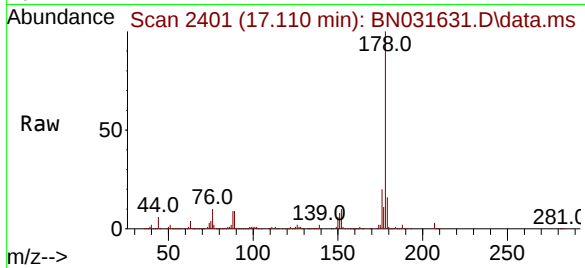

#80
Fluoranthene
Concen: 4.864 ng/ul
RT: 19.128 min Scan# 2744
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12


Tgt Ion:202 Resp: 524976
Ion Ratio Lower Upper
202 100
101 14.1 10.1 15.1
100 10.8 8.0 12.0

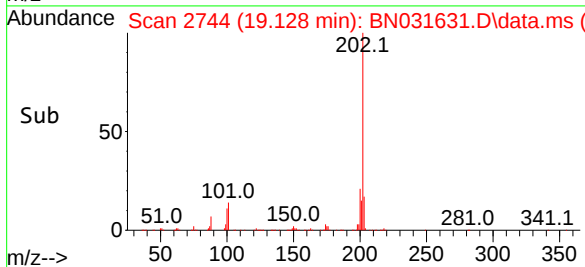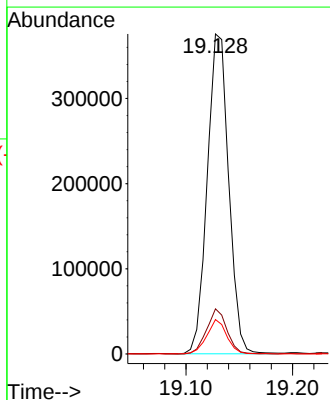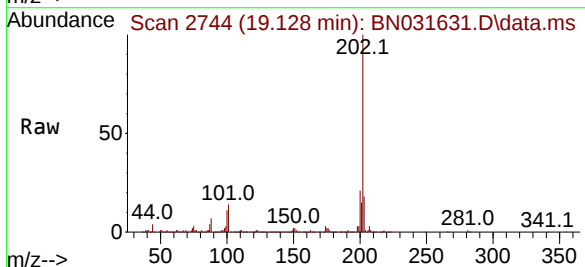

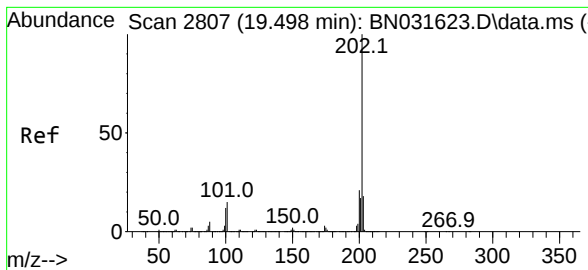

#82
Pyrene
Concen: 4.376 ng/ul
RT: 19.492 min Scan# 2110
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12




Instrument :
BNA_N
ClientSampleId :
BH5P3

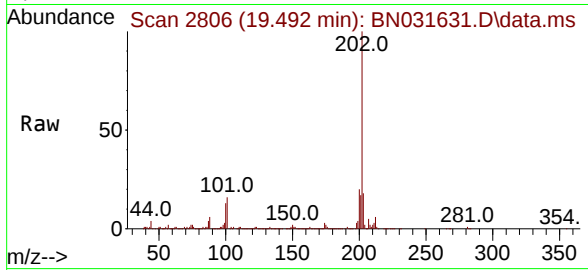


Tgt Ion:202 Resp: 484409
Ion Ratio Lower Upper
202 100
101 15.7 11.4 17.2
100 12.7 9.3 13.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 05/24/2024
Supervised By :mohammad ahmed 05/25/2024

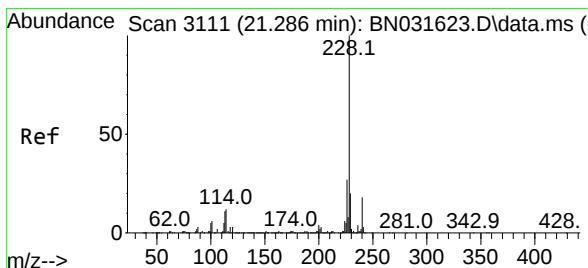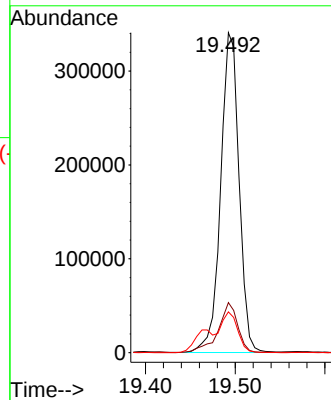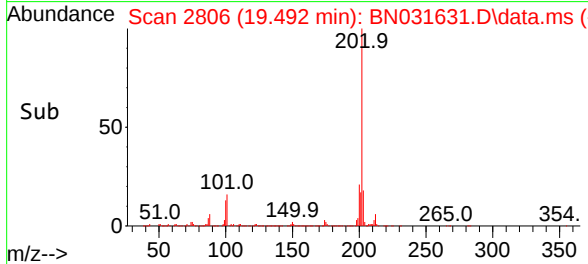


#85
Benzo(a)anthracene
Concen: 2.489 ng/ul
RT: 21.281 min Scan# 3110
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12

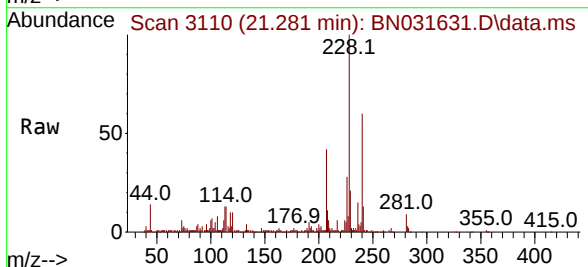

Tgt Ion:228 Resp: 233041
Ion Ratio Lower Upper
228 100
229 20.6 15.7 23.5
226 27.9 21.9 32.9

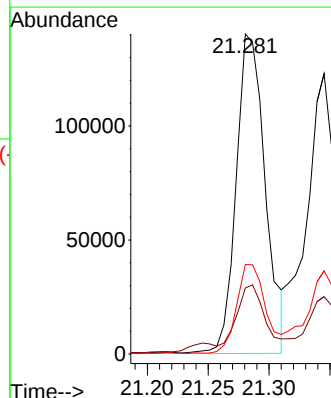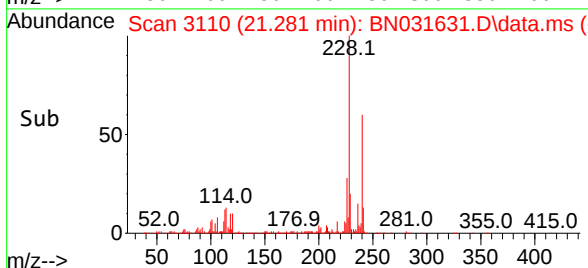

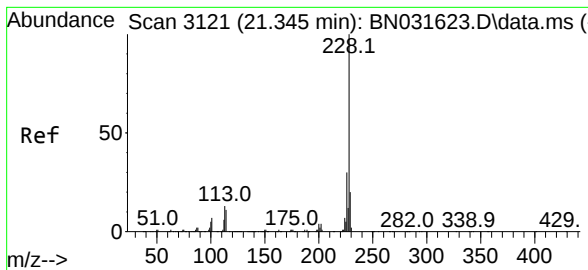

#87

Chrysene

Concen: 2.374 ng/ul

RT: 21.345 min Scan# 3121

Delta R.T. 0.000 min

Lab File: BN031631.D

Acq: 23 May 2024 14:12

Instrument :

BNA_N

ClientSampleId :

BH5P3





Tgt Ion:228	Resp: 205312
Ion Ratio	Lower Upper
228 100	
226 29.7	22.9 34.3
229 20.5	15.2 22.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/24/2024

Supervised By :mohammad ahmed 05/25/2024

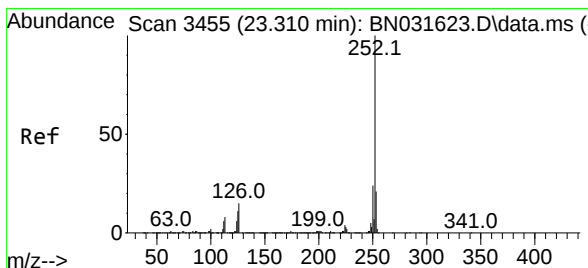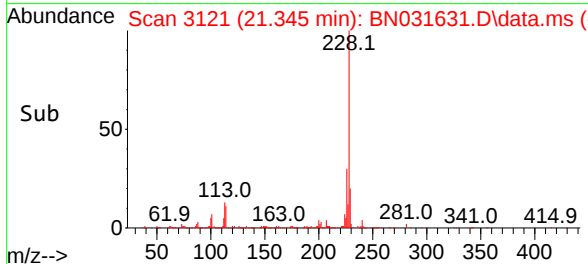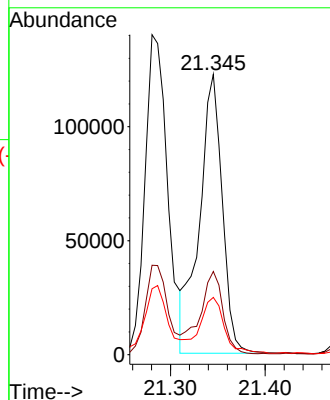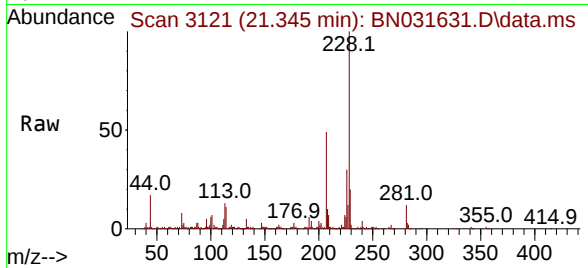

#90

Benzo(b)fluoranthene

Concen: 3.400 ng/ul m




RT: 23.304 min Scan# 3454


Delta R.T. -0.006 min

Lab File: BN031631.D

Acq: 23 May 2024 14:12


Tgt Ion:252	Resp: 254694
Ion Ratio	Lower Upper
252 100	
253 21.6	16.8 25.2
125 14.0	9.3 13.9

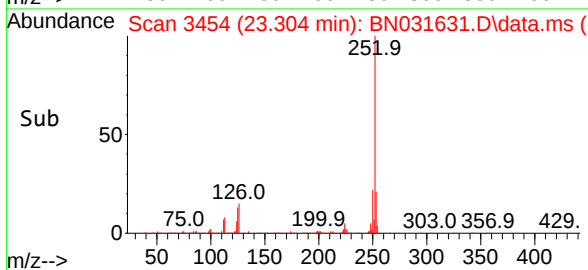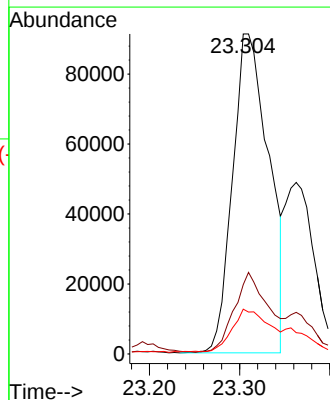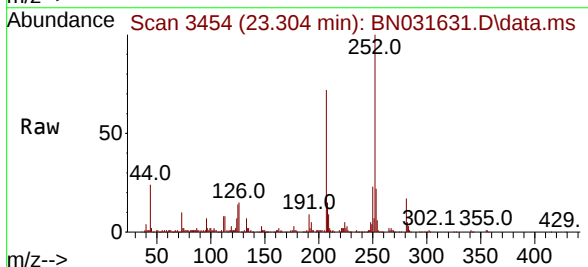

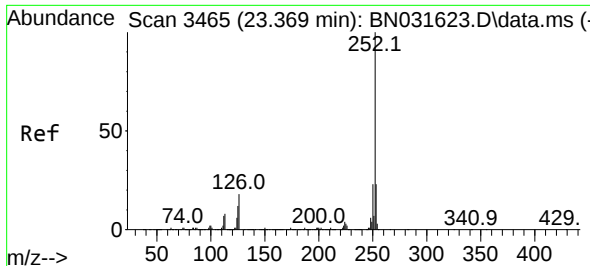

#91
Benzo(k)fluoranthene
Concen: 1.383 ng/ul
RT: 23.363 min Scan# 3465
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12




Instrument :
BNA_N
ClientSampleId :
BH5P3

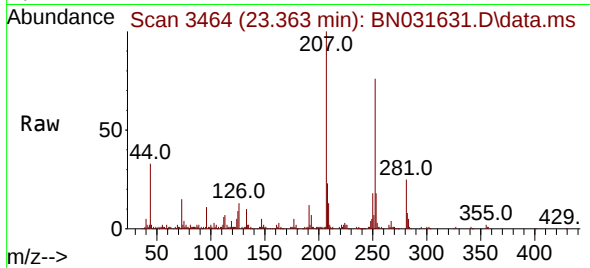

Tgt Ion:252 Resp: 105618
Ion Ratio Lower Upper
252 100
253 24.3 17.4 26.0
125 12.4 9.3 13.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 05/24/2024
Supervised By :mohammad ahmed 05/25/2024

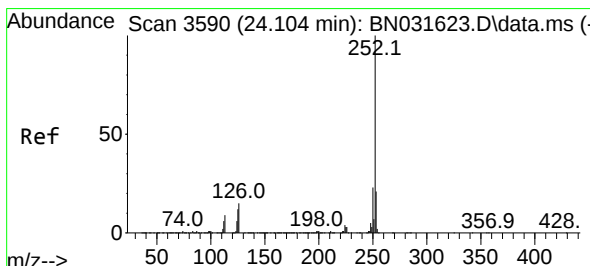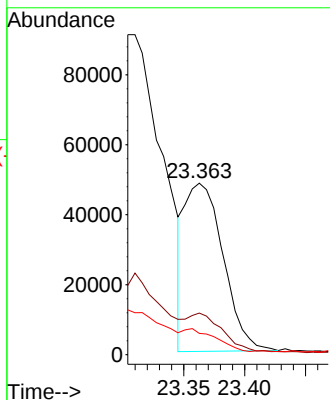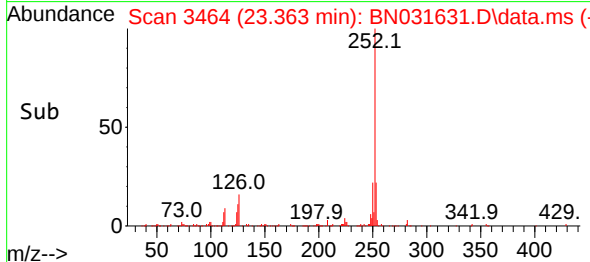

#93
Benzo(a)pyrene
Concen: 2.994 ng/ul
RT: 24.098 min Scan# 3589
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12


Tgt Ion:252 Resp: 215421
Ion Ratio Lower Upper
252 100
253 22.0 16.6 24.8
125 14.0 9.8 14.8

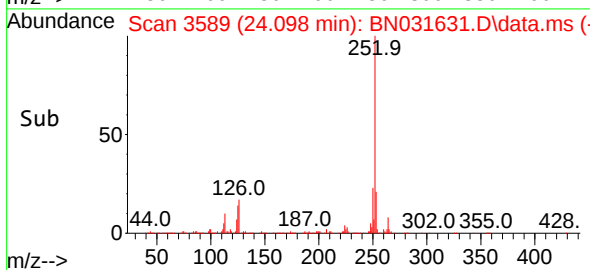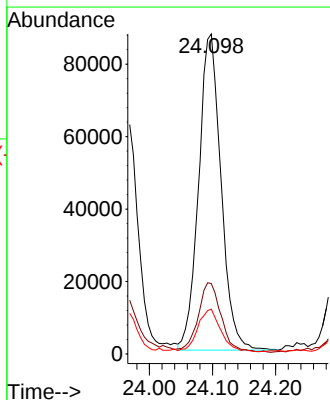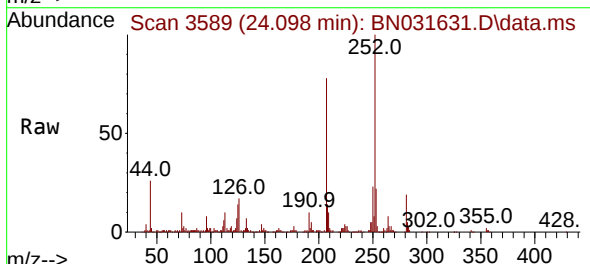

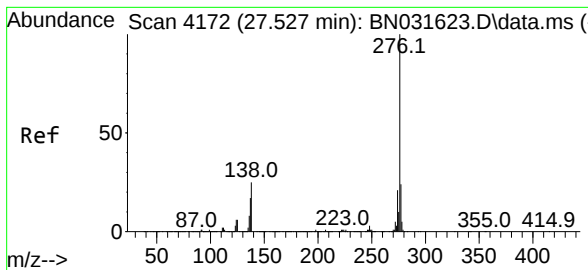

#94
Indeno(1,2,3-cd)pyrene
Concen: 1.791 ng/ul
RT: 27.527 min Scan# 4172
Delta R.T. -0.006 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12




Instrument :
BNA_N
ClientSampleId :
BH5P3

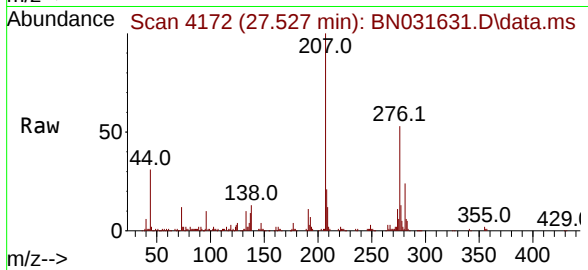


Tgt Ion:276 Resp: 154704
Ion Ratio Lower Upper
276 100
138 23.8 19.8 29.6
277 23.8 18.2 27.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2024
Supervised By :mohammad ahmed 05/25/2024

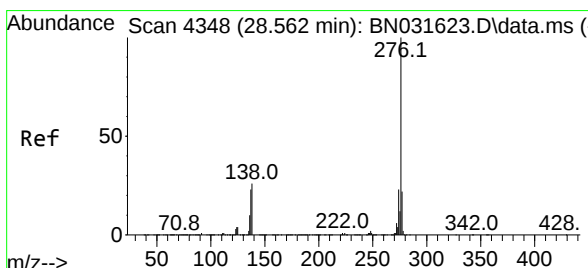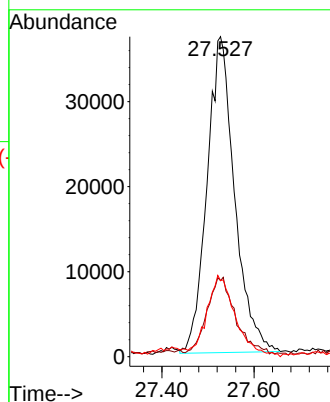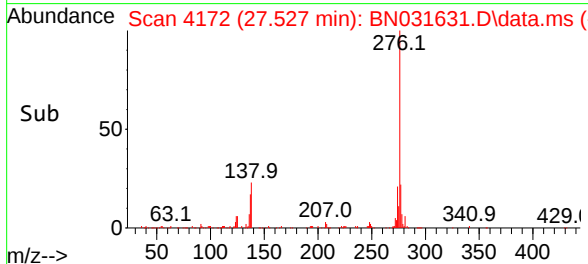

#96
Benzo(g,h,i)perylene
Concen: 2.231 ng/ul
RT: 28.545 min Scan# 4345
Delta R.T. -0.012 min
Lab File: BN031631.D
Acq: 23 May 2024 14:12

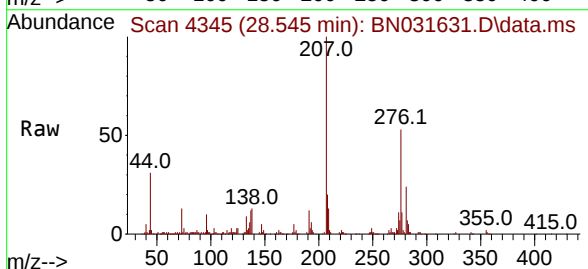

Tgt Ion:276 Resp: 159165
Ion Ratio Lower Upper
276 100
138 24.8 19.5 29.3
277 21.7 17.6 26.4

