

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031624.D
 Acq On : 23 May 2024 09:27
 Operator : MA/JU
 Sample : PB161002BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	45	rVB	133489	178069	1.90%	0.169%
2	3.599	101	104	122	rBV	1816797	2644607	28.16%	2.512%
3	3.922	155	159	166	rVB	30438	47262	0.50%	0.045%
4	6.852	650	657	672	rVB	1909330	3027462	32.23%	2.876%
5	7.028	681	687	701	rVB	1657147	2593880	27.62%	2.464%
6	7.222	712	720	728	rBV	1921796	3046677	32.44%	2.894%
7	7.687	791	799	808	rBV	1617994	2613455	27.83%	2.483%
8	8.387	910	918	933	rBV	2448719	3834557	40.83%	3.643%
9	8.840	988	995	1005	rBV	1783711	2975248	31.68%	2.826%
10	9.557	1109	1117	1130	rBV	1303847	2150666	22.90%	2.043%
11	10.087	1198	1207	1224	rBV	2204695	3698819	39.38%	3.514%
12	10.469	1264	1272	1280	rBV	2282692	3899684	41.52%	3.705%
13	10.610	1287	1296	1304	rBV	2463358	4133842	44.01%	3.927%
14	12.063	1538	1543	1551	rBV3	42303	72041	0.77%	0.068%
15	13.228	1736	1741	1747	rBV2	26161	42600	0.45%	0.040%
16	13.293	1749	1752	1757	rVB3	7197	9763	0.10%	0.009%
17	13.745	1822	1829	1837	rBV	4003599	5728958	61.00%	5.442%
18	14.022	1868	1876	1885	rBV	4579708	7076535	75.35%	6.723%
19	14.328	1921	1928	1937	rBV	3626132	5279267	56.21%	5.015%
20	14.522	1954	1961	1980	rBV	1903072	2781683	29.62%	2.643%
21	14.740	1995	1998	2002	rVB5	7592	9679	0.10%	0.009%
22	15.322	2090	2097	2110	rBV	5926964	8555941	91.10%	8.128%
23	15.434	2110	2116	2130	rBV	1328275	1875788	19.97%	1.782%
24	15.563	2133	2138	2142	rVB2	27440	43176	0.46%	0.041%
25	16.104	2226	2230	2235	rVB7	7717	11609	0.12%	0.011%
26	16.857	2354	2358	2366	rVB4	11066	17633	0.19%	0.017%
27	17.069	2388	2394	2402	rBV	4097985	5839574	62.18%	5.547%
28	17.169	2404	2411	2426	rVV2	6151595	8917573	94.95%	8.471%
29	17.969	2544	2547	2552	rBV6	8753	13358	0.14%	0.013%
30	19.028	2723	2727	2733	rBV3	68540	93302	0.99%	0.089%
31	19.098	2735	2739	2747	rVB	64105	90851	0.97%	0.086%
32	19.410	2790	2792	2795	rBV4	11779	11667	0.12%	0.011%
33	19.463	2795	2801	2816	rVV	6870416	9392154	100.00%	8.922%
34	21.298	3107	3113	3125	rBV	3222047	4623354	49.23%	4.392%
35	24.033	3569	3578	3593	rVB2	2568791	6054742	64.47%	5.752%
36	24.233	3604	3612	3629	rVB	1538009	3880813	41.32%	3.687%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031624.D
Acq On : 23 May 2024 09:27
Operator : MA/JU
Sample : PB161002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK002

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 105266289

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031624.D
Acq On : 23 May 2024 09:27
Operator : MA/JU
Sample : PB161002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

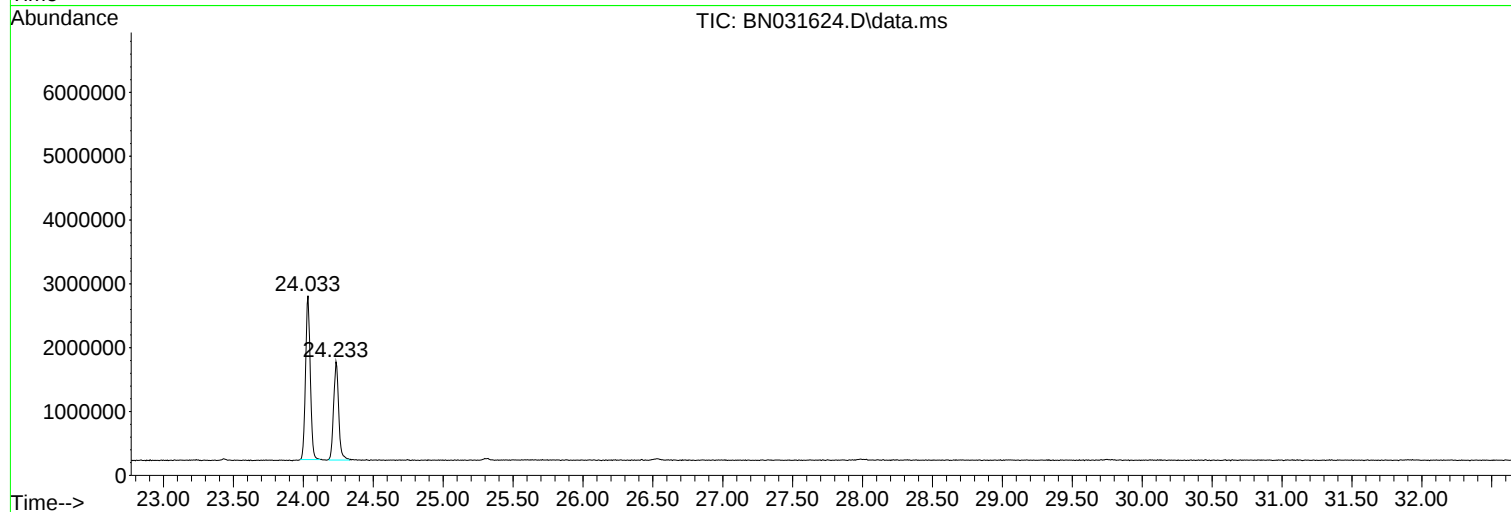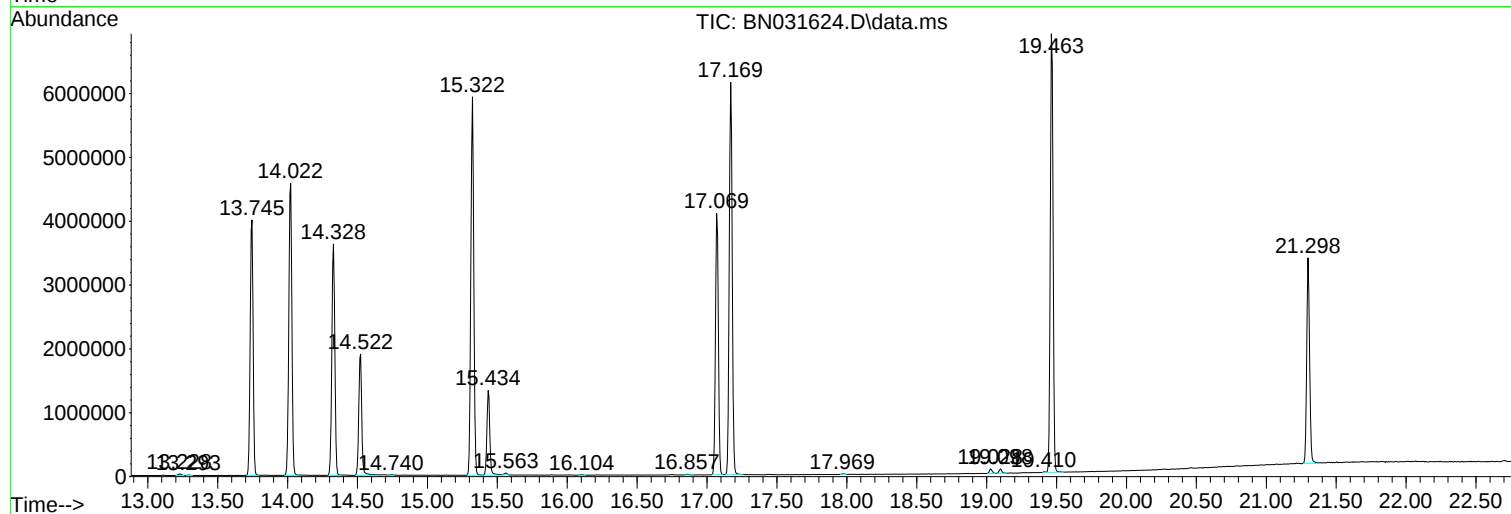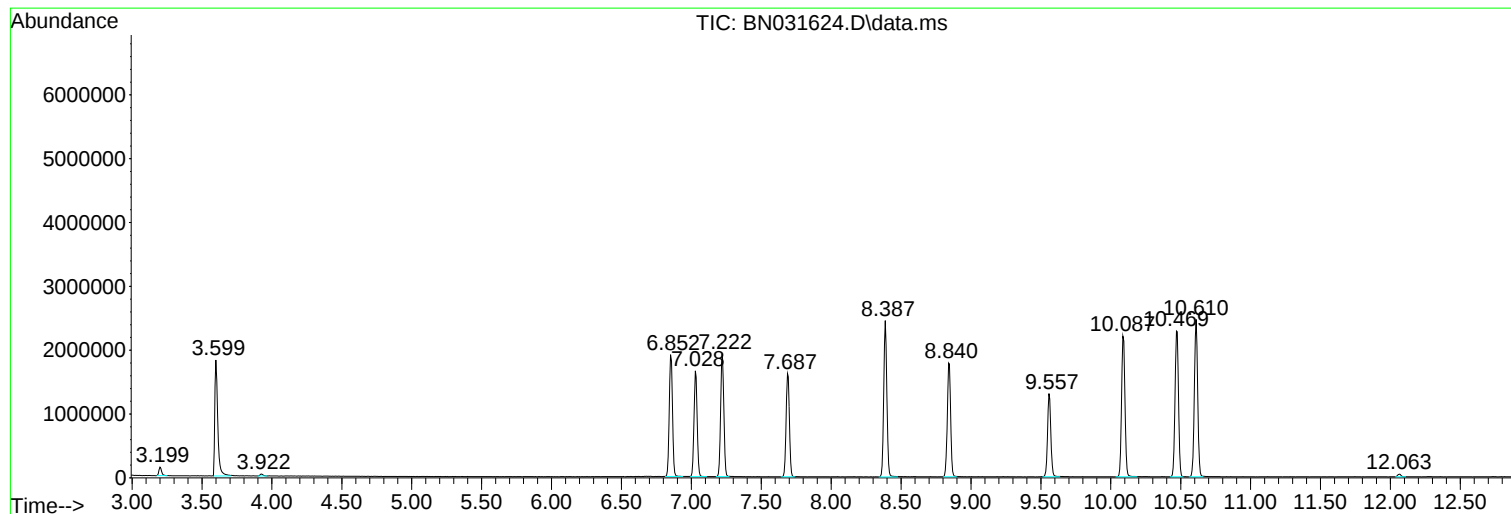

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031624.D
Acq On : 23 May 2024 09:27
Operator : MA/JU
Sample : PB161002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031624.D
Acq On : 23 May 2024 09:27
Operator : MA/JU
Sample : PB161002BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------