

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031632.D
 Acq On : 23 May 2024 14:57
 Operator : MA/JU
 Sample : P2547-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5Q3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rVB	70470	93877	1.57%	0.128%
2	3.458	76	80	88	rBV	187853	257219	4.30%	0.350%
3	3.599	102	104	118	rBV	643730	950351	15.89%	1.293%
4	3.922	155	159	164	rBV	27788	40872	0.68%	0.056%
5	4.134	192	195	200	rVB7	5491	8210	0.14%	0.011%
6	4.593	269	273	275	rBV5	4814	8321	0.14%	0.011%
7	4.822	308	312	318	rBV6	6103	12159	0.20%	0.017%
8	5.181	369	373	380	rBV7	3576	6585	0.11%	0.009%
9	5.787	469	476	482	rBV	27818	45568	0.76%	0.062%
10	6.852	650	657	666	rBV	1106198	1734218	28.99%	2.359%
11	7.028	680	687	695	rBV	966911	1495749	25.00%	2.035%
12	7.216	711	719	727	rBV	1061547	1725900	28.85%	2.348%
13	7.293	727	732	743	rVB	40814	77575	1.30%	0.106%
14	7.687	792	799	807	rBV	1825120	2913984	48.71%	3.964%
15	7.758	807	811	821	rVB2	27242	47676	0.80%	0.065%
16	8.387	911	918	927	rBV	1288236	2024867	33.85%	2.754%
17	8.840	988	995	1004	rBV	1025303	1668159	27.89%	2.269%
18	9.005	1020	1023	1028	rVB5	7438	12613	0.21%	0.017%
19	9.257	1061	1066	1071	rBV6	11428	20337	0.34%	0.028%
20	9.410	1086	1092	1103	rVB	116025	180870	3.02%	0.246%
21	9.557	1109	1117	1128	rBV	694477	1157600	19.35%	1.575%
22	9.775	1152	1154	1159	rVB5	4540	6686	0.11%	0.009%
23	9.981	1182	1189	1193	rBV8	4958	10477	0.18%	0.014%
24	10.087	1198	1207	1221	rBV	1275825	2119472	35.43%	2.883%
25	10.252	1229	1235	1247	rBV	119760	203597	3.40%	0.277%
26	10.469	1265	1272	1280	rBV	2554101	4336075	72.48%	5.898%
27	10.610	1286	1296	1308	rBV	1311600	2168990	36.26%	2.950%
28	10.899	1338	1345	1350	rVB2	9708	20203	0.34%	0.027%
29	10.957	1350	1355	1360	rVB8	6157	10256	0.17%	0.014%
30	11.016	1360	1365	1372	rBV3	32506	56937	0.95%	0.077%
31	11.210	1391	1398	1409	rBV	207123	380846	6.37%	0.518%
32	11.810	1496	1500	1504	rBV6	3302	6861	0.11%	0.009%
33	12.063	1536	1543	1547	rBV	27001	43045	0.72%	0.059%
34	12.134	1553	1555	1565	rVB10	4398	8447	0.14%	0.011%
35	13.157	1725	1729	1735	rVB7	8626	13774	0.23%	0.019%
36	13.293	1749	1752	1761	rVB7	7302	11980	0.20%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031632.D
 Acq On : 23 May 2024 14:57
 Operator : MA/JU
 Sample : P2547-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5Q3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

37	13.645	1808	1812	1818	rVB8	5004	7323	0.12%	0.010%
38	13.740	1822	1828	1841	rVB	2209886	3163938	52.89%	4.304%
39	14.016	1864	1875	1888	rBV	2631875	4129975	69.04%	5.618%
40	14.234	1909	1912	1917	rVB5	7379	9187	0.15%	0.012%
41	14.328	1921	1928	1936	rBV	3823043	5602070	93.64%	7.621%
42	14.516	1953	1960	1965	rBV	673174	1085093	18.14%	1.476%
43	14.692	1982	1990	1993	rVB10	6566	17262	0.29%	0.023%
44	14.740	1993	1998	2005	rBV9	10697	22802	0.38%	0.031%
45	14.845	2014	2016	2023	rVB6	5742	8896	0.15%	0.012%
46	15.134	2062	2065	2070	rVV3	8379	13700	0.23%	0.019%
47	15.187	2070	2074	2081	rVB8	8672	15779	0.26%	0.021%
48	15.322	2089	2097	2104	rBV	3400346	4885278	81.66%	6.645%
49	15.434	2110	2116	2126	rBV	490913	709372	11.86%	0.965%
50	15.557	2133	2137	2140	rBV4	11574	17652	0.30%	0.024%
51	15.816	2178	2181	2185	rBV6	5062	6170	0.10%	0.008%
52	15.881	2188	2192	2199	rVB7	12723	17803	0.30%	0.024%
53	16.057	2216	2222	2225	rBV7	15547	26407	0.44%	0.036%
54	16.104	2228	2230	2233	rVB4	6384	7305	0.12%	0.010%
55	16.216	2244	2249	2255	rBV7	6577	16630	0.28%	0.023%
56	16.481	2291	2294	2298	rBV5	6206	6868	0.11%	0.009%
57	16.851	2352	2357	2360	rVV4	14715	25324	0.42%	0.034%
58	16.886	2361	2363	2368	rVB2	7016	9638	0.16%	0.013%
59	17.004	2379	2383	2387	rVB6	27345	36576	0.61%	0.050%
60	17.069	2387	2394	2399	rBV	4158739	5982264	100.00%	8.138%
61	17.110	2399	2401	2405	rVV	155363	204583	3.42%	0.278%
62	17.169	2405	2411	2423	rVB	3559232	4794503	80.15%	6.522%
63	17.369	2441	2445	2450	rVB	19343	31953	0.53%	0.043%
64	17.469	2455	2462	2467	rBV5	15426	36108	0.60%	0.049%
65	17.757	2506	2511	2514	rBV2	34922	46859	0.78%	0.064%
66	17.857	2523	2528	2529	rBV5	5939	10213	0.17%	0.014%
67	17.975	2537	2548	2556	rBV2	217277	450792	7.54%	0.613%
68	18.045	2558	2560	2563	rVB2	12096	16033	0.27%	0.022%
69	18.133	2570	2575	2579	rBV4	44932	84697	1.42%	0.115%
70	18.175	2579	2582	2588	rVB2	30610	44429	0.74%	0.060%
71	18.281	2596	2600	2601	rBV4	11403	15500	0.26%	0.021%
72	18.451	2625	2629	2632	rBV2	21008	29414	0.49%	0.040%
73	18.486	2633	2635	2641	rVB3	19852	26765	0.45%	0.036%
74	18.745	2676	2679	2682	rBV3	12419	14926	0.25%	0.020%
75	18.863	2696	2699	2704	rVB2	38185	55996	0.94%	0.076%
76	18.922	2705	2709	2713	rVB5	21293	39000	0.65%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031632.D
 Acq On : 23 May 2024 14:57
 Operator : MA/JU
 Sample : P2547-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5Q3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

77	19.028	2720	2727	2732	rBV2	45391	82688	1.38%	0.112%
78	19.128	2735	2744	2749	rBV	331883	520818	8.71%	0.708%
79	19.257	2763	2766	2774	rVB5	63546	85363	1.43%	0.116%
80	19.463	2795	2801	2816	rBV	3412160	5293963	88.49%	7.201%
81	19.992	2888	2891	2894	rVB2	41256	47359	0.79%	0.064%
82	20.027	2895	2897	2900	rVV2	30241	29241	0.49%	0.040%
83	20.145	2915	2917	2922	rVB3	34959	45282	0.76%	0.062%
84	20.527	2979	2982	2985	rBV	35065	38757	0.65%	0.053%
85	20.992	3058	3061	3068	rBV4	157490	272213	4.55%	0.370%
86	21.298	3107	3113	3119	rBV	2700546	4333762	72.44%	5.895%
87	24.033	3570	3578	3594	rVB2	1280877	3280254	54.83%	4.462%
88	24.233	3604	3612	3628	rVB	1550279	3877656	64.82%	5.275%




Sum of corrected areas: 73512795

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031632.D
Acq On : 23 May 2024 14:57
Operator : MA/JU
Sample : P2547-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

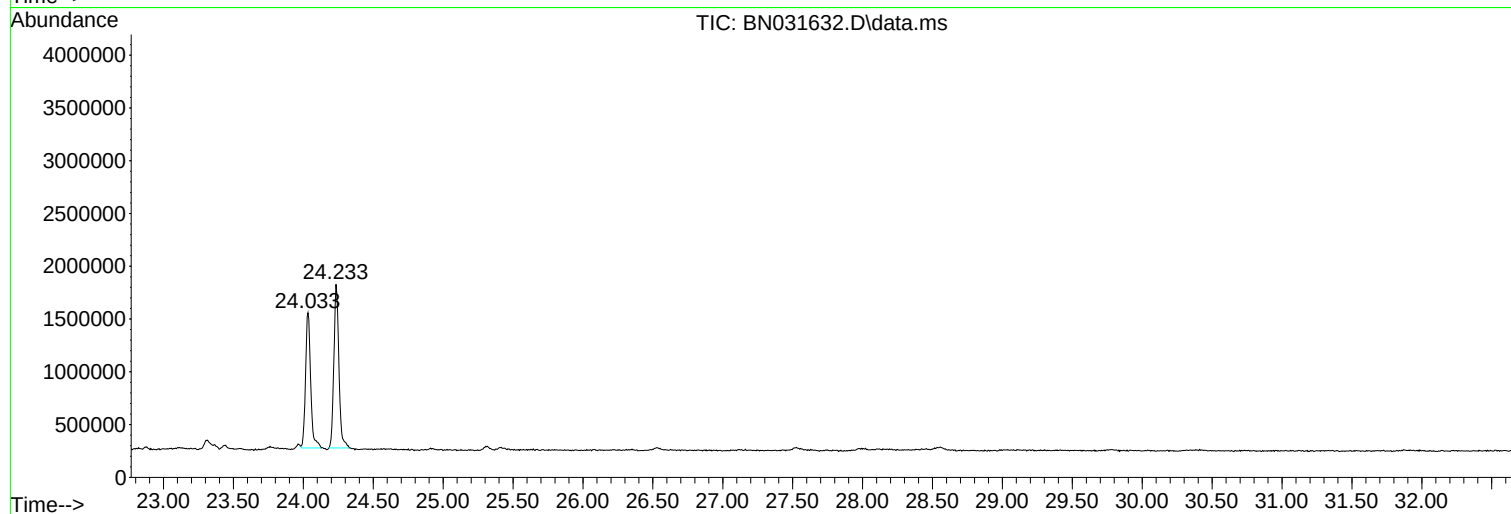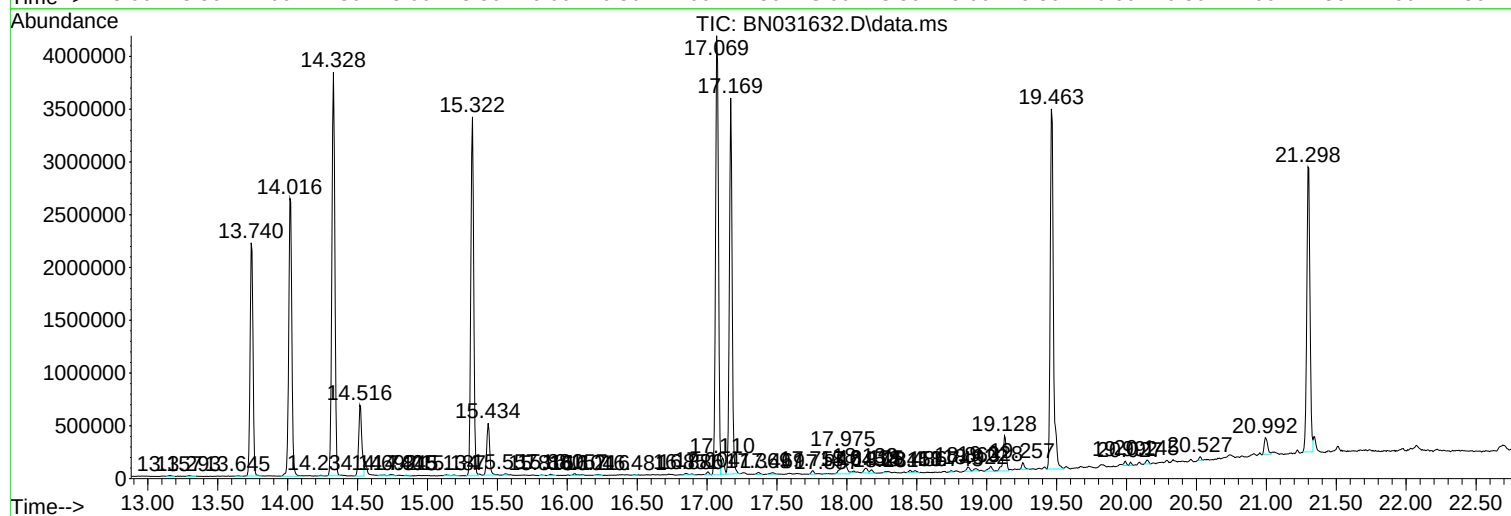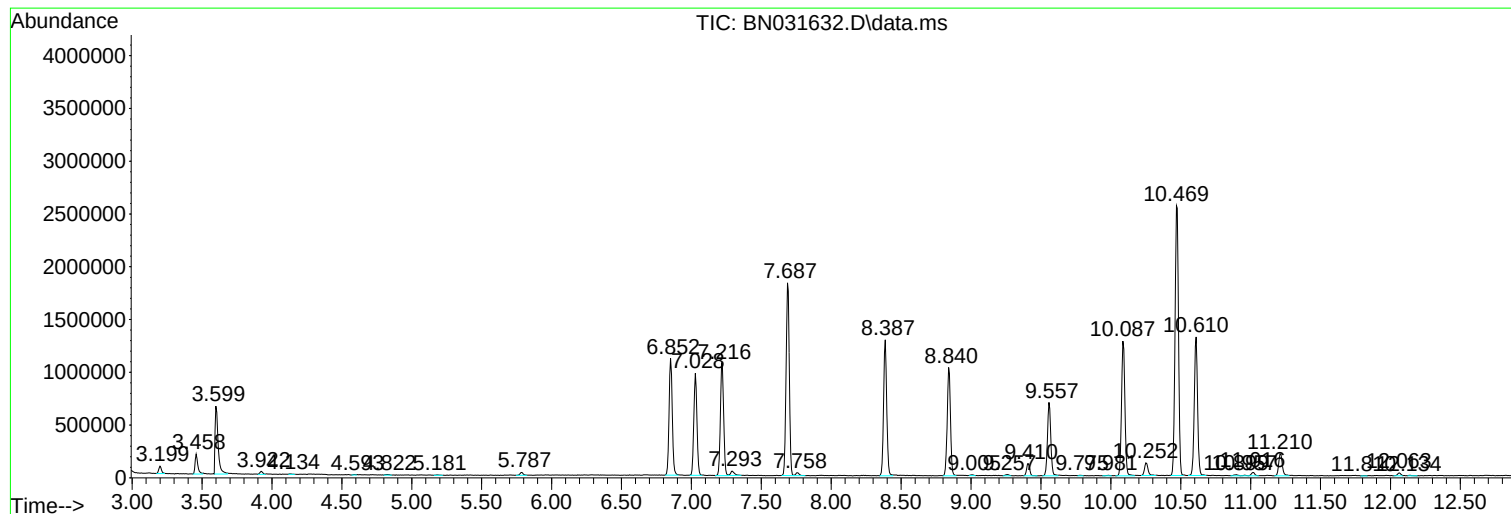

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031632.D
Acq On : 23 May 2024 14:57
Operator : MA/JU
Sample : P2547-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031632.D
Acq On : 23 May 2024 14:57
Operator : MA/JU
Sample : P2547-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc