

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
 Data File : BN031634.D
 Acq On : 23 May 2024 16:16
 Operator : MA/JU
 Sample : PB161044BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	32	37	45	rVB	127289	172361	2.49%	0.197%
2	3.599	101	104	125	rBV	1699072	2451799	35.39%	2.801%
3	3.928	155	160	164	rBV	36501	49049	0.71%	0.056%
4	6.681	622	628	629	rBV5	5662	7508	0.11%	0.009%
5	6.857	650	658	670	rBV	1786631	2877790	41.54%	3.287%
6	7.034	680	688	696	rVB	1540633	2442363	35.25%	2.790%
7	7.222	712	720	731	rBV	1843088	2897454	41.82%	3.310%
8	7.693	791	800	808	rBV	1526322	2449589	35.36%	2.798%
9	8.110	866	871	877	rVB7	5478	12374	0.18%	0.014%
10	8.387	911	918	928	rBV	2219939	3528730	50.94%	4.031%
11	8.846	988	996	1003	rBV	1660101	2726715	39.36%	3.115%
12	9.563	1109	1118	1130	rBV	1161057	1952121	28.18%	2.230%
13	10.093	1200	1208	1223	rBV	2035024	3369942	48.64%	3.849%
14	10.475	1264	1273	1281	rBV	2073016	3568084	51.50%	4.076%
15	10.610	1288	1296	1305	rBV	2243341	3688877	53.25%	4.214%
16	11.751	1484	1490	1496	rVB7	3534	9225	0.13%	0.011%
17	12.063	1537	1543	1550	rBV2	39368	70090	1.01%	0.080%
18	13.292	1748	1752	1755	rBV5	5795	9797	0.14%	0.011%
19	13.739	1821	1828	1841	rBV	3269110	4686382	67.65%	5.353%
20	14.022	1868	1876	1886	rBV	4060724	5982412	86.35%	6.833%
21	14.328	1920	1928	1940	rBV	3011158	4468604	64.50%	5.104%
22	14.416	1940	1943	1948	rVB7	5639	7052	0.10%	0.008%
23	14.522	1953	1961	1971	rBV	1333912	1993458	28.77%	2.277%
24	14.686	1987	1989	1994	rVB5	6830	8398	0.12%	0.010%
25	14.751	1994	2000	2004	rBV9	8104	13414	0.19%	0.015%
26	15.322	2090	2097	2110	rBV	4987701	6927764	100.00%	7.913%
27	15.434	2110	2116	2132	rVV	847648	1235135	17.83%	1.411%
28	15.557	2133	2137	2144	rVB2	24304	39348	0.57%	0.045%
29	15.886	2188	2193	2198	rBV7	6670	13899	0.20%	0.016%
30	16.004	2209	2213	2216	rBV6	4729	7211	0.10%	0.008%
31	16.104	2228	2230	2236	rVB5	8179	11486	0.17%	0.013%
32	16.857	2354	2358	2359	rBV3	7479	8022	0.12%	0.009%
33	17.069	2388	2394	2404	rBV	3020098	4386814	63.32%	5.011%
34	17.169	2404	2411	2426	rVV2	4670356	6593594	95.18%	7.532%
35	17.451	2453	2459	2462	rBV4	7937	15134	0.22%	0.017%
36	17.498	2463	2467	2473	rVB8	4814	8793	0.13%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031634.D
Acq On : 23 May 2024 16:16
Operator : MA/JU
Sample : PB161044BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Title : SVOA CALIBRATION

37	17.969	2544	2547	2553	rBV5	15246	24680	0.36%	0.028%
38	18.298	2600	2603	2607	rBV6	6057	11397	0.16%	0.013%
39	19.027	2723	2727	2733	rBV	47850	68794	0.99%	0.079%
40	19.098	2735	2739	2746	rVB	43896	62087	0.90%	0.071%
41	19.410	2790	2792	2795	rVB4	10358	10847	0.16%	0.012%
42	19.463	2795	2801	2816	rBV	4834289	6290959	90.81%	7.186%
43	21.298	3108	3113	3127	rVB2	2191780	3283085	47.39%	3.750%
44	24.033	3569	3578	3592	rVB	2271645	5526470	79.77%	6.313%
45	24.233	3603	3612	3628	rVB	1438997	3577605	51.64%	4.087%




Sum of corrected areas: 87546712

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031634.D
Acq On : 23 May 2024 16:16
Operator : MA/JU
Sample : PB161044BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

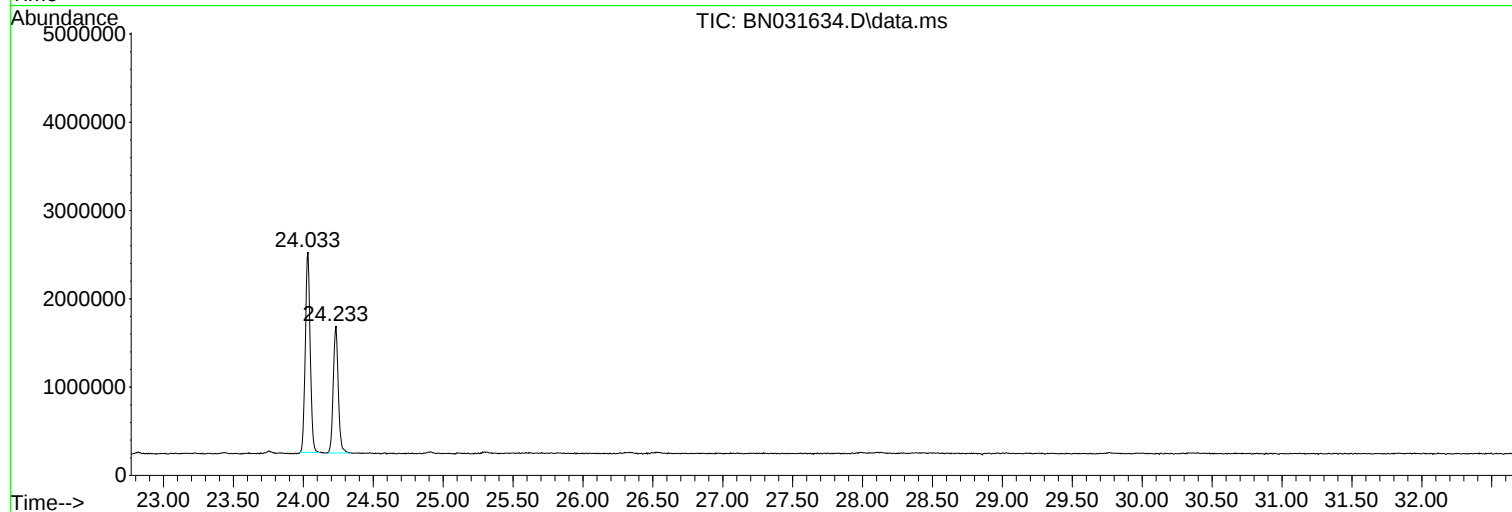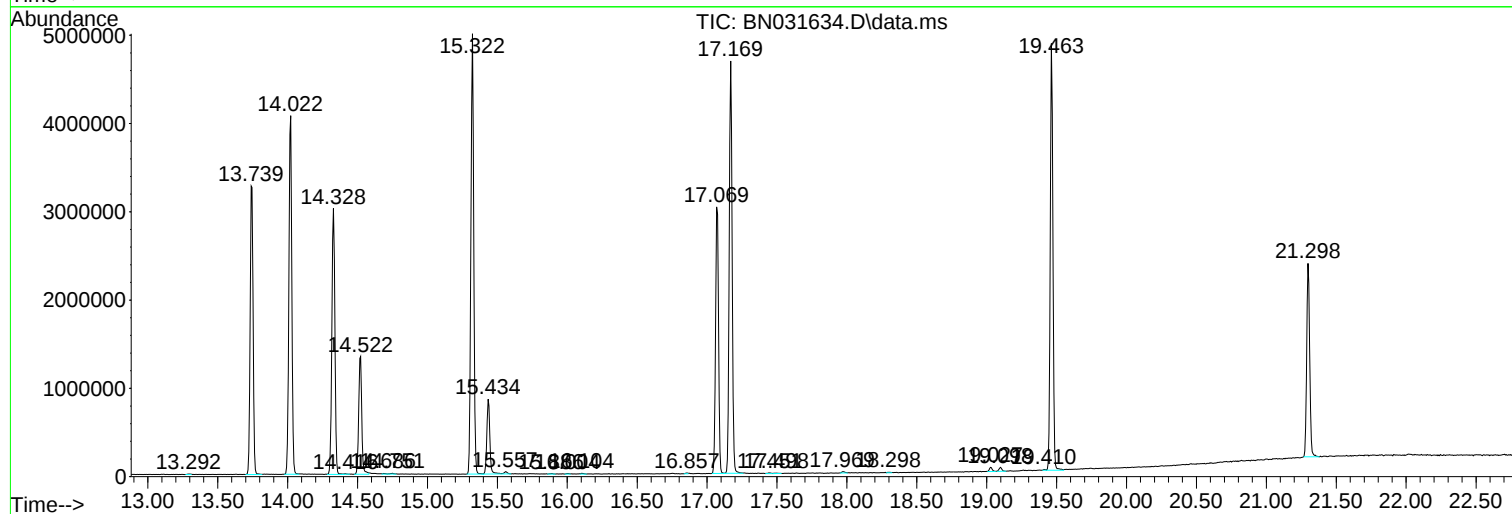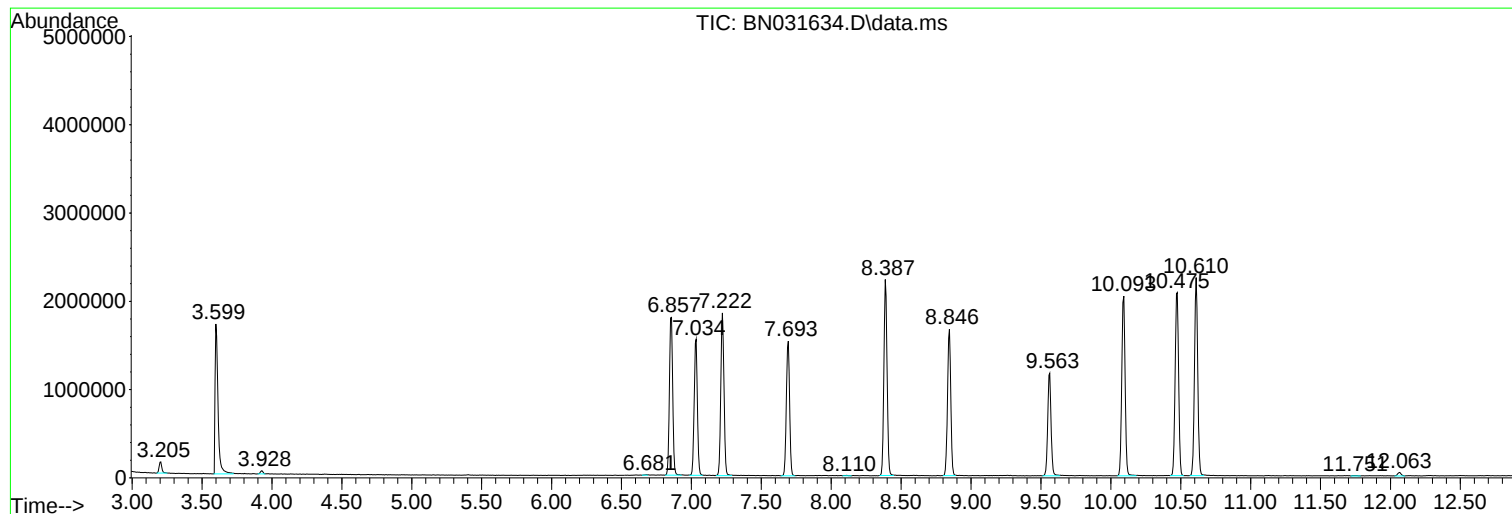

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031634.D
Acq On : 23 May 2024 16:16
Operator : MA/JU
Sample : PB161044BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052324\
Data File : BN031634.D
Acq On : 23 May 2024 16:16
Operator : MA/JU
Sample : PB161044BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK044

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------