
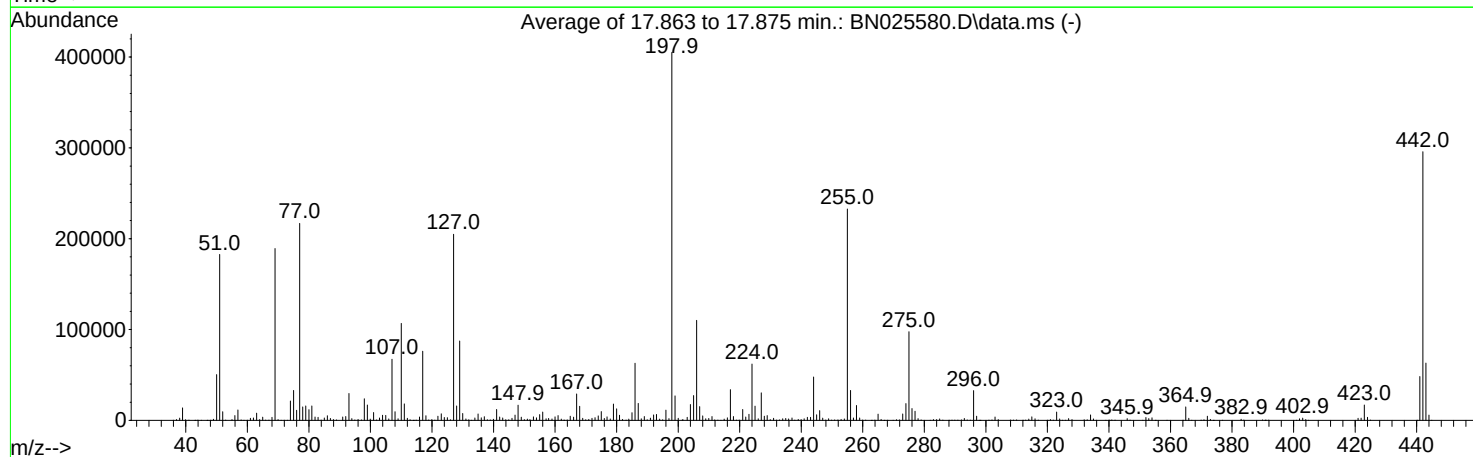


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052423\
Data File : BN025580.D
Acq On : 24 May 2023 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 23 03:22:57 2023

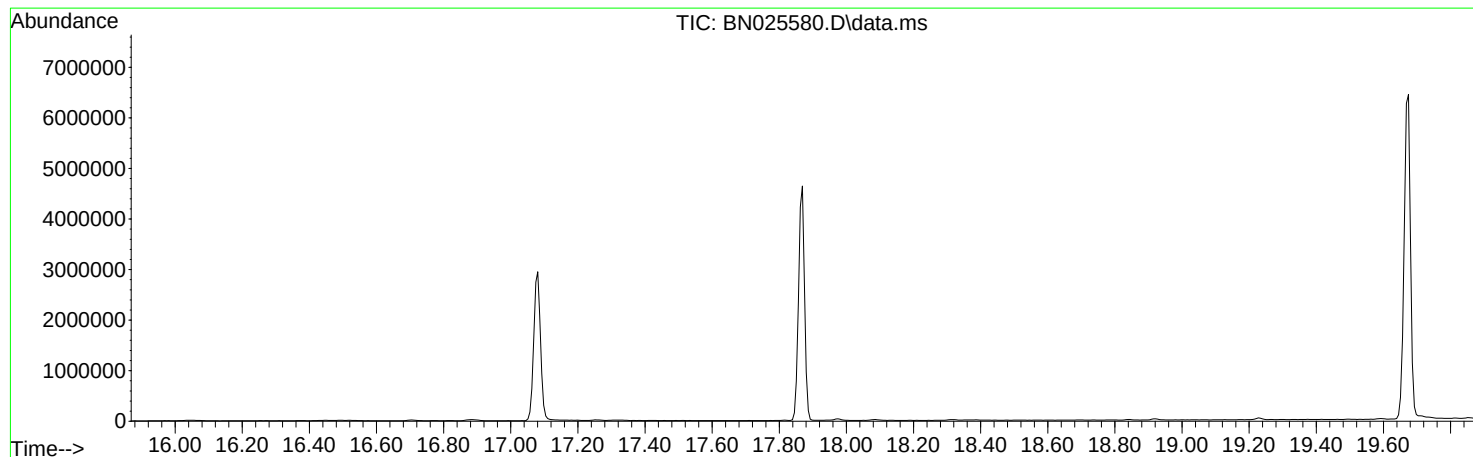

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	182667	PASS
68	69	0.00	2	1.8	3333	PASS
69	198	0.00	100	46.7	189149	PASS
70	69	0.00	2	0.5	931	PASS
127	198	10	80	50.6	204971	PASS
197	198	0.00	2	0.5	1935	PASS
198	198	100	100	100.0	405013	PASS
199	198	5	9	6.7	26952	PASS
275	198	10	60	24.1	97557	PASS
365	198	1	100	3.7	14808	PASS
441	198	0.01	100	11.9	48235	PASS
442	442	50	100	100.0	295744	PASS
443	442	15	24	21.3	63005	PASS