
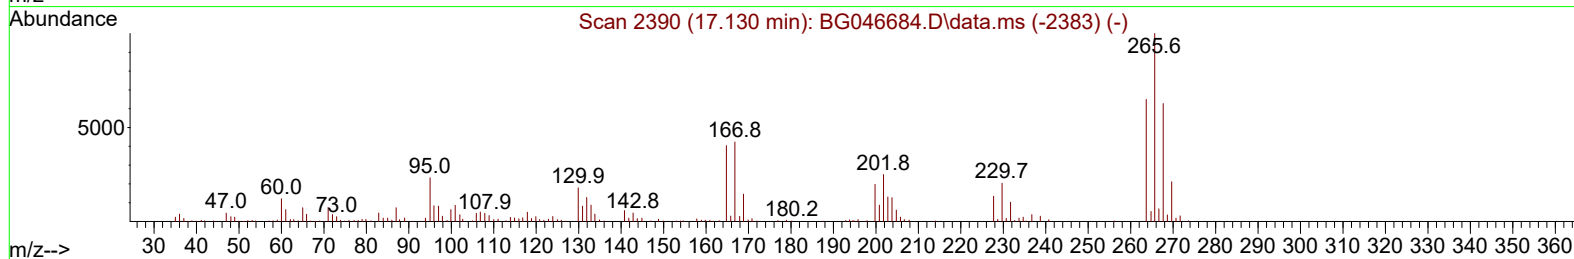
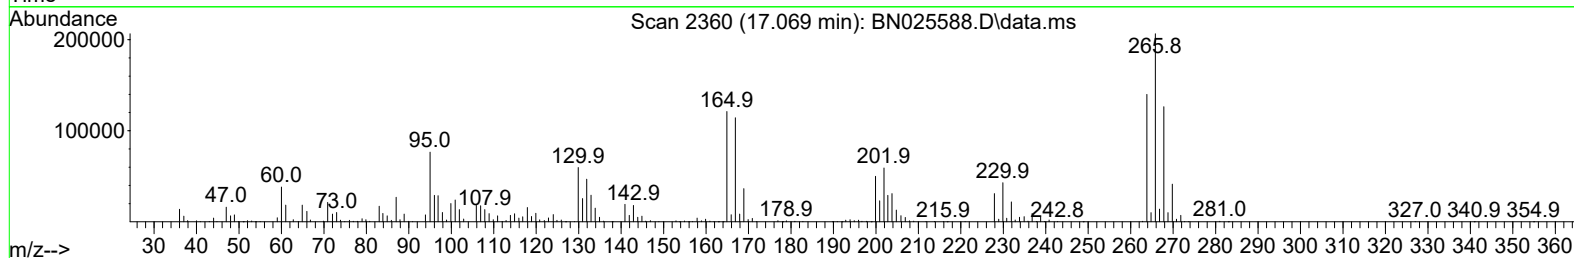


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052523\  
Data File : BN025588.D  
Acq On : 25 May 2023 14:36  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 06:42:47 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 26 06:42:42 2023  
Response via : Initial Calibration

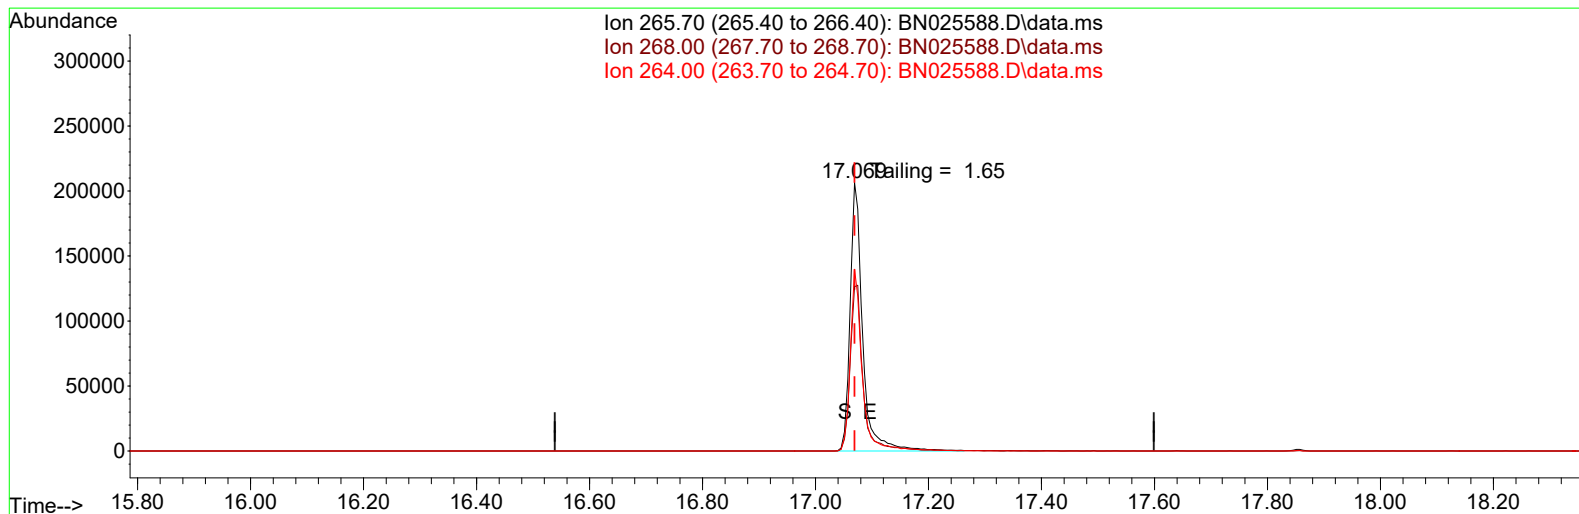

TIC: BN025588.D\data.ms

**(70) Pentachlorophenol (C)**




17.069min ( 0.000) 13726.37 ng

response 321332

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.24  |
| 264.00 | 61.60  | 67.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052523\  
Data File : BN025588.D  
Acq On : 25 May 2023 14:36  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 06:42:47 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 26 06:42:42 2023  
Response via : Initial Calibration

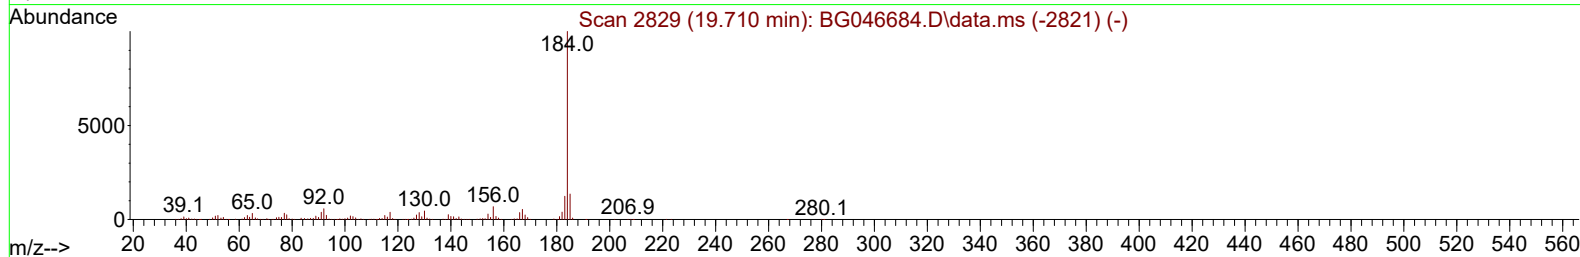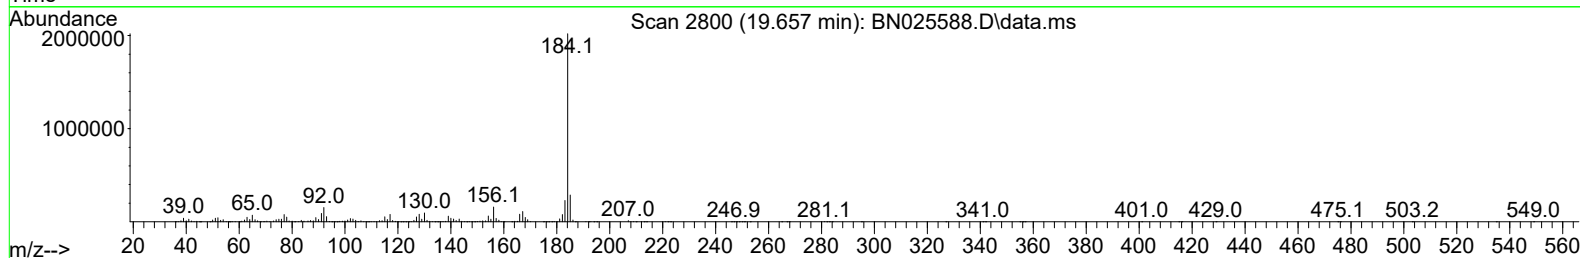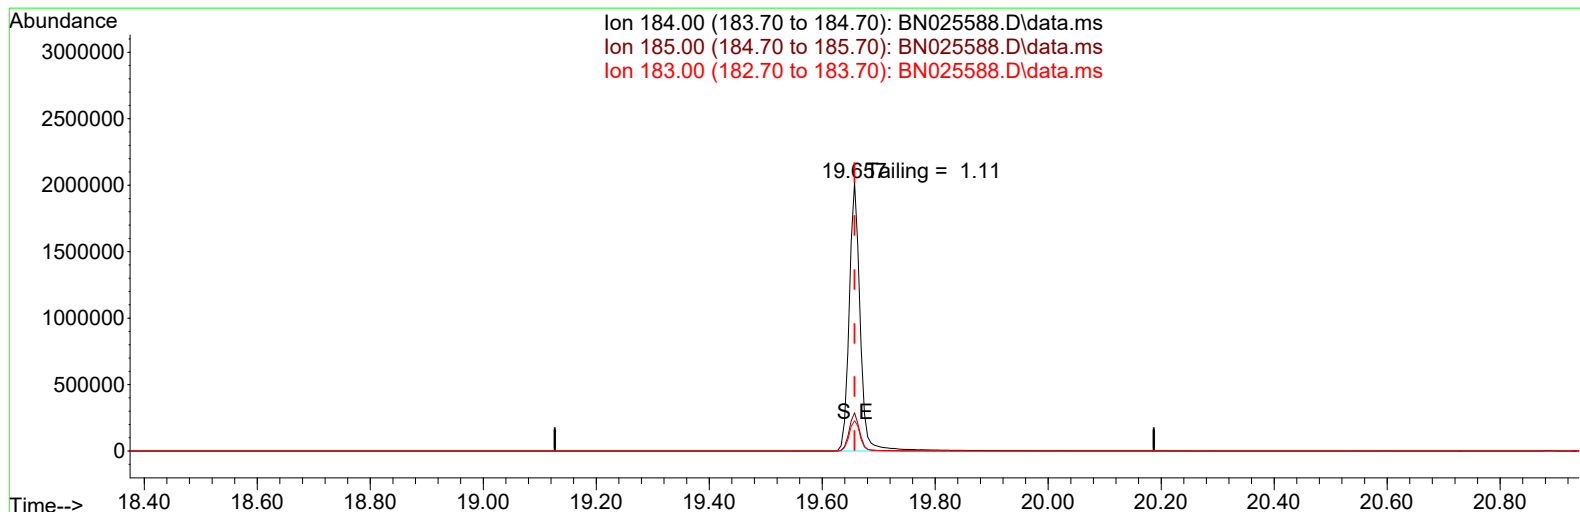

TIC: BN025588.D\data.ms

**(77) Benzidine**

19.657min ( 0.000) 0.00 ng

response 2749218

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.27  |
| 183.00 | 13.20  | 11.31  |
| 0.00   | 0.00   | 0.00   |