
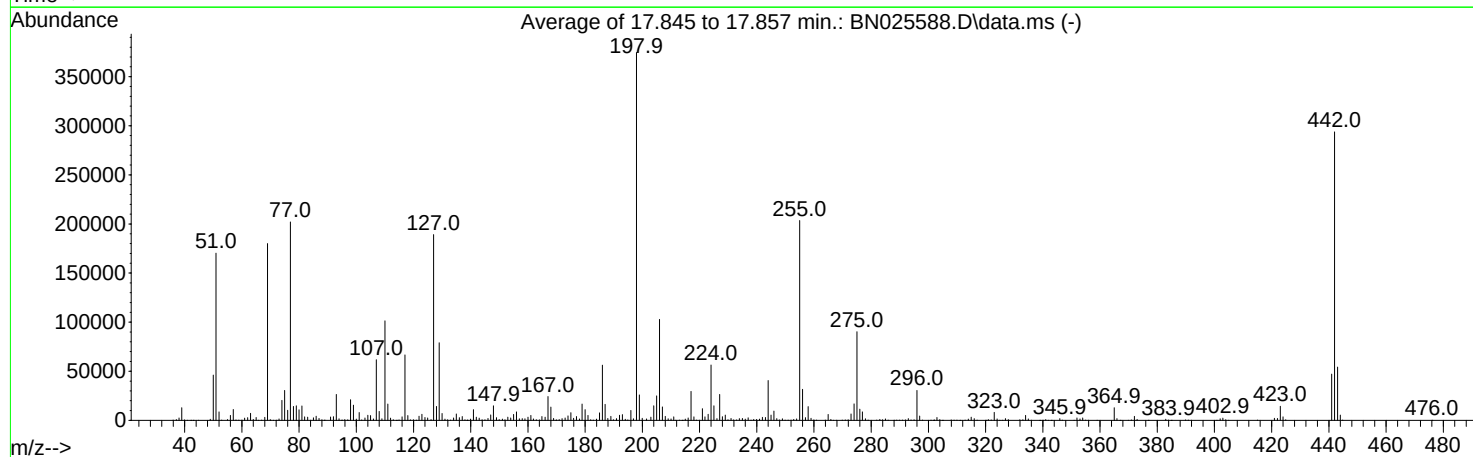


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052523\
 Data File : BN025588.D
 Acq On : 25 May 2023 14:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 00:32:23 2023

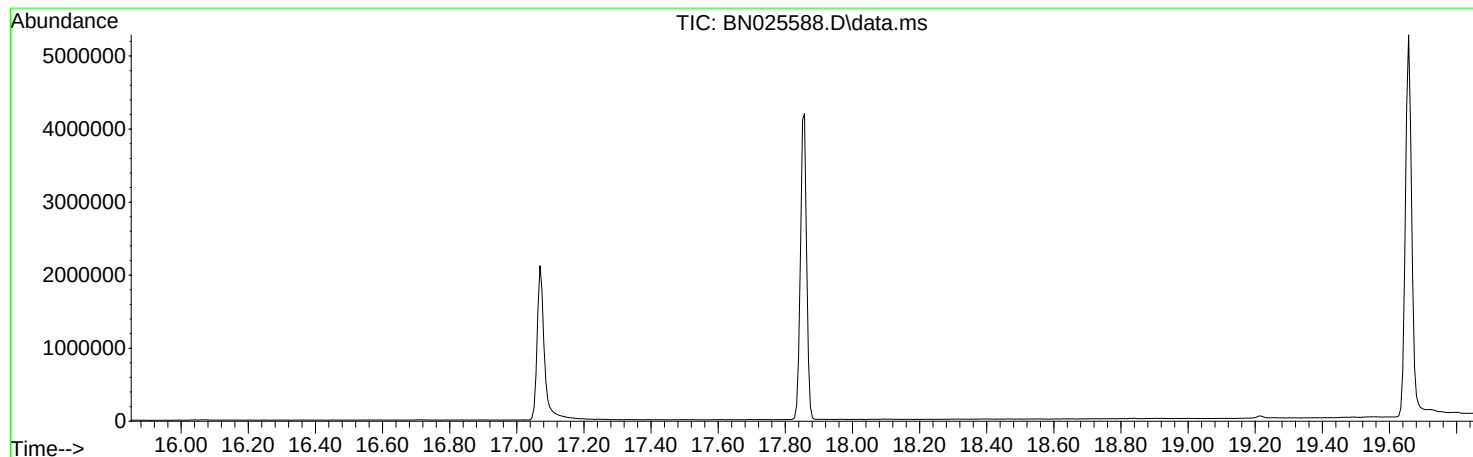

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	170247	PASS
68	69	0.00	2	1.7	3035	PASS
69	198	0.00	100	48.1	180032	PASS
70	69	0.00	2	0.4	631	PASS
127	198	10	80	50.5	189120	PASS
197	198	0.00	2	0.4	1664	PASS
198	198	100	100	100.0	374592	PASS
199	198	5	9	6.9	25976	PASS
275	198	10	60	24.1	90275	PASS
365	198	1	100	3.5	12937	PASS
441	198	0.01	100	12.6	47059	PASS
442	442	50	100	100.0	293803	PASS
443	442	15	24	18.5	54232	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/25/2023	BNA_N	<u>BN025588.D</u>
Compound Name	Response	Retention Time
DDT	501155	20.886
DDD	49823	20.498
DDE	0	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49823	550978	9.04

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052523\
 Data File : BN025588.D
 Acq On : 25 May 2023 14:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 26 06:42:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 26 06:42:42 2023
 Response via : Initial Calibration

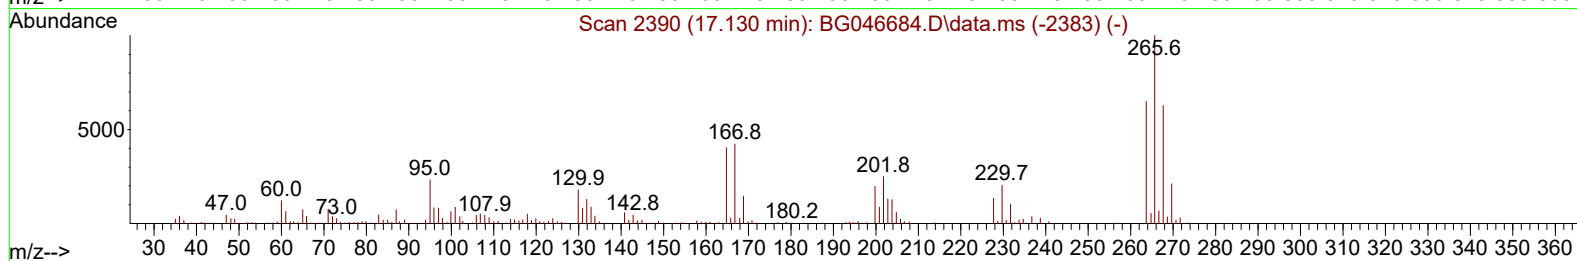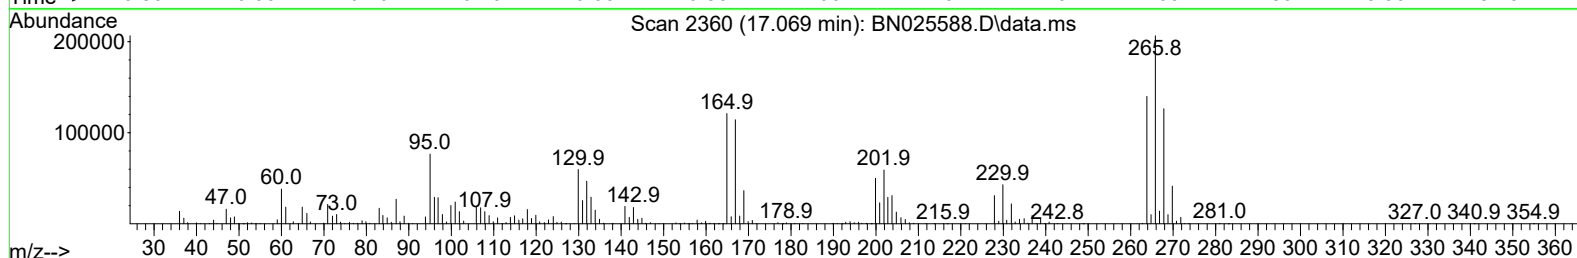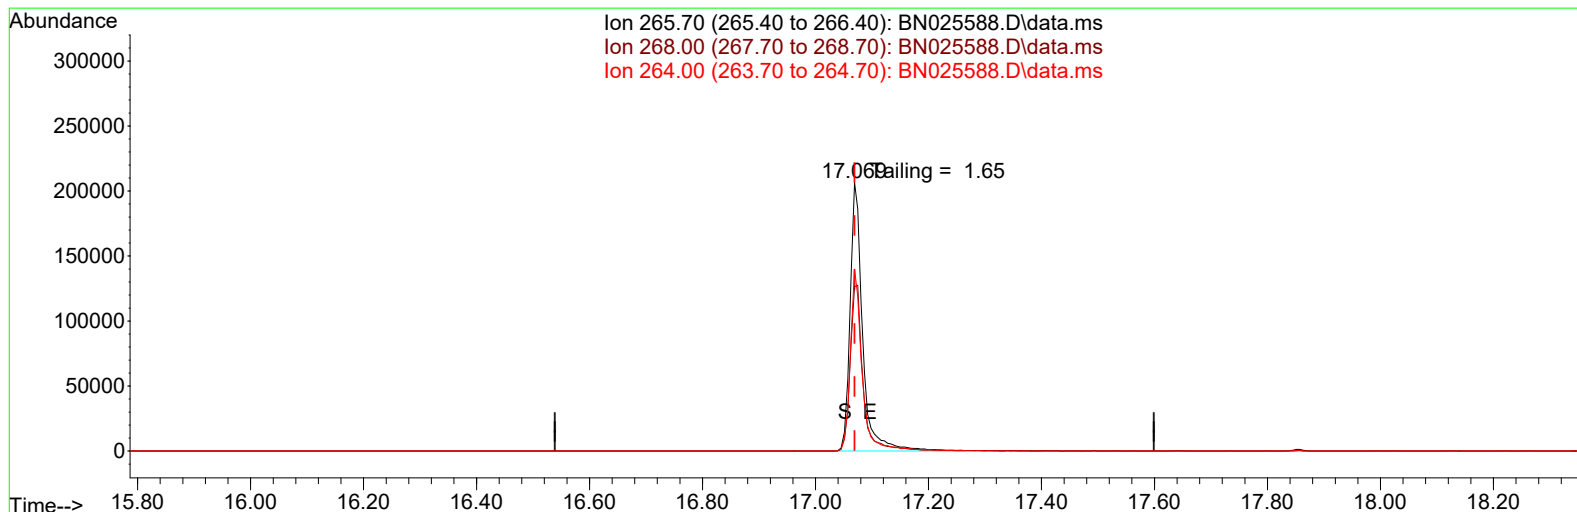

TIC: BN025588.D\data.ms

(70) Pentachlorophenol (C)

17.069min (0.000) 13726.37 ng




response 321332

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.24
264.00	61.60	67.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052523\
Data File : BN025588.D
Acq On : 25 May 2023 14:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 26 06:42:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 06:42:42 2023
Response via : Initial Calibration

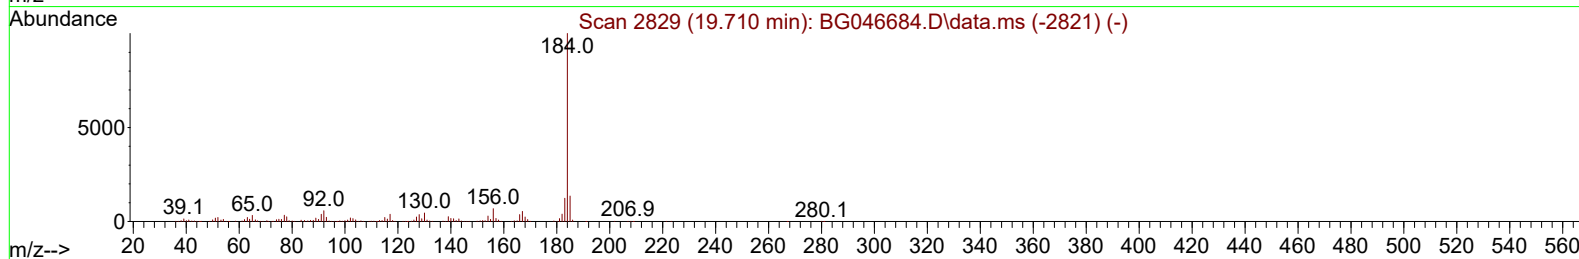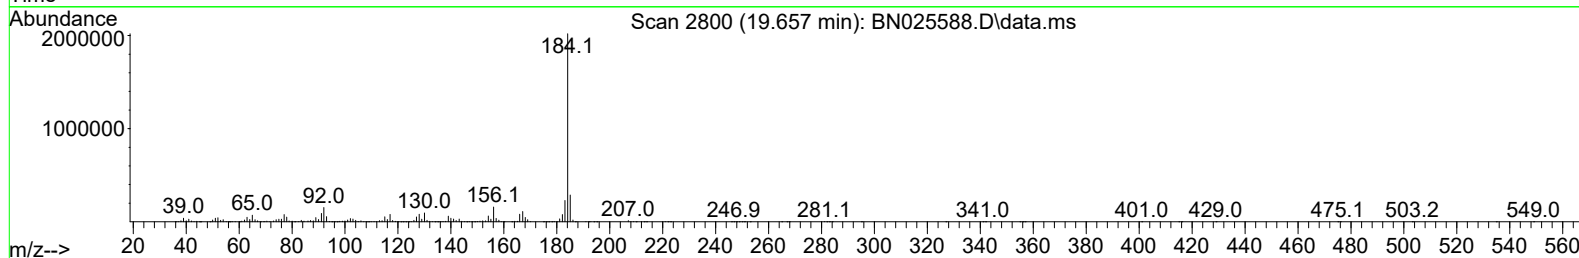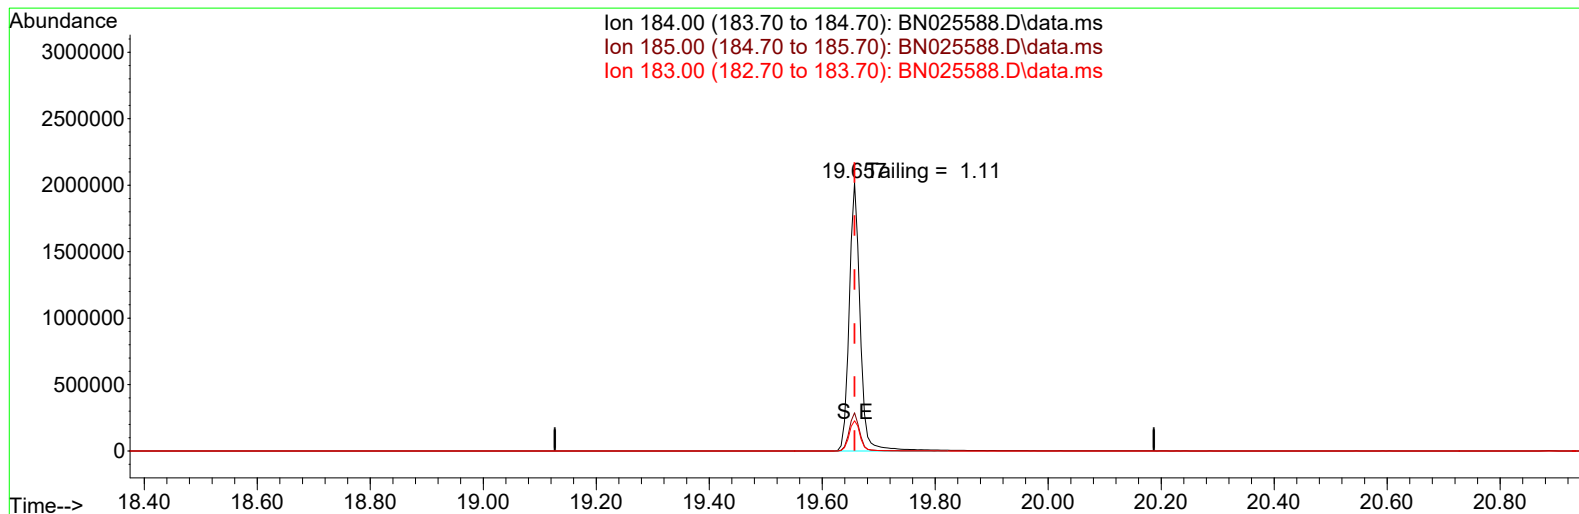

TIC: BN025588.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 2749218

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.27
183.00	13.20	11.31
0.00	0.00	0.00