


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052622\
 Data File : BN019982.D
 Acq On : 26 May 2022 20:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

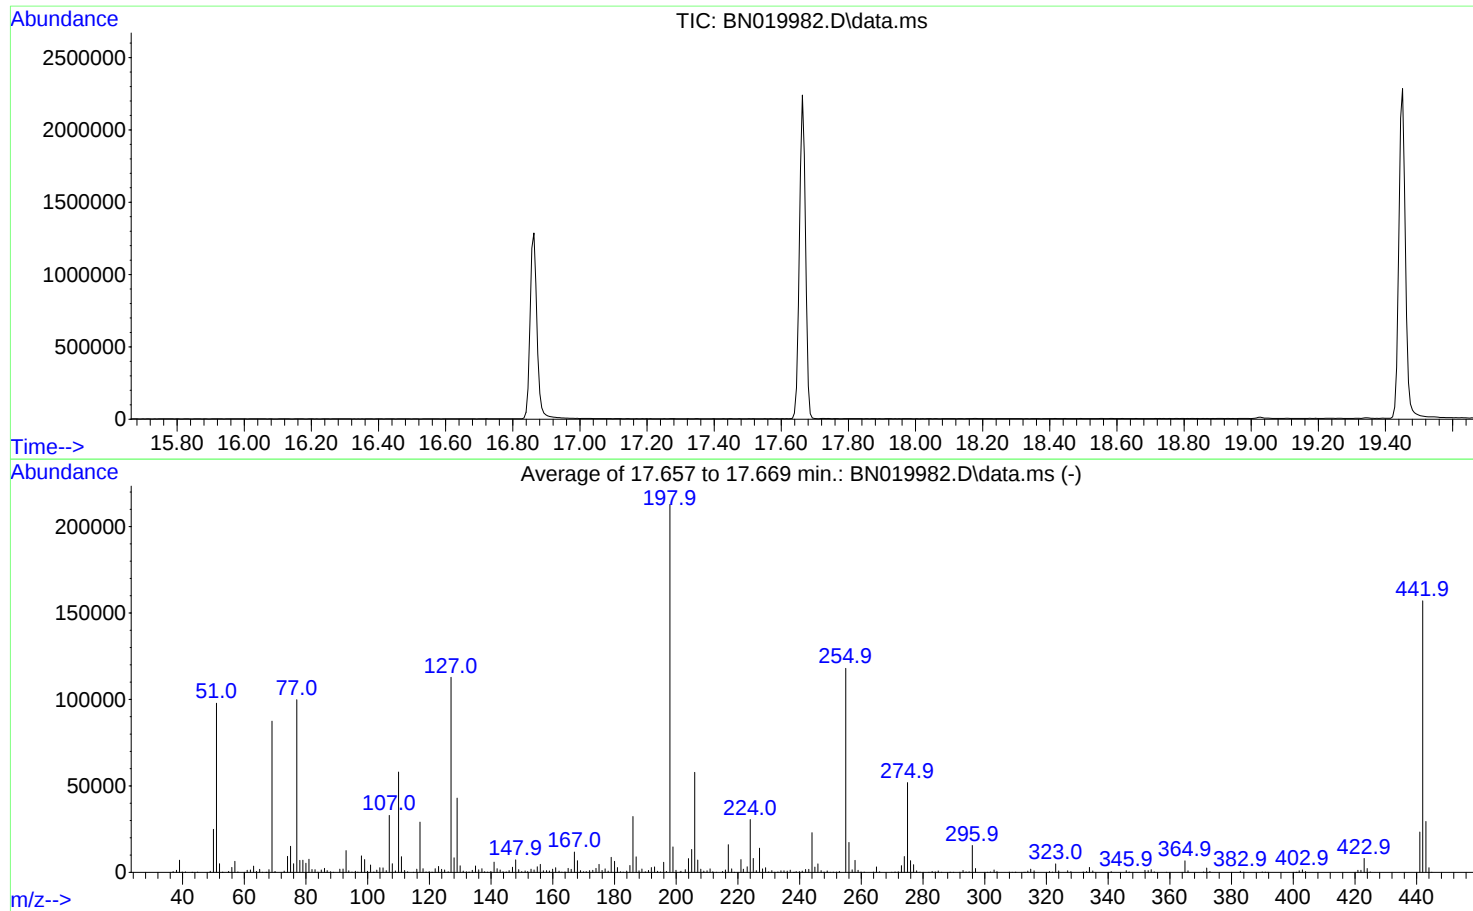




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	97853	PASS
68	69	0.00	2	1.8	1584	PASS
69	198	0.00	100	41.1	87429	PASS
70	69	0.00	2	0.7	569	PASS
127	198	10	80	53.0	112803	PASS
197	198	0.00	2	0.2	520	PASS
198	198	100	100	100.0	212757	PASS
199	198	5	9	6.9	14700	PASS
275	198	10	60	24.4	51904	PASS
365	198	1	100	3.1	6634	PASS
441	198	0.01	100	10.9	23282	PASS
442	442	50	100	100.0	157024	PASS
443	442	15	24	18.8	29459	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052622\
 Data File : BN019982.D
 Acq On : 26 May 2022 20:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 27 07:46:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

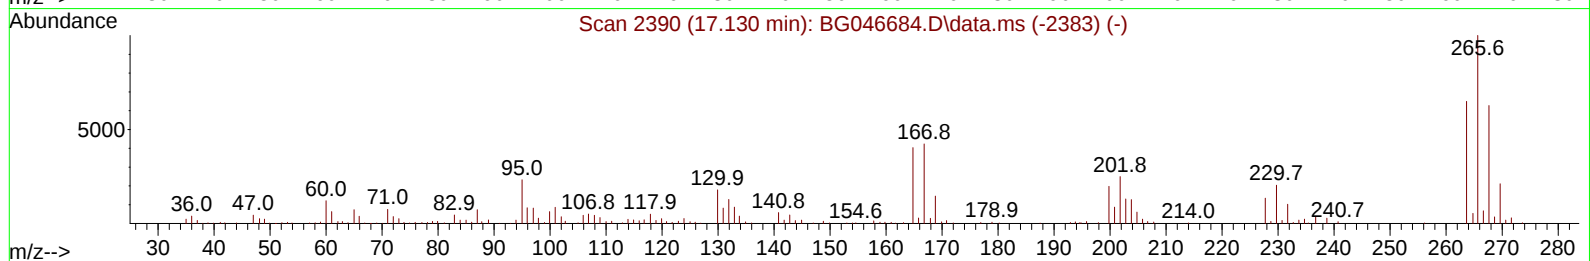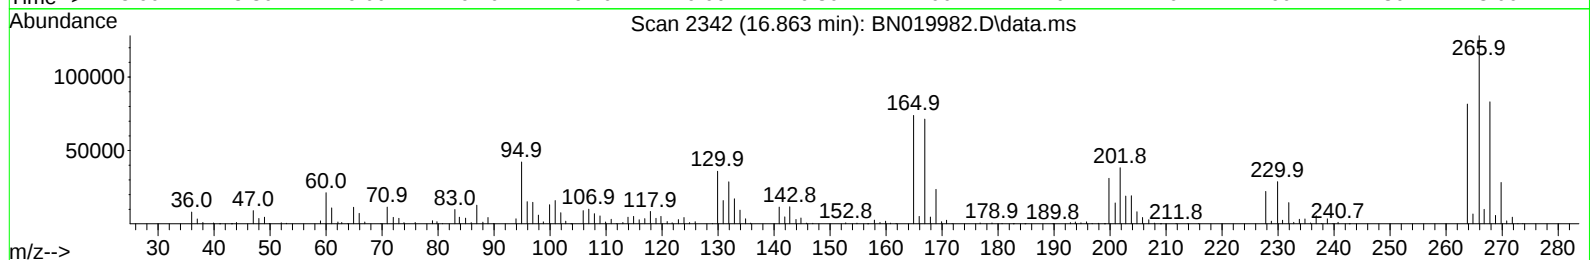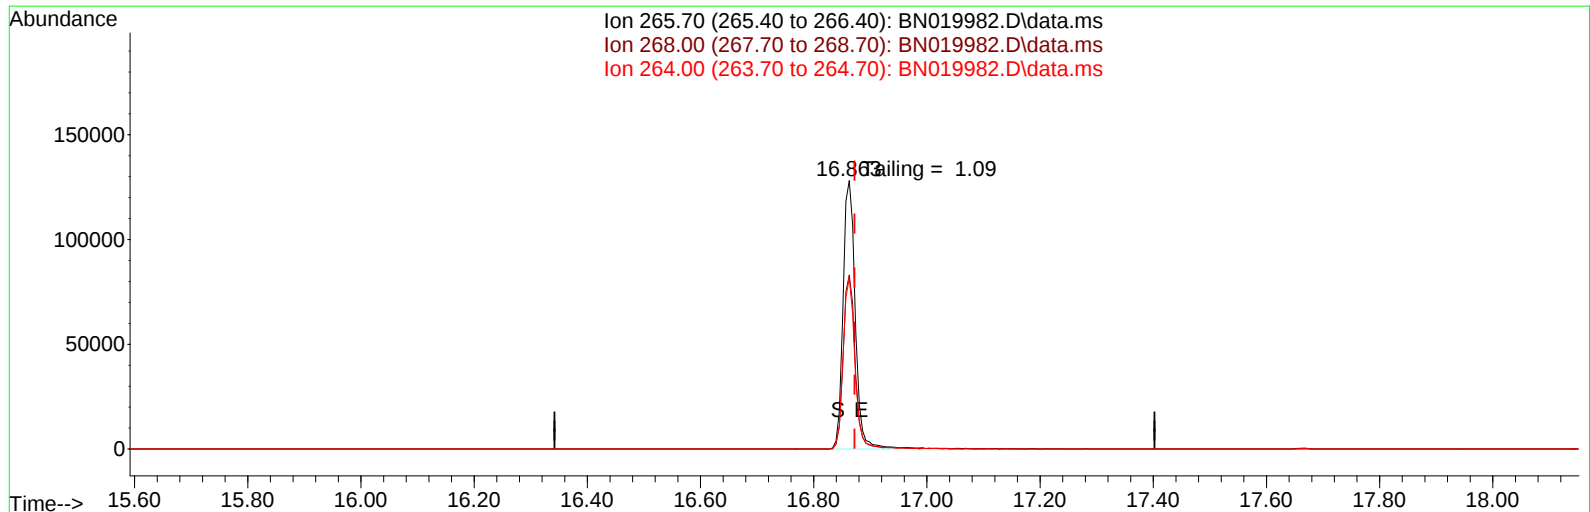

TIC: BN019982.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 19489.97 ng




response 192567

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.89
264.00	61.60	63.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052622\
Data File : BN019982.D
Acq On : 26 May 2022 20:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 27 07:46:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

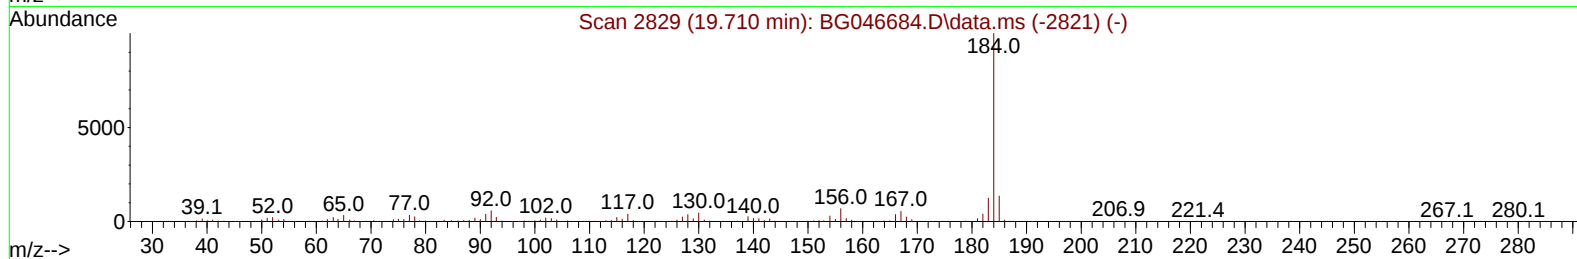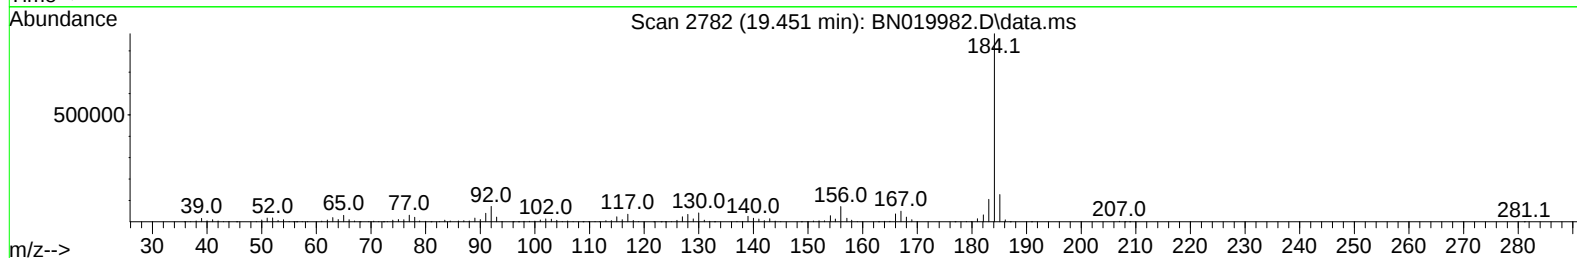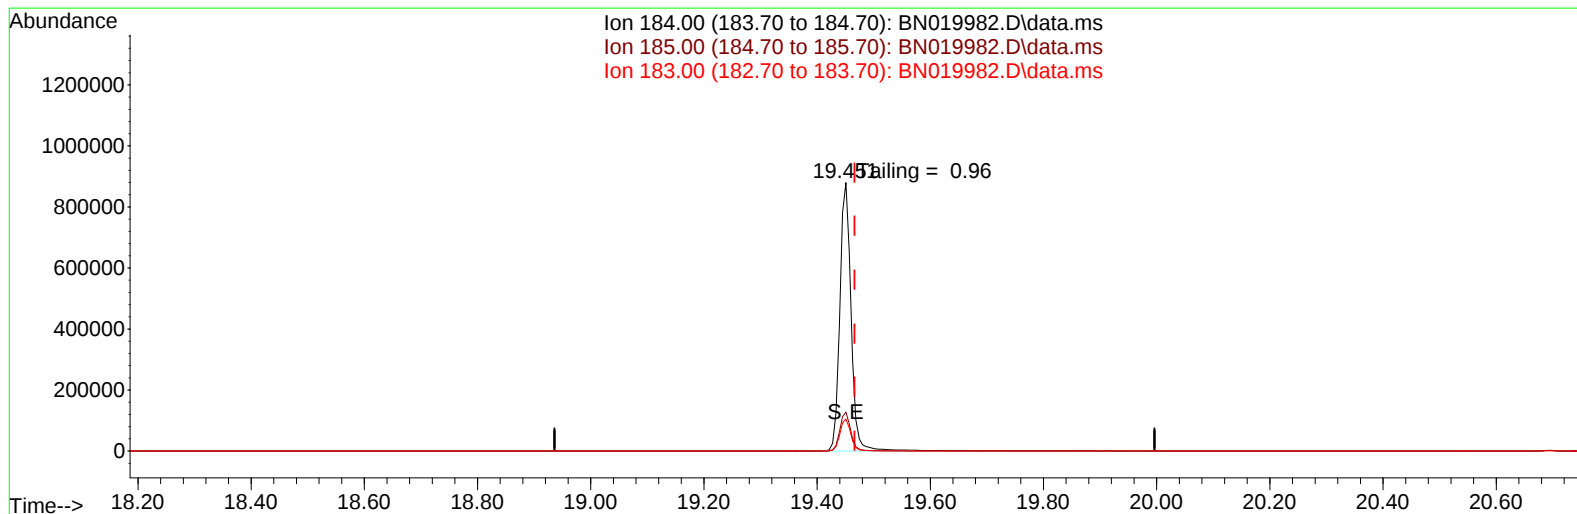

TIC: BN019982.D\data.ms

(77) Benzidine

19.451min (-0.015) 0.00 ng

response 1214955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.48
183.00	13.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2022	BNA_N	<u>BN019982.D</u>
Compound Name	Response	Retention Time
DDT	559895	20.692
DDD	87303	20.251
DDE	5256	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
92559	652454	14.19

Instrument :
BNA_N
ClientSampleId :
DFTPP